

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
 Data File : BG016446.D
 Acq On : 16 Apr 2015 6:36
 Operator : TP/IZ
 Sample : G1829-23
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TE-PMW-11S

Quant Time: Apr 16 07:30:41 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 16 04:13:21 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	83451	20.00	ng	0.00
21) Naphthalene-d8	10.45	136	368753	20.00	ng	0.00
38) Acenaphthene-d10	14.31	164	211861	20.00	ng	0.00
63) Phenanthrene-d10	17.05	188	460018	20.00	ng	0.00
75) Chrysene-d12	21.23	240	392196	20.00	ng	0.00
86) Perylene-d12	23.46	264	366931	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	332740	62.93	ng	0.00
7) Phenol-d6	6.86	99	298371	37.59	ng	0.00
23) Nitrobenzene-d5	8.82	82	523580	82.25	ng	0.00
41) 2,4,6-Tribromophenol	15.80	330	228161	159.24	ng	0.00
44) 2-Fluorobiphenyl	12.93	172	1151933	92.57	ng	0.00
78) Terphenyl-d14	19.68	244	1189550	70.99	ng	0.00
Target Compounds						
83) Bis(2-ethylhexyl)phthalate	21.15	149	39197	2.16	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
Data File : BG016446.D
Acq On : 16 Apr 2015 6:36
Operator : TP/IZ
Sample : G1829-23
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TE-PMW-11S

Quant Time: Apr 16 07:30:41 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 16 04:13:21 2015
Response via : Initial Calibration

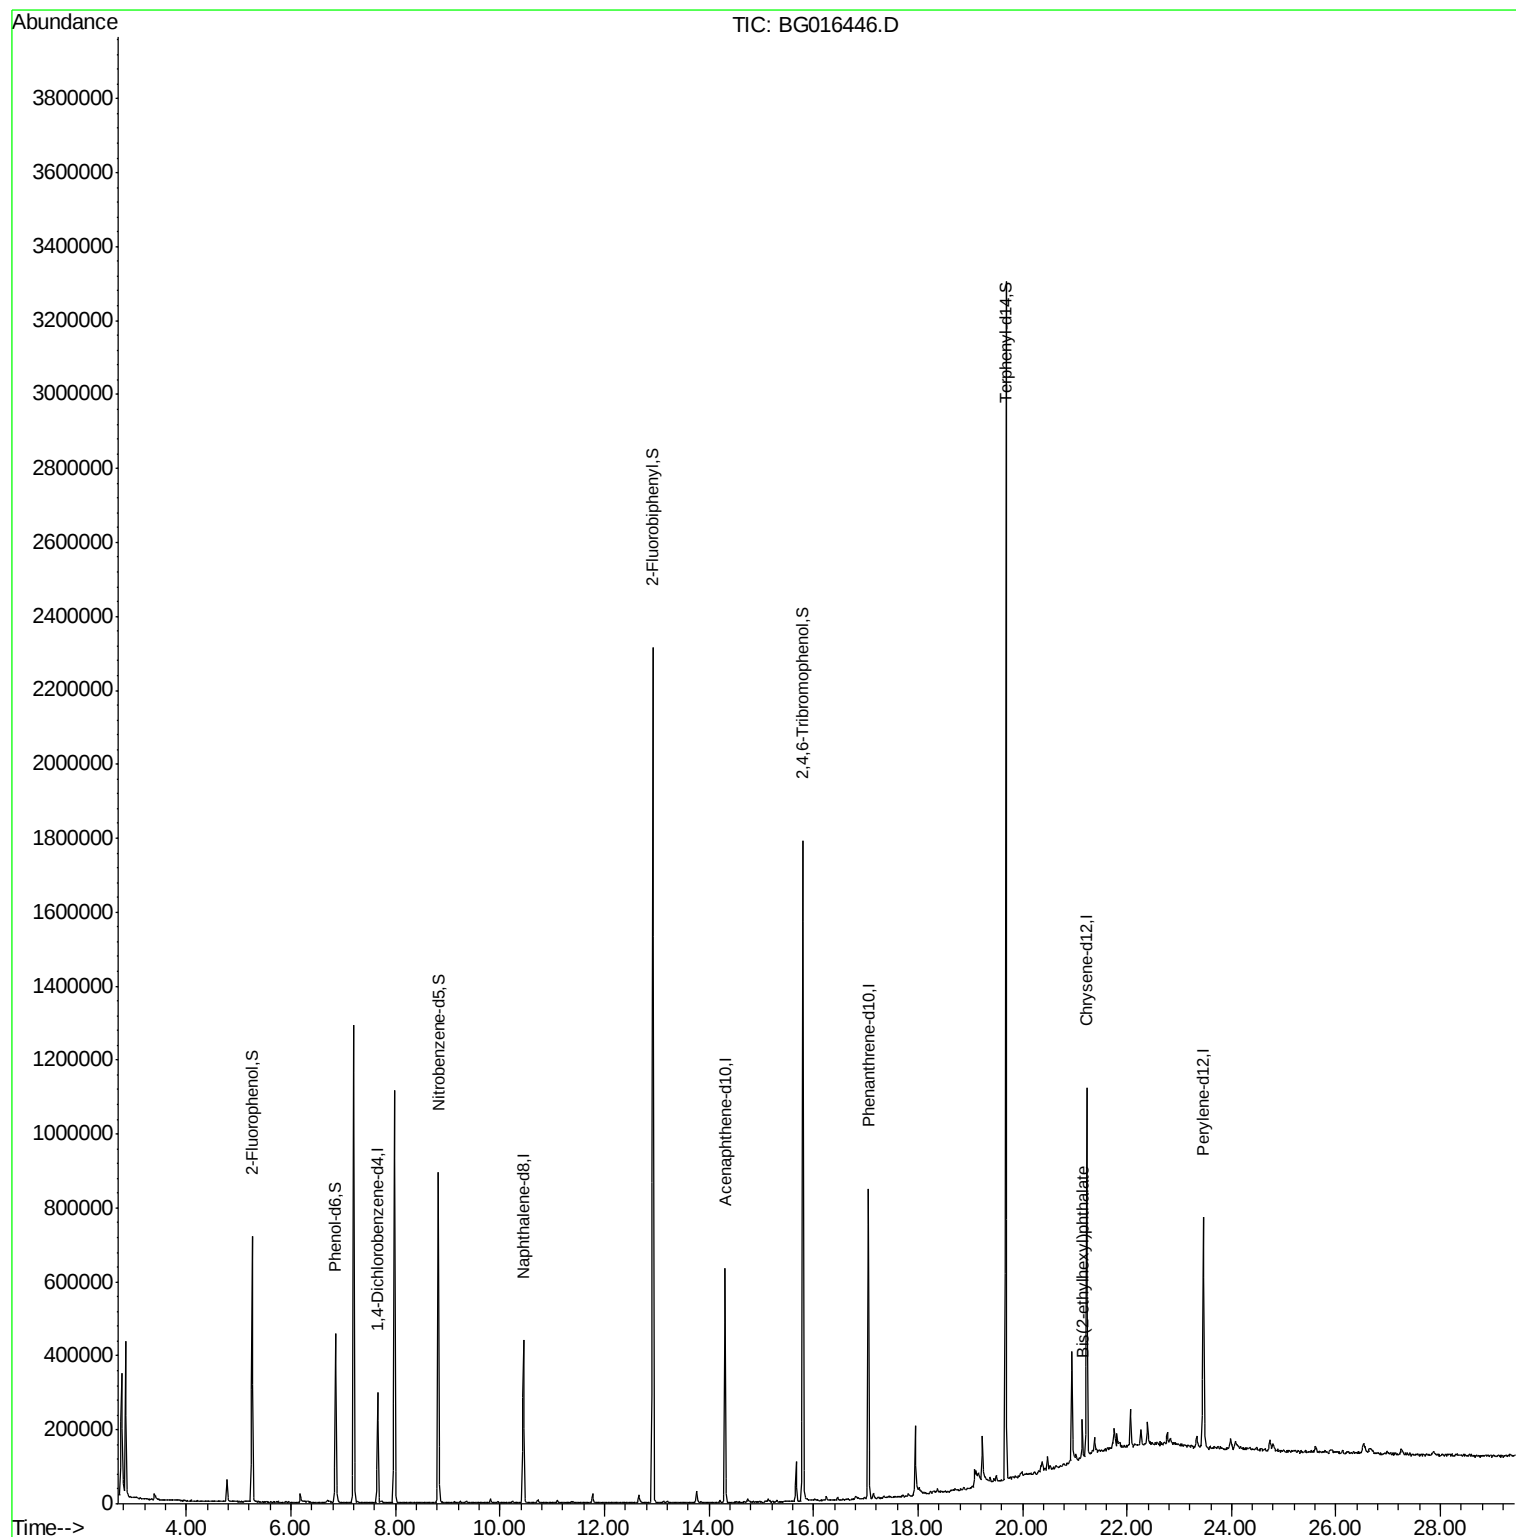

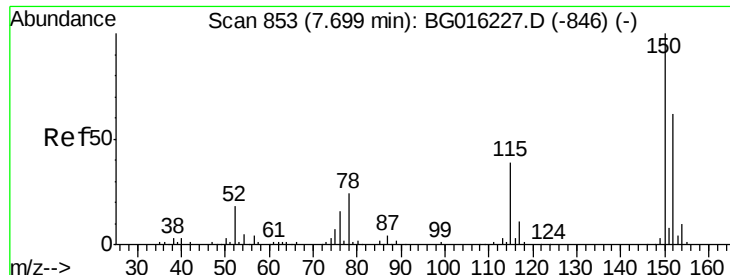


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.67 min Scan# 847
 Delta R.T. 0.00 min
 Lab File: BG016446.D
 Acq: 16 Apr 2015 6:36

Instrument :
 BNA_G
 ClientSampleId :
 TE-PMW-11S

Tgt Ion:152 Resp: 83451
 Ion Ratio Lower Upper
 152 100
 150 156.0 130.1 195.1
 115 55.1 50.5 75.7

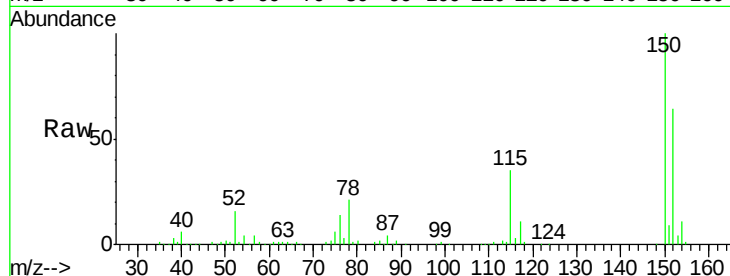


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

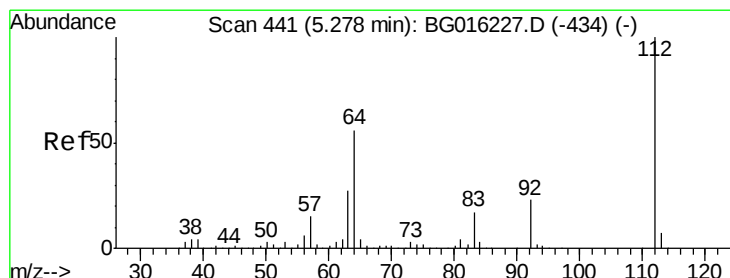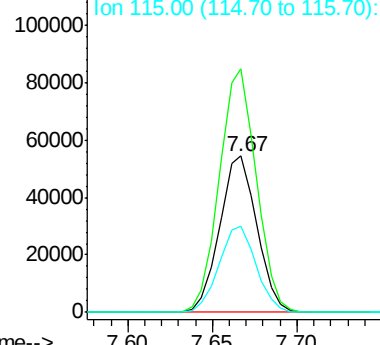



#5


2-Fluorophenol
 Concen: 62.93 ng
 RT: 5.26 min Scan# 437
 Delta R.T. 0.00 min
 Lab File: BG016446.D
 Acq: 16 Apr 2015 6:36

Tgt Ion:112 Resp: 332740
 Ion Ratio Lower Upper
 112 100
 64 50.3 44.5 66.7
 63 24.1 21.4 32.0

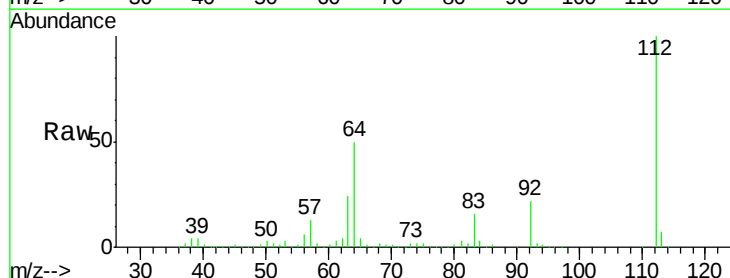

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

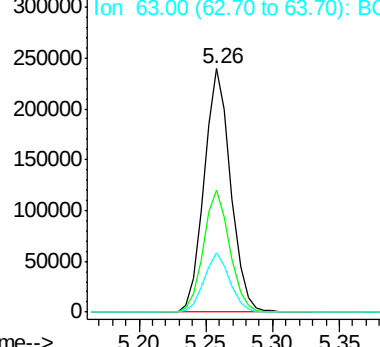

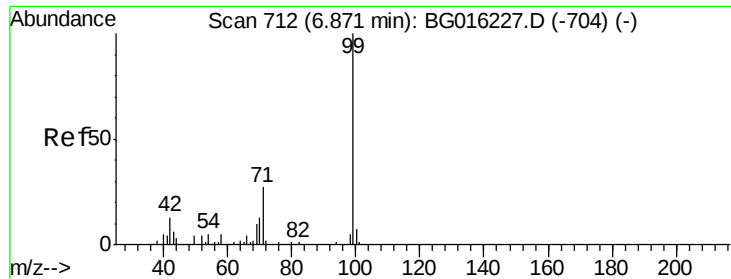

#7

Phenol-d6

Concen: 37.59 ng

RT: 6.86 min Scan# 709

Delta R.T. -0.00 min

Lab File: BG016446.D

Acq: 16 Apr 2015 6:36

Instrument :

BNA_G

ClientSampleId :

TE-PMW-11S


Tgt Ion: 99 Resp: 298371

Ion Ratio Lower Upper



99 100

42 11.0 10.0 15.0

71 24.3 21.5 32.3

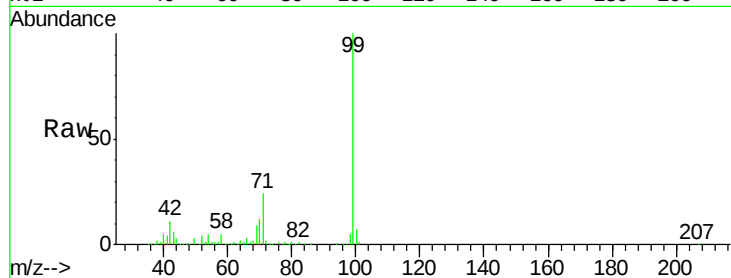

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

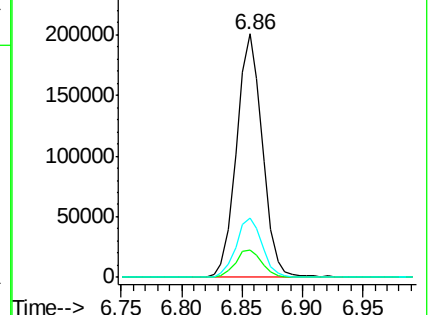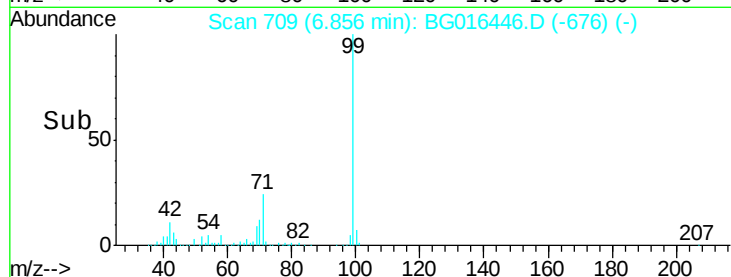

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.45 min Scan# 1321

Delta R.T. -0.00 min

Lab File: BG016446.D

Acq: 16 Apr 2015 6:36

Tgt Ion: 136 Resp: 368753


Ion Ratio Lower Upper

136 100



137 10.9 8.7 13.1


54 6.5 6.3 9.5

68 6.5 6.5 9.7#

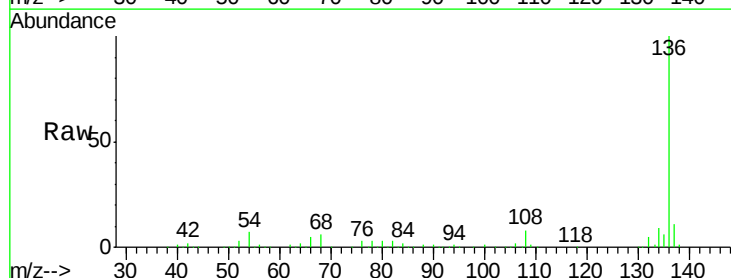

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



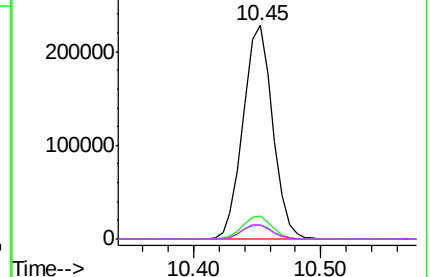
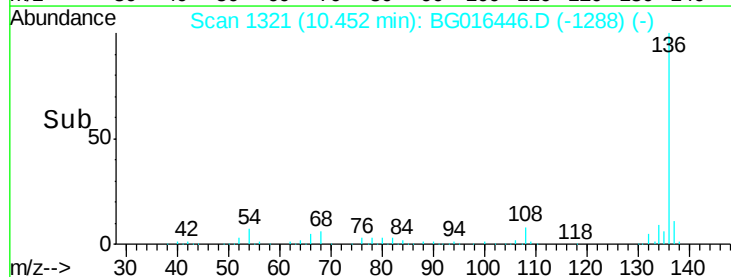


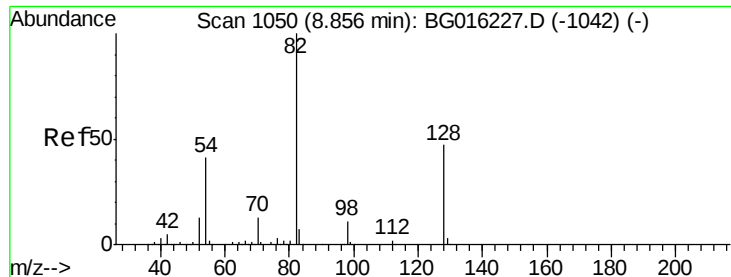

#23
 Nitrobenzene-d5
 Concen: 82.25 ng
 RT: 8.82 min Scan# 1044
 Delta R.T. -0.00 min
 Lab File: BG016446.D
 Acq: 16 Apr 2015 6:36




Instrument :
 BNA_G
 ClientSampleId :
 TE-PMW-11S


Tgt Ion: 82 Resp: 523580
 Ion Ratio Lower Upper
 82 100
 128 52.7 37.8 56.8
 54 39.5 32.6 49.0

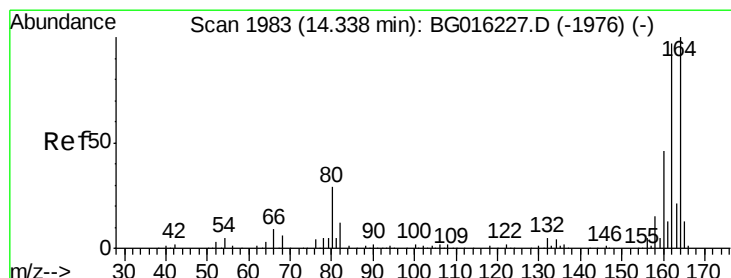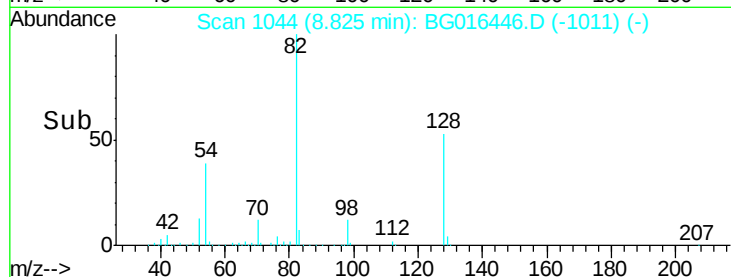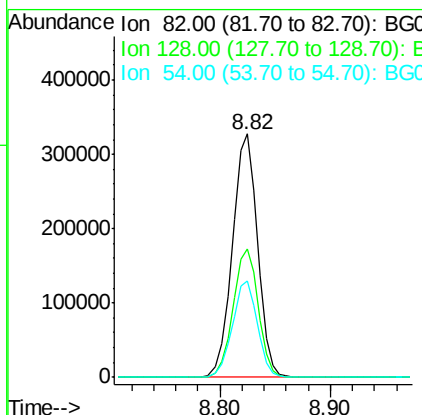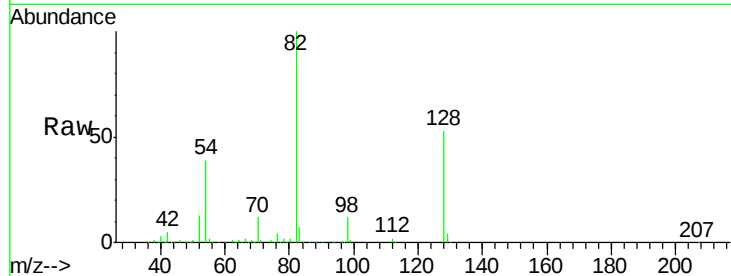

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.31 min Scan# 1977
 Delta R.T. -0.00 min
 Lab File: BG016446.D
 Acq: 16 Apr 2015 6:36

Tgt Ion: 164 Resp: 211861
 Ion Ratio Lower Upper
 164 100
 162 98.5 77.3 115.9
 160 44.2 36.7 55.1

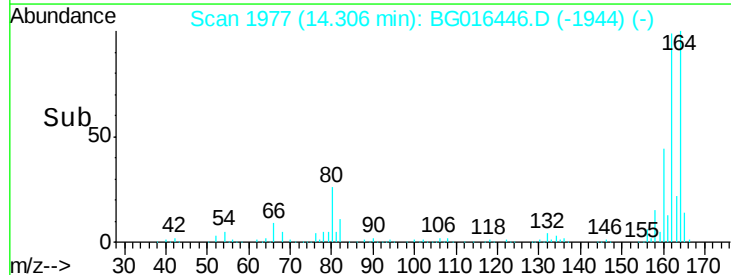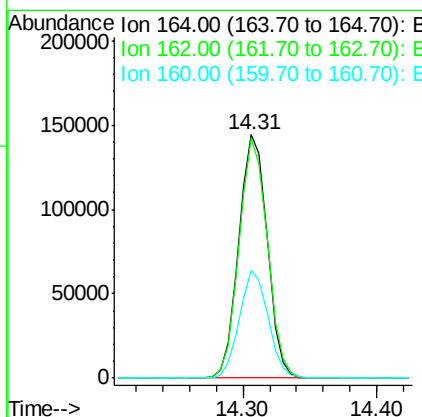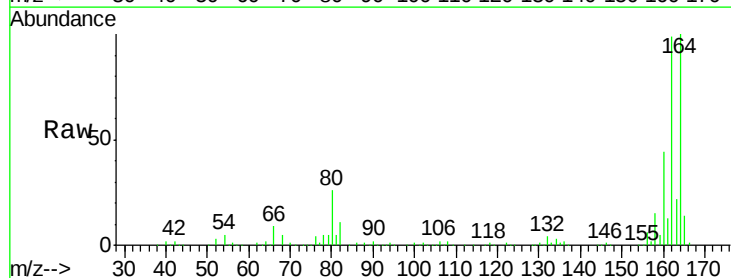







#41
 2,4,6-Tribromophenol
 Concen: 159.24 ng
 RT: 15.80 min Scan# 2232
 Delta R.T. 0.00 min
 Lab File: BG016446.D
 Acq: 16 Apr 2015 6:36

Instrument :
 BNA_G
 ClientSampleId :
 TE-PMW-11S

Tgt Ion:330 Resp: 228161
 Ion Ratio Lower Upper
 330 100
 332 95.6 75.8 113.6
 141 56.9 46.6 69.8

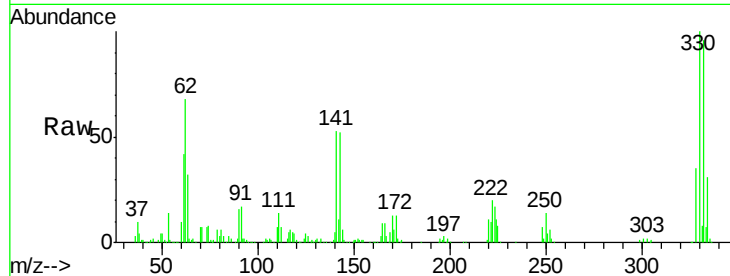


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

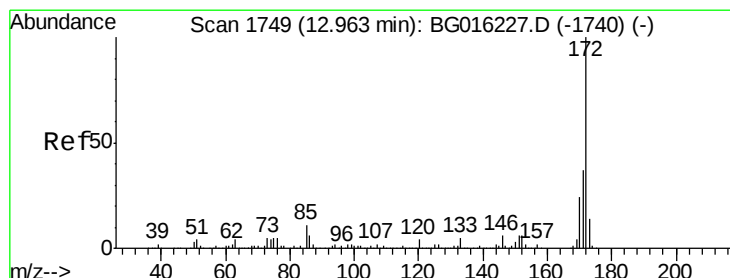
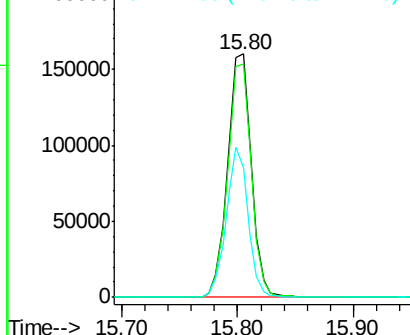



#44
 2-Fluorobiphenyl
 Concen: 92.57 ng
 RT: 12.93 min Scan# 1743
 Delta R.T. 0.00 min
 Lab File: BG016446.D
 Acq: 16 Apr 2015 6:36

Tgt Ion:172 Resp: 1151933
 Ion Ratio Lower Upper
 172 100
 171 37.4 29.6 44.4
 170 24.9 19.4 29.2

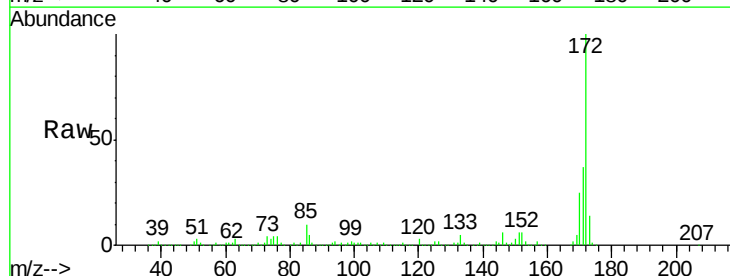

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

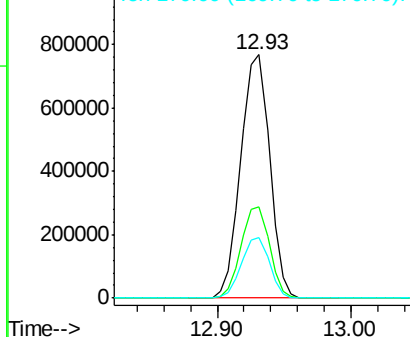







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.05 min Scan# 2444
Delta R.T. -0.00 min
Lab File: BG016446.D
Acq: 16 Apr 2015 6:36

Instrument :
BNA_G
ClientSampleId :
TE-PMW-11S

Tgt Ion:188 Resp: 460018
Ion Ratio Lower Upper
188 100
94 14.4 12.2 18.4
80 14.1 12.8 19.2

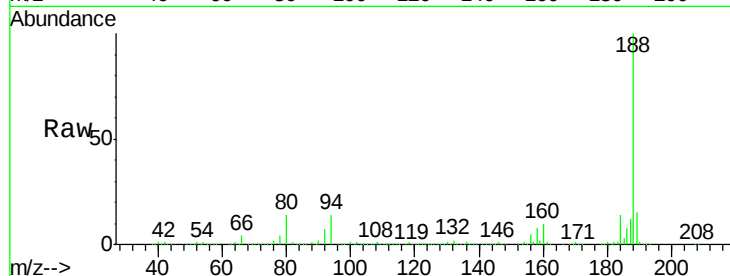


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

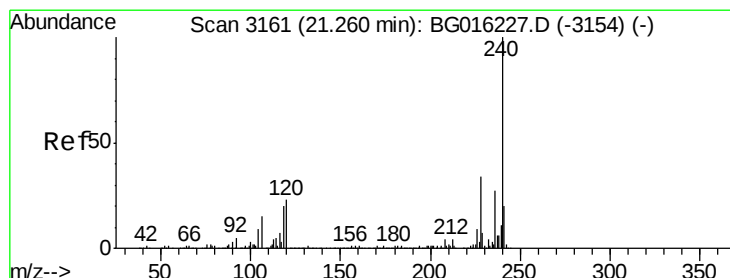
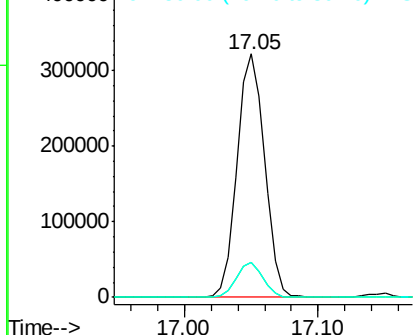



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.23 min Scan# 3155
Delta R.T. -0.00 min
Lab File: BG016446.D
Acq: 16 Apr 2015 6:36

Tgt Ion:240 Resp: 392196
Ion Ratio Lower Upper
240 100
120 21.7 18.6 28.0
236 26.1 21.7 32.5

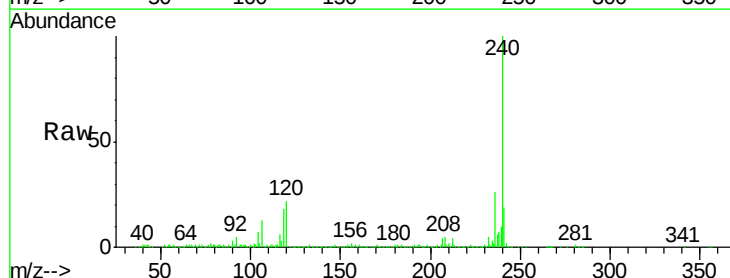

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

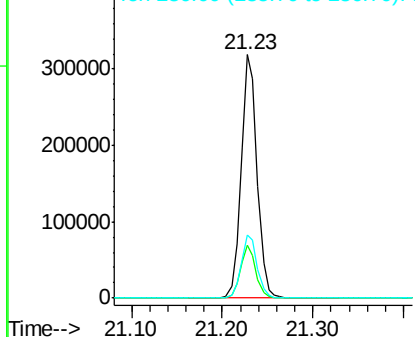



#78

Terphenyl-d14

Concen: 70.99 ng

RT: 19.68 min Scan# 2892

Delta R.T. 0.00 min

Lab File: BG016446.D

Acq: 16 Apr 2015 6:36

Instrument :

BNA_G

ClientSampleId :

TE-PMW-11S


Tgt Ion:244 Resp: 1189550

Ion Ratio Lower Upper

244 100

212 8.7 6.6 9.8




122 22.0 19.1 28.7

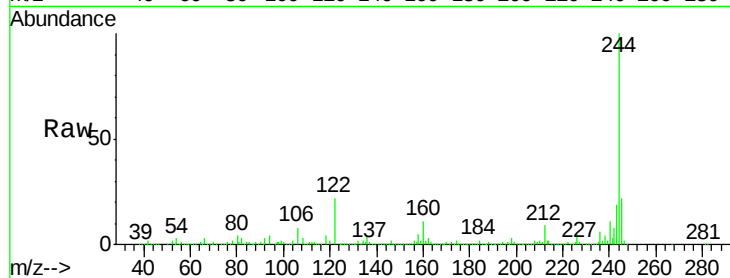

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

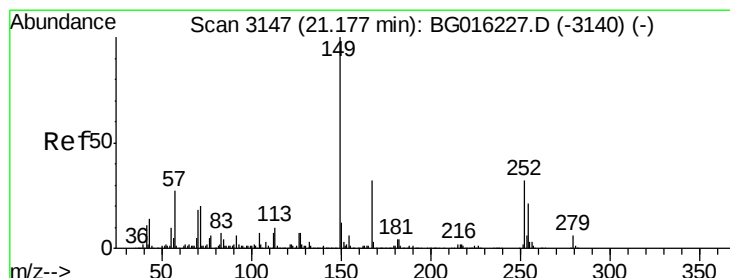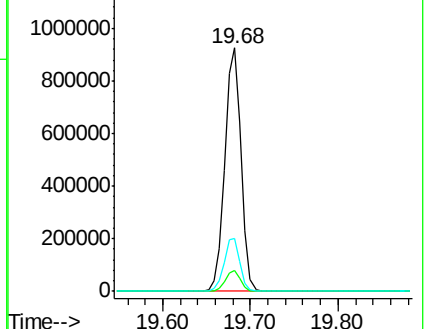

#83

Bis(2-ethylhexyl)phthalate

Concen: 2.16 ng

RT: 21.15 min Scan# 3141

Delta R.T. -0.00 min

Lab File: BG016446.D

Acq: 16 Apr 2015 6:36


Tgt Ion:149 Resp: 39197

Ion Ratio Lower Upper

149 100

167 30.7 25.8 38.6



279 6.6 4.7 7.1

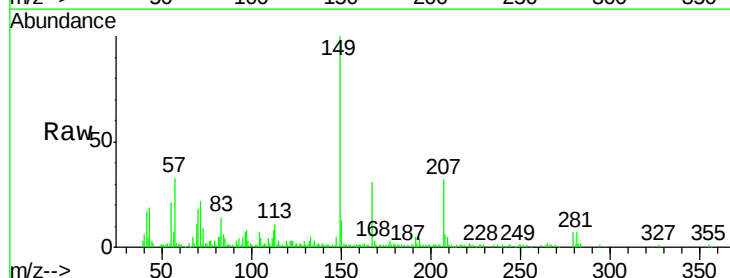


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

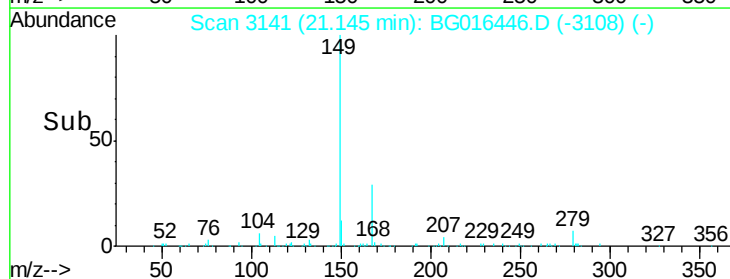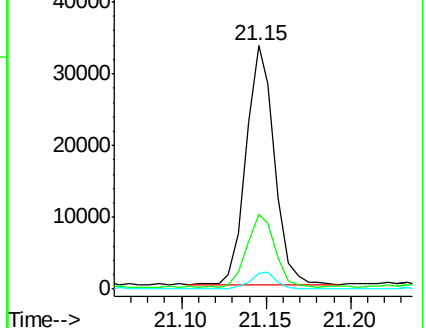

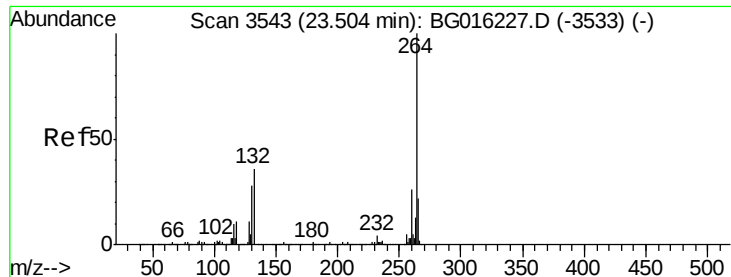

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.46 min Scan# 3535
Delta R.T. -0.00 min
Lab File: BG016446.D
Acq: 16 Apr 2015 6:36

Instrument :
BNA_G
ClientSampleId :
TE-PMW-11S

Tgt Ion: 264 Resp: 366931
Ion Ratio Lower Upper
264 100
260 23.3 20.4 30.6
265 21.6 17.2 25.8

