

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
 Data File : BG016426.D
 Acq On : 15 Apr 2015 17:00
 Operator : TP/IZ
 Sample : G1849-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TWP-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.758	7	12	22	rBV	380170	576177	20.44%	3.340%
2	2.840	22	26	35	rVB	354301	439916	15.61%	2.550%
3	4.180	248	254	266	rVB	242475	328501	11.65%	1.904%
4	4.779	350	356	365	rBV	635960	822411	29.18%	4.767%
5	5.255	431	437	445	rVB	260630	369294	13.10%	2.141%
6	5.860	534	540	546	rVB	88430	126546	4.49%	0.734%
7	6.847	702	708	718	rBV	166978	268964	9.54%	1.559%
8	7.199	761	768	776	rBV	493432	759562	26.95%	4.403%
9	7.664	841	847	855	rVB	280541	434474	15.41%	2.518%
10	7.987	894	902	910	rVB	571908	919531	32.62%	5.330%
11	8.821	1037	1044	1054	rBV	482831	766023	27.18%	4.440%
12	10.449	1314	1321	1328	rBV	407041	677130	24.02%	3.925%
13	11.777	1538	1547	1554	rBV	20354	33640	1.19%	0.195%
14	12.928	1734	1743	1753	rBV	1360615	1912385	67.85%	11.085%
15	13.768	1879	1886	1894	rBV	43578	61236	2.17%	0.355%
16	14.309	1971	1978	1987	rBV2	680136	979938	34.77%	5.680%
17	15.666	2203	2209	2216	rBV	74356	103709	3.68%	0.601%
18	15.795	2225	2231	2240	rBV	660351	926759	32.88%	5.372%
19	17.053	2438	2445	2454	rBV2	882092	1262538	44.79%	7.318%
20	17.946	2592	2597	2606	rBV4	30335	45710	1.62%	0.265%
21	19.679	2886	2892	2900	rBV	2376341	2818648	100.00%	16.338%
22	20.942	3103	3107	3114	rBV	40577	62143	2.20%	0.360%
23	21.230	3150	3156	3164	rBV	1078887	1301356	46.17%	7.543%
24	23.463	3528	3536	3549	rBV2	666170	1255100	44.53%	7.275%


Sum of corrected areas: 17251691

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
Data File : BG016426.D
Acq On : 15 Apr 2015 17:00
Operator : TP/IZ
Sample : G1849-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TWP-01

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

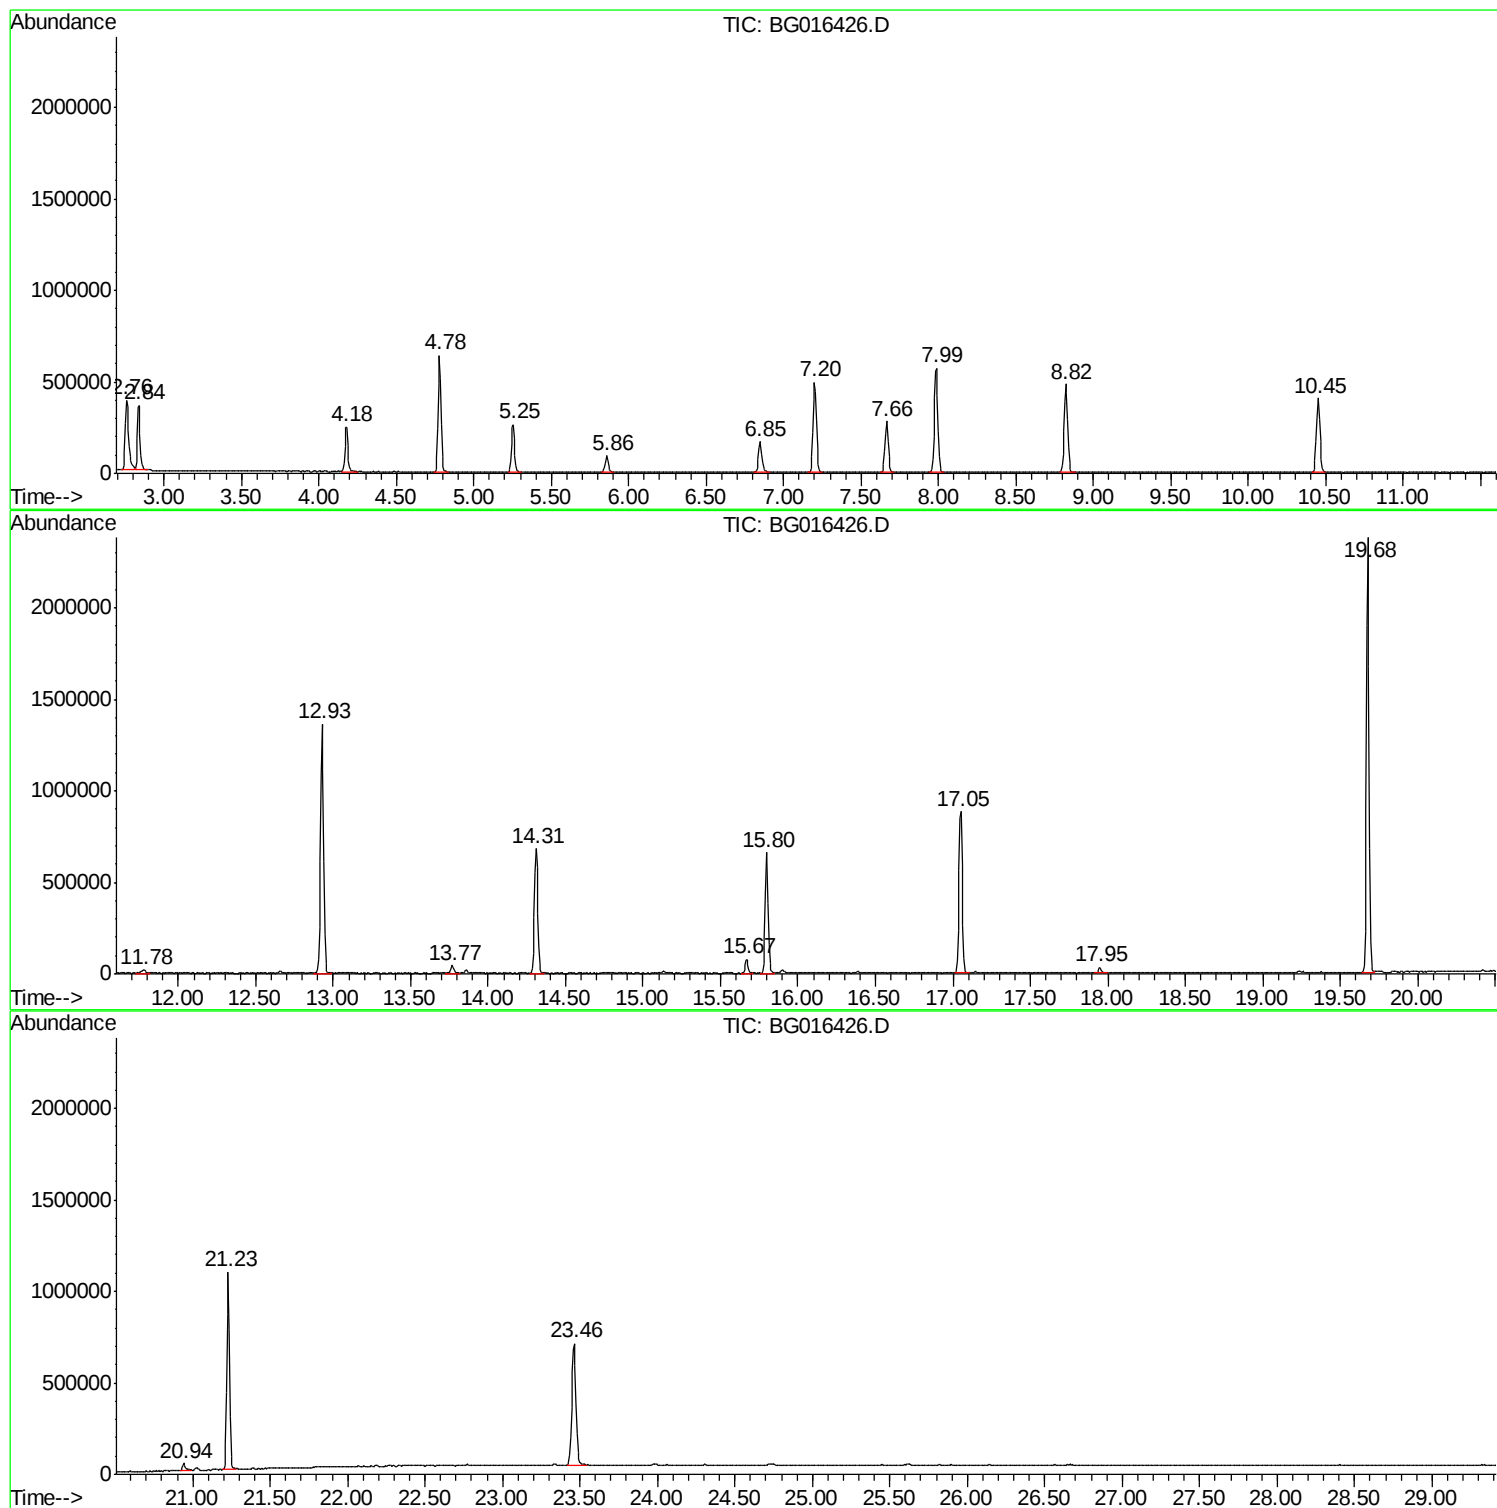

DbaaaPathh::ZZ\NRPBHHM1BBAAGGDBAA\BB0015555\
 DbaaaFile::BB0060206DD
 Aeqq00n ::155Apr20055 177000
 Opeaaor ::TPIIZ
 Sample ::G68809001
 Misc ::
 AASSVaal ::300 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 TWP-01

QqaantMebbdd::ZZ\NRPBHHM1BBAAGGMEH#00S8270BB000065MM
 QqaantTitle ::ASBPBBAASSANDBBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DATAABASSEN055002LL
 TICInteggaionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
