


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041515\
 Data File : BG016414.D
 Acq On : 15 Apr 2015 10:03
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 14 14:00:56 2015

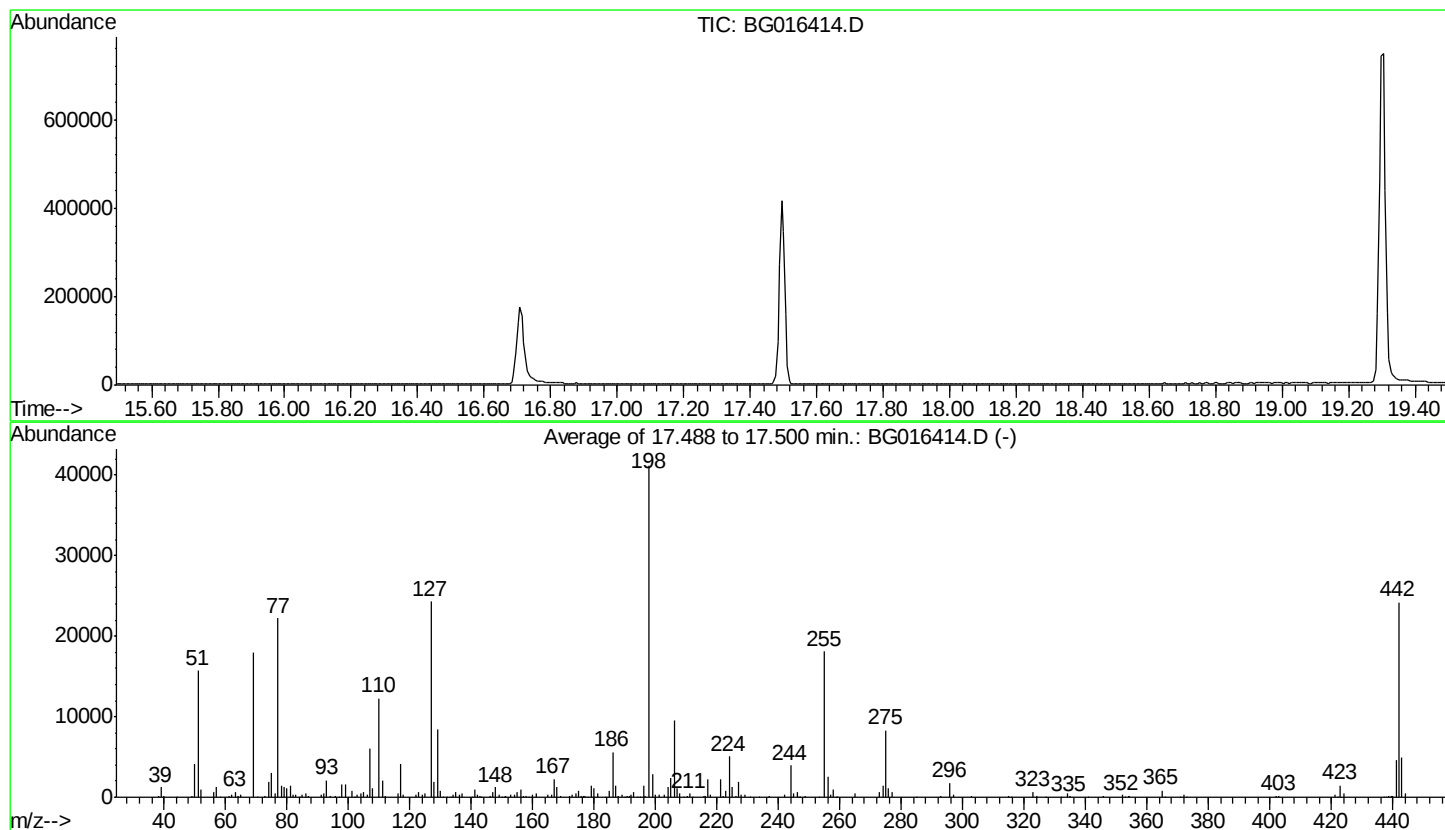

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	15728	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.7	18002	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	59.0	24288	PASS
197	198	0.00	2	0.4	174	PASS
198	198	100	100	100.0	41186	PASS
199	198	5	9	6.8	2794	PASS
275	198	10	60	20.2	8309	PASS
365	198	1	100	2.0	804	PASS
441	442	0.01	24	18.9	4566	PASS
442	198	50	100	58.7	24190	PASS
443	442	15	24	20.6	4981	PASS