
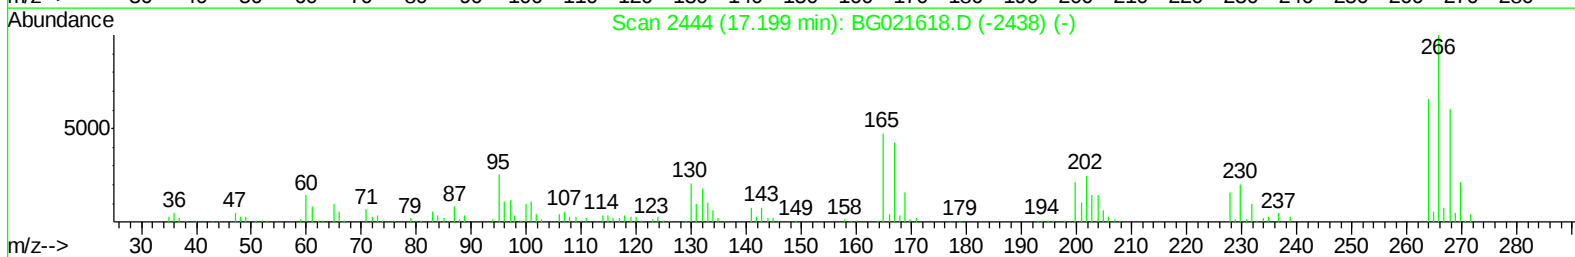
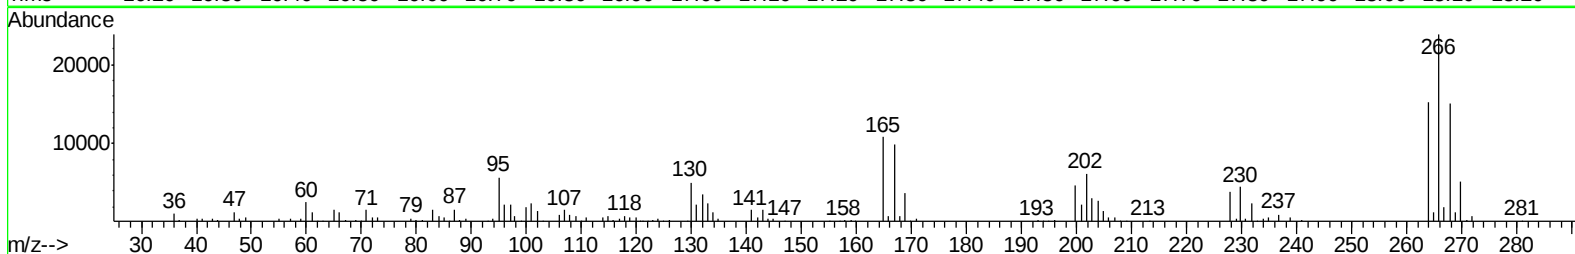


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041516\
Data File : BG021704.D
Acq On : 16 Apr 2016 6:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 06:50:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

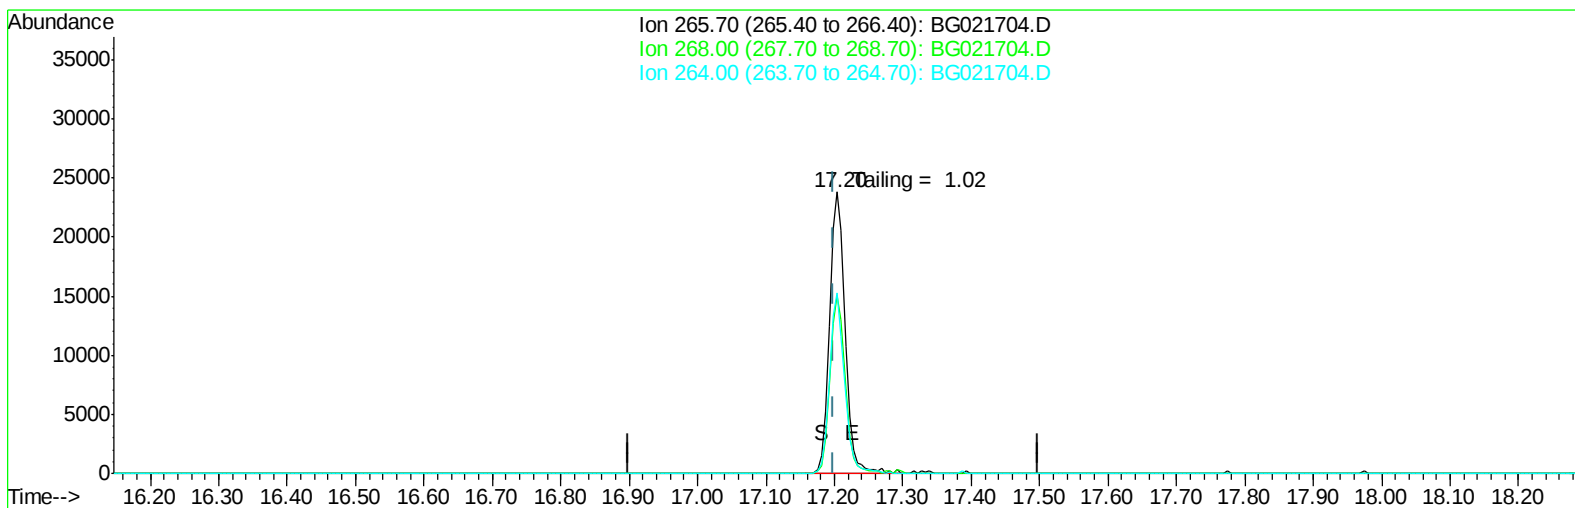

TIC: BG021704.D

(69) Pentachlorophenol (C)




17.204min (+0.005) 0.00ng

response 37246

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	63.13
264.00	67.20	63.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041516\
Data File : BG021704.D
Acq On : 16 Apr 2016 6:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 06:50:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 15:48:13 2016
Response via : Initial Calibration

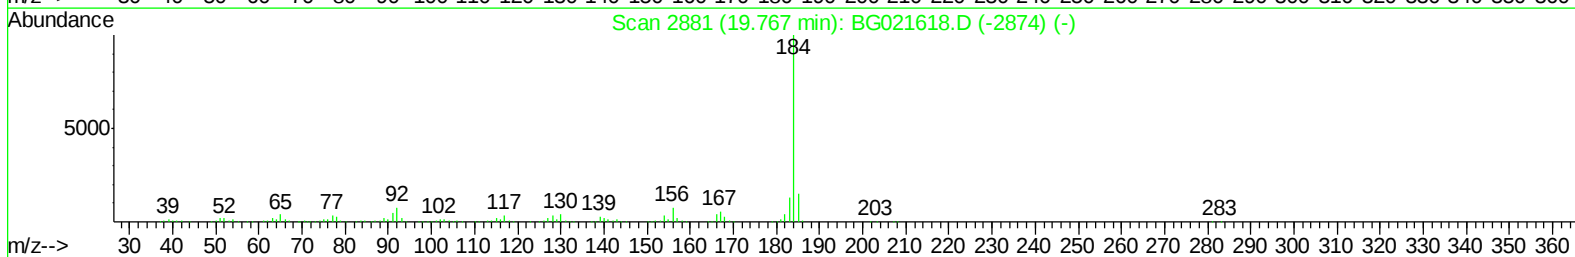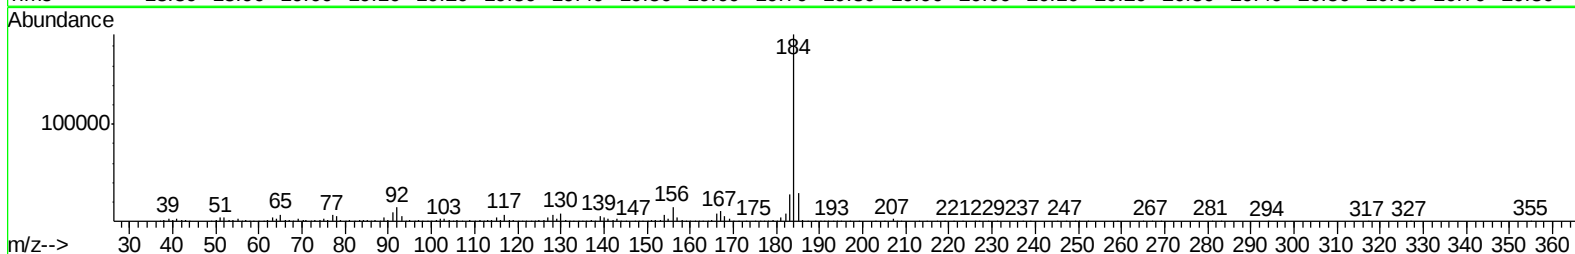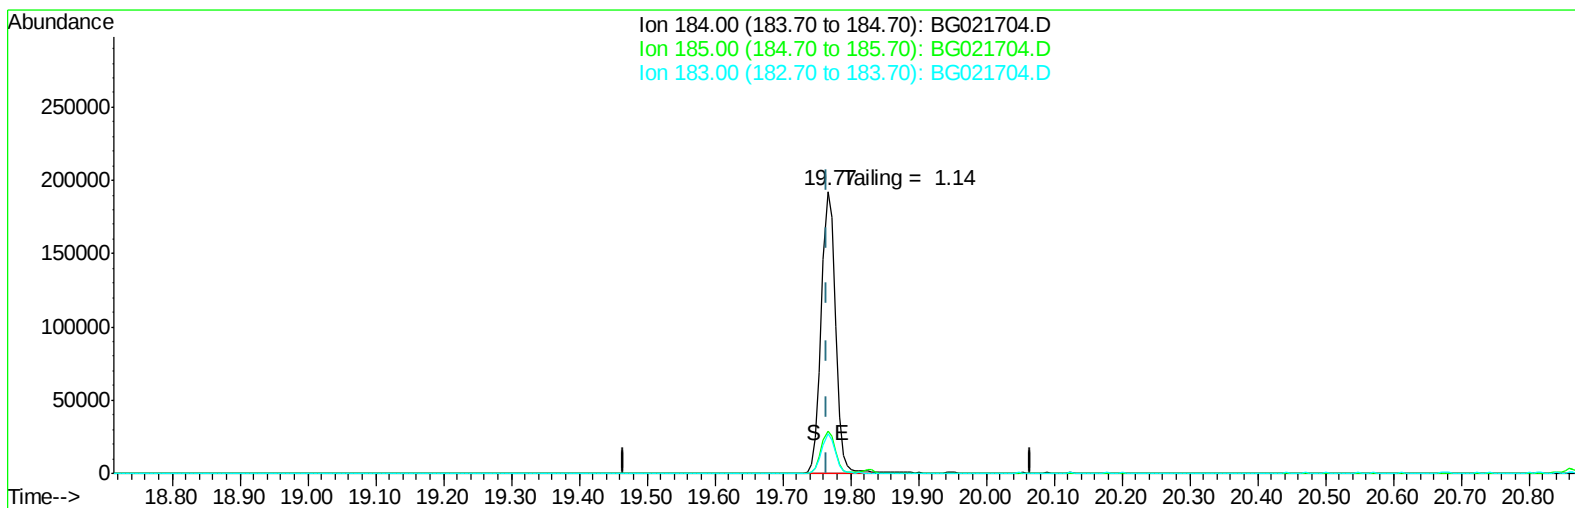

TIC: BG021704.D

(76) Benzidine

19.766min (-0.001) 117289.39ng

response 277541

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.91
183.00	12.80	14.21
0.00	0.00	0.00