


Data Path : Z:\HPCHEM1\BNA G\Data\BG041516\
 Data File : BG021690.D
 Acq On : 15 Apr 2016 18:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

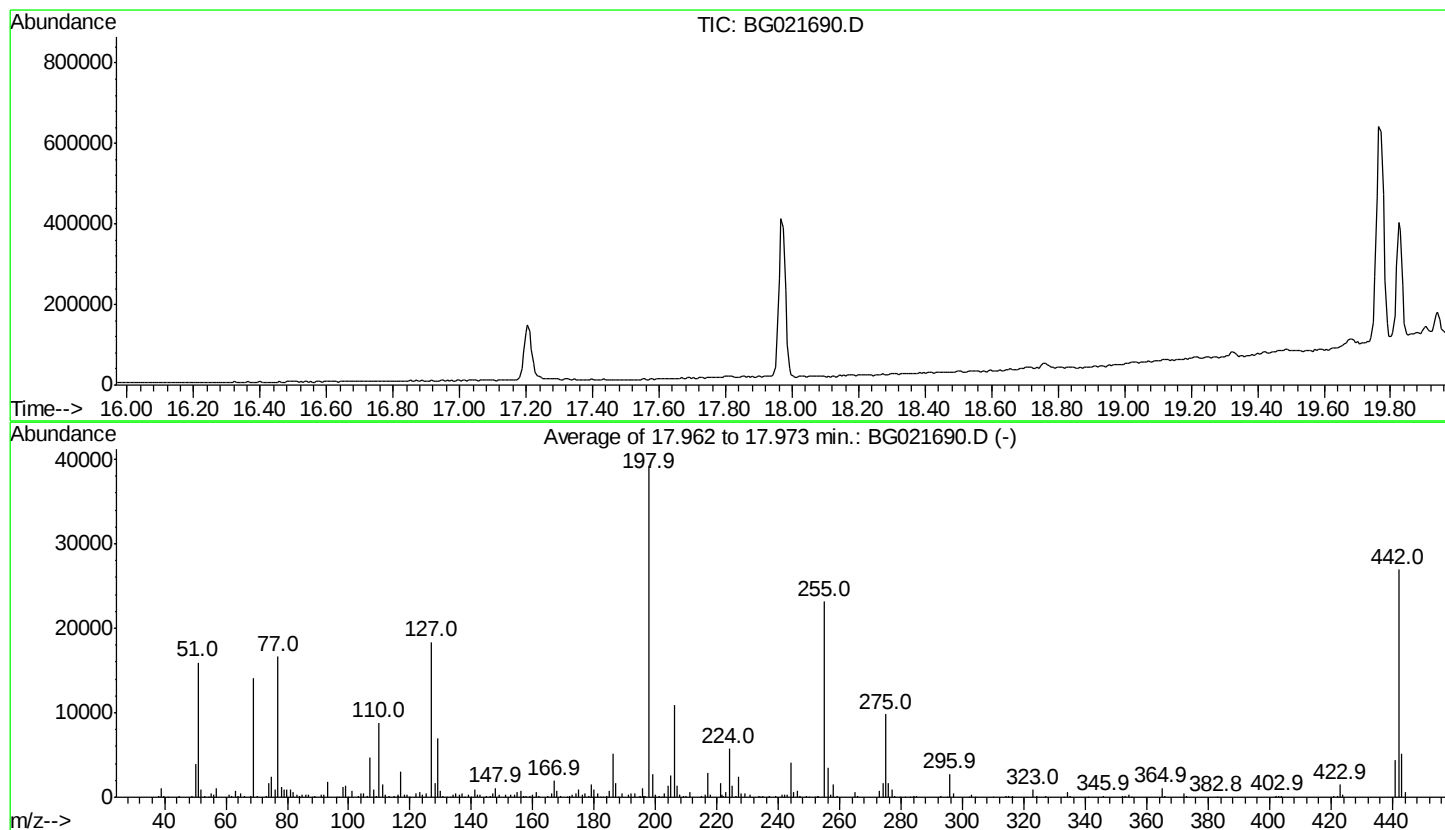

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	15943	PASS
68	69	0.00	2	1.1	157	PASS
69	198	0.00	100	35.9	14074	PASS
70	69	0.00	2	1.0	142	PASS
127	198	10	80	46.8	18385	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39256	PASS
199	198	5	9	6.8	2678	PASS
275	198	10	60	25.1	9834	PASS
365	198	1	100	2.9	1137	PASS
441	442	0.01	24	16.2	4378	PASS
442	198	50	100	68.7	26962	PASS
443	442	15	24	19.3	5210	PASS