


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041516\
 Data File : BG021704.D
 Acq On : 16 Apr 2016 6:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

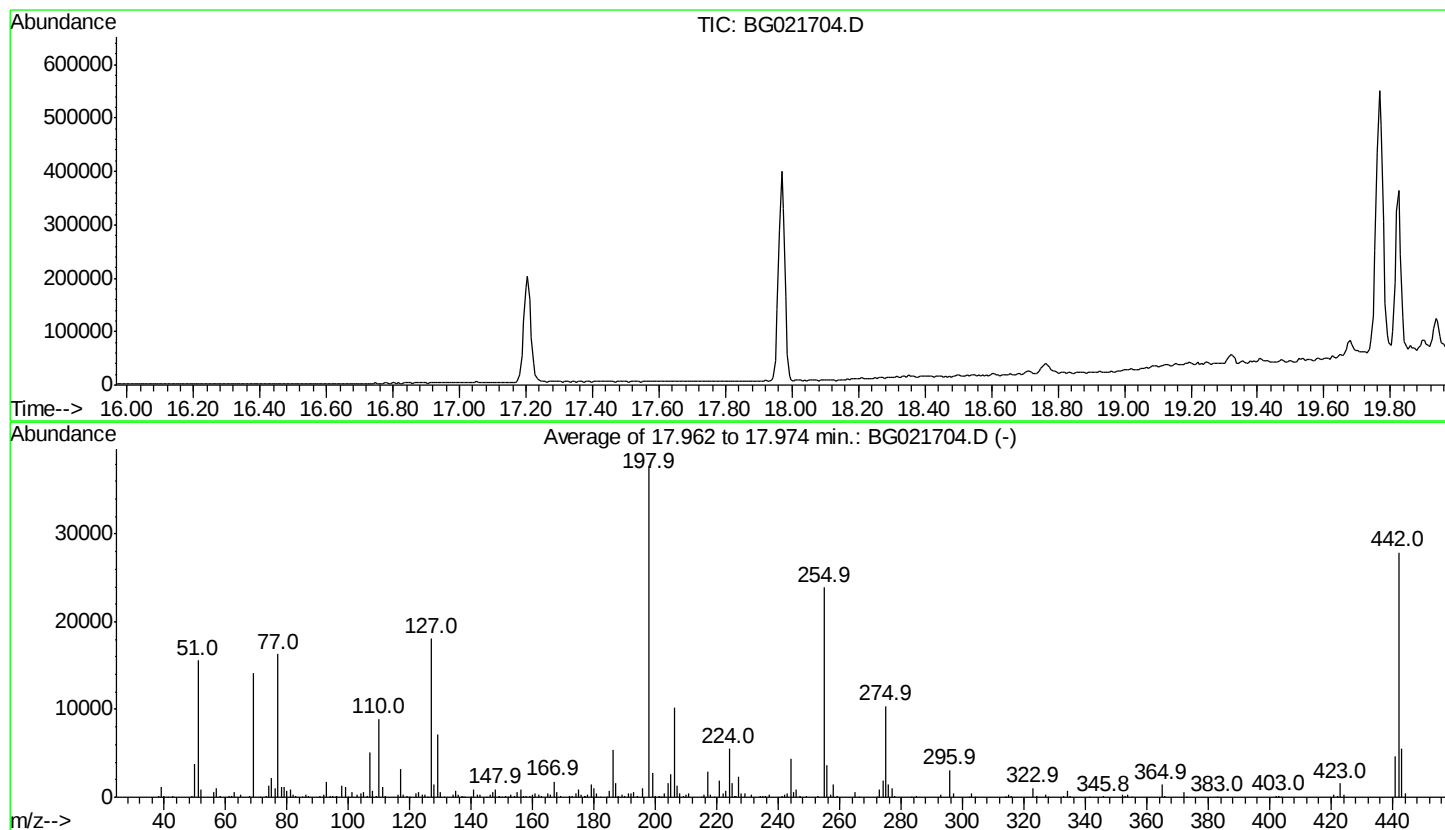

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	15565	PASS
68	69	0.00	2	0.6	81	PASS
69	198	0.00	100	37.4	14125	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	18044	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37792	PASS
199	198	5	9	7.4	2784	PASS
275	198	10	60	27.6	10427	PASS
365	198	1	100	3.7	1401	PASS
441	442	0.01	24	16.6	4644	PASS
442	198	50	100	73.9	27922	PASS
443	442	15	24	19.9	5555	PASS