
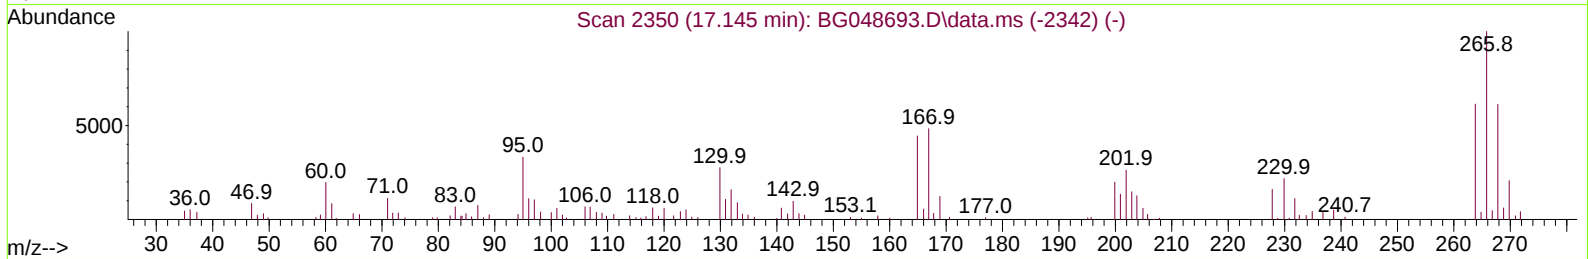
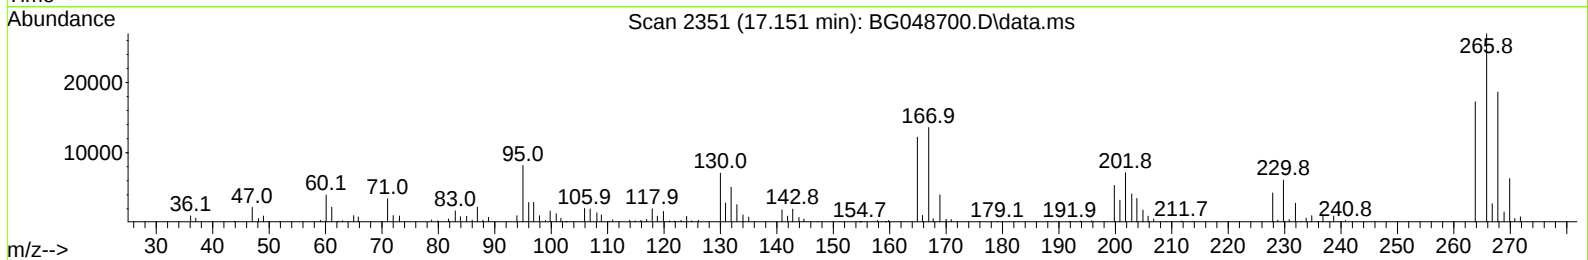


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048700.D
 Acq On : 15 Apr 2021 8:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 09:55:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 15 01:59:11 2021
 Response via : Initial Calibration

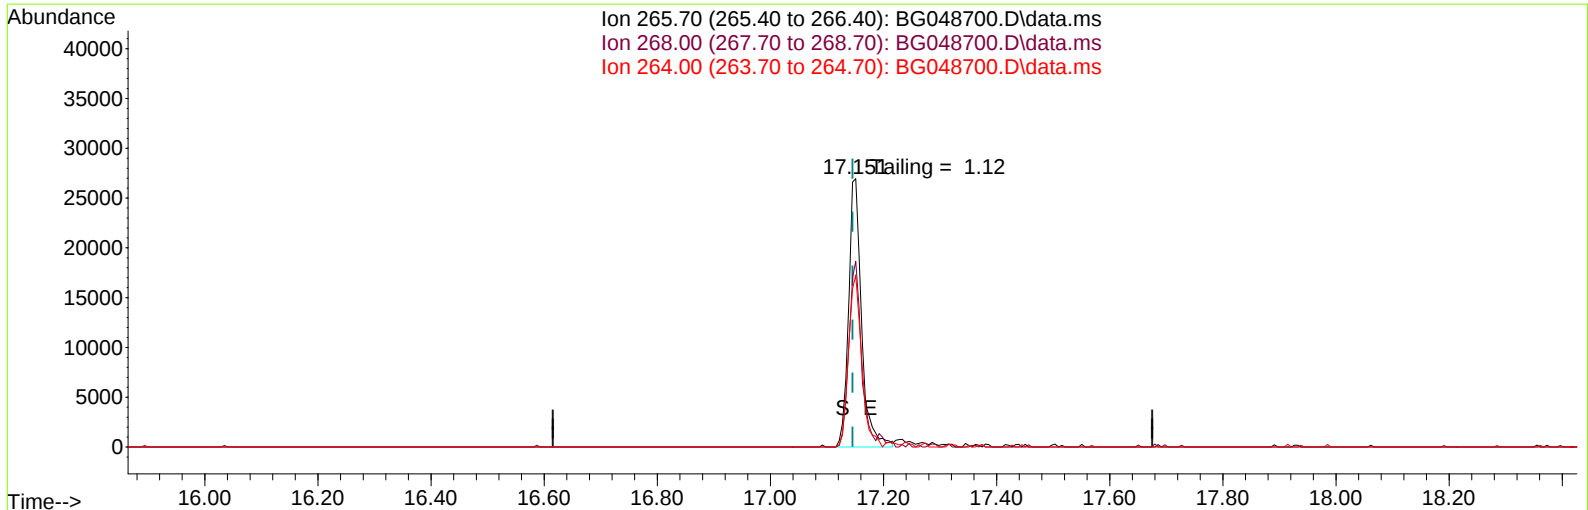

TIC: BG048700.D\data.ms

(70) Pentachlorophenol (C)




17.151min (+ 0.006) 100607.71 ng

response 43125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	69.22
264.00	61.30	64.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048700.D
 Acq On : 15 Apr 2021 8:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 15 09:55:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 15 01:59:11 2021
 Response via : Initial Calibration

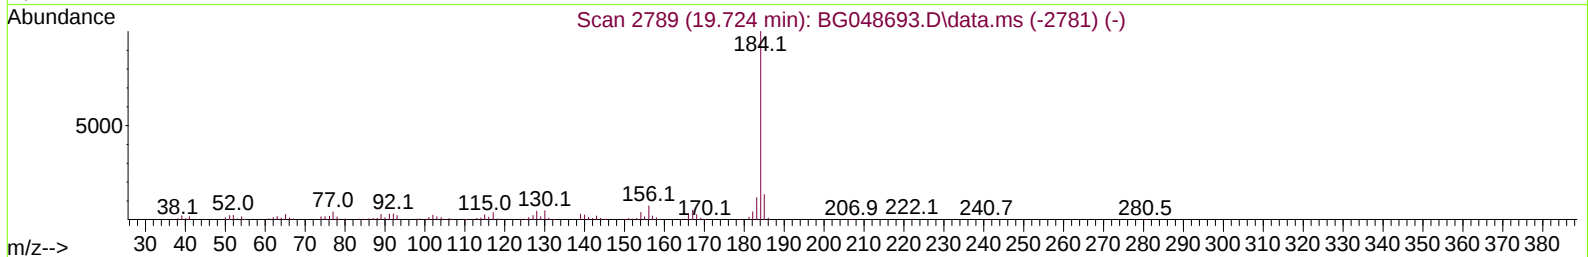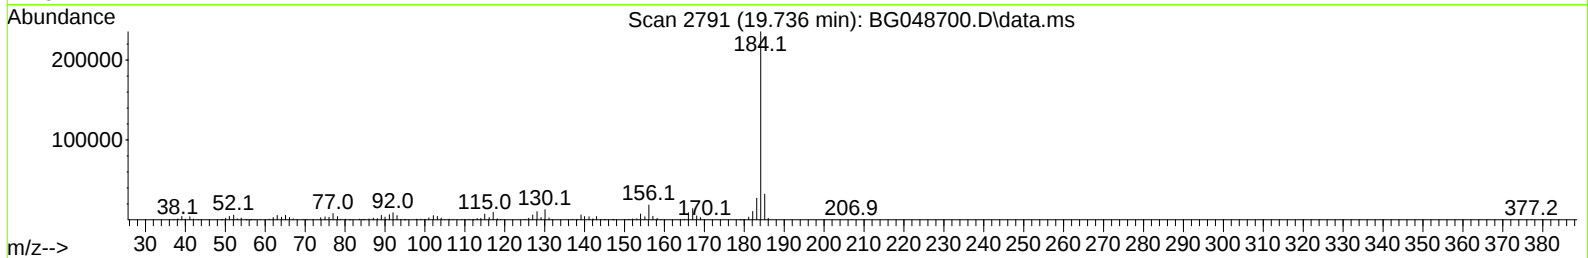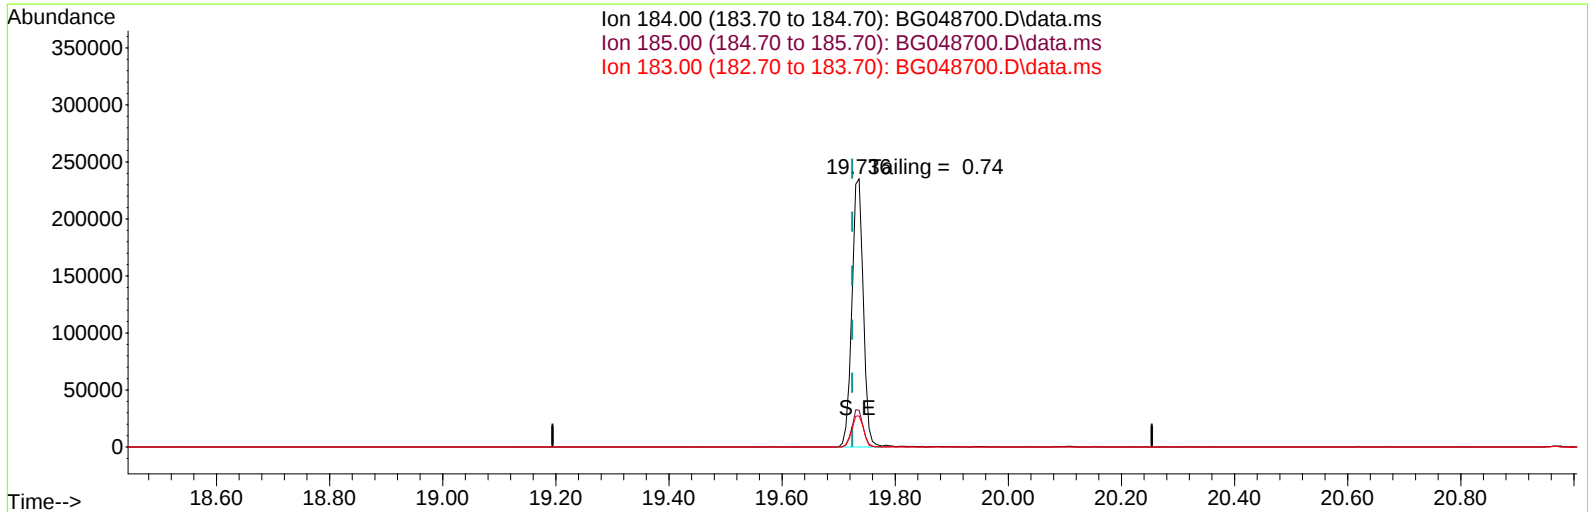

TIC: BG048700.D\data.ms

(77) Benzidine**19.736min (+ 0.012) 7019.08 ng****response 329378**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.72
183.00	11.70	11.60
0.00	0.00	0.00