

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048717.D
 Acq On : 15 Apr 2021 20:26
 Operator : CG/JU
 Sample : M1998-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-4C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.162	302	310	319	rBV	214240	336684	38.03%	3.983%
2	5.638	384	391	398	rBV	150586	240391	27.15%	2.844%
3	6.619	554	558	563	rVB3	7749	11021	1.24%	0.130%
4	7.060	627	633	637	rBV3	6082	10575	1.19%	0.125%
5	7.248	655	665	680	rBV2	325758	853444	96.40%	10.096%
6	7.524	705	712	716	rBV4	8317	15231	1.72%	0.180%
7	7.712	738	744	749	rVB2	15643	26296	2.97%	0.311%
8	7.864	765	770	775	rBV2	24161	36705	4.15%	0.434%
9	8.088	798	808	813	rBV	106639	207178	23.40%	2.451%
10	8.135	813	816	824	rVB3	27682	46180	5.22%	0.546%
11	8.205	824	828	834	rBV4	6511	14022	1.58%	0.166%
12	8.264	834	838	842	rBV6	9502	14070	1.59%	0.166%
13	8.311	842	846	852	rBV3	8524	14398	1.63%	0.170%
14	8.628	894	900	901	rBV3	7615	13672	1.54%	0.162%
15	8.752	917	921	926	rVB7	8282	14344	1.62%	0.170%
16	8.857	934	939	943	rBV5	5287	11194	1.26%	0.132%
17	9.163	987	991	993	rBV5	7849	11783	1.33%	0.139%
18	9.198	993	997	1000	rVB4	10630	15405	1.74%	0.182%
19	9.257	1000	1007	1014	rBV	234039	426127	48.13%	5.041%
20	9.410	1028	1033	1035	rBV4	8849	14961	1.69%	0.177%
21	9.568	1053	1060	1063	rVB7	5698	10951	1.24%	0.130%
22	9.651	1070	1074	1079	rVV6	6344	11319	1.28%	0.134%
23	9.727	1083	1087	1092	rVB5	9824	15315	1.73%	0.181%
24	9.821	1100	1103	1107	rBV4	7452	9986	1.13%	0.118%
25	10.021	1133	1137	1141	rVB6	8001	13495	1.52%	0.160%
26	10.080	1141	1147	1153	rBV7	14086	27844	3.14%	0.329%
27	10.315	1180	1187	1191	rBV7	8458	19078	2.15%	0.226%
28	10.473	1209	1214	1216	rBV5	7122	11512	1.30%	0.136%
29	10.608	1232	1237	1238	rBV5	7472	10619	1.20%	0.126%
30	10.867	1276	1281	1282	rBV4	14983	18141	2.05%	0.215%
31	10.914	1283	1289	1294	rVB	146229	248687	28.09%	2.942%
32	11.055	1308	1313	1318	rVB2	25793	41263	4.66%	0.488%
33	11.396	1365	1371	1376	rVB8	13204	25753	2.91%	0.305%
34	11.566	1397	1400	1403	rBV5	6053	9147	1.03%	0.108%
35	11.613	1403	1408	1414	rVB9	12011	25504	2.88%	0.302%
36	11.731	1424	1428	1434	rBV8	11514	24046	2.72%	0.284%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048717.D
 Acq On : 15 Apr 2021 20:26
 Operator : CG/JU
 Sample : M1998-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-4C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.819	1436	1443	1444	rBV6	10321	17354	1.96%	0.205%
38	11.919	1452	1460	1464	rBV3	34798	61927	6.99%	0.733%
39	11.966	1464	1468	1471	rVV6	16068	25115	2.84%	0.297%
40	12.007	1471	1475	1483	rVB8	16464	33397	3.77%	0.395%
41	12.095	1483	1490	1496	rBV9	12784	34555	3.90%	0.409%
42	12.189	1502	1506	1509	rVB5	10979	12237	1.38%	0.145%
43	12.312	1524	1527	1533	rBV7	12831	23758	2.68%	0.281%
44	12.400	1538	1542	1549	rVB	56883	95790	10.82%	1.133%
45	12.647	1576	1584	1588	rBV9	18354	42070	4.75%	0.498%
46	12.788	1605	1608	1614	rVB8	10368	16482	1.86%	0.195%
47	12.894	1623	1626	1629	rBV5	6978	9322	1.05%	0.110%
48	12.947	1630	1635	1641	rVV10	17358	36093	4.08%	0.427%
49	13.094	1656	1660	1661	rBV4	8157	10362	1.17%	0.123%
50	13.182	1670	1675	1677	rBV5	11862	21076	2.38%	0.249%
51	13.264	1685	1689	1693	rVB3	43859	63462	7.17%	0.751%
52	13.358	1699	1705	1713	rVB	506110	796427	89.96%	9.422%
53	13.528	1729	1734	1735	rBV5	22478	31405	3.55%	0.372%
54	13.998	1810	1814	1816	rBV5	7618	11621	1.31%	0.137%
55	14.063	1820	1825	1830	rVV9	22527	49201	5.56%	0.582%
56	14.116	1830	1834	1836	rVV5	18776	18872	2.13%	0.223%
57	14.157	1838	1841	1846	rVV4	41780	78096	8.82%	0.924%
58	14.204	1846	1849	1853	rVB4	67185	89886	10.15%	1.063%
59	14.251	1855	1857	1860	rBV4	13554	17527	1.98%	0.207%
60	14.380	1876	1879	1883	rVB6	10155	12198	1.38%	0.144%
61	14.480	1892	1896	1901	rBV8	19558	35935	4.06%	0.425%
62	14.568	1907	1911	1916	rVB5	48272	73729	8.33%	0.872%
63	14.621	1917	1920	1921	rBV3	11647	12069	1.36%	0.143%
64	14.703	1930	1934	1935	rBV3	20108	25520	2.88%	0.302%
65	14.739	1935	1940	1947	rVB	209569	337457	38.12%	3.992%
66	15.127	2003	2006	2012	rVB7	28287	48558	5.48%	0.574%
67	15.179	2012	2015	2017	rBV4	10225	11603	1.31%	0.137%
68	15.450	2059	2061	2063	rBV3	13263	15731	1.78%	0.186%
69	15.532	2068	2075	2078	rBV8	35221	75291	8.50%	0.891%
70	15.626	2087	2091	2095	rBV7	17024	31125	3.52%	0.368%
71	15.978	2147	2151	2156	rVB	55181	84908	9.59%	1.004%
72	16.196	2186	2188	2192	rBV5	16932	15972	1.80%	0.189%
73	16.237	2192	2195	2199	rBV5	22500	29016	3.28%	0.343%
74	16.460	2227	2233	2241	rVB3	142968	228952	25.86%	2.709%
75	16.560	2247	2250	2255	rBV4	31322	51324	5.80%	0.607%
76	17.230	2362	2364	2368	rVB5	19729	16036	1.81%	0.190%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048717.D
 Acq On : 15 Apr 2021 20:26
 Operator : CG/JU
 Sample : M1998-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-4C

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	17.289	2369	2374	2378	rVB	72806	106057	11.98%	1.255%
78	17.500	2404	2410	2414	rBV	219247	350221	39.56%	4.143%
79	17.565	2419	2421	2428	rVB3	77609	100488	11.35%	1.189%
80	17.765	2453	2455	2457	rBV3	18910	19538	2.21%	0.231%
81	17.900	2474	2478	2484	rBV9	33584	67911	7.67%	0.803%
82	19.228	2702	2704	2707	rVB3	54166	51697	5.84%	0.612%
83	19.474	2742	2746	2752	rBV9	43324	78127	8.82%	0.924%
84	19.551	2756	2759	2763	rVV	58270	73795	8.34%	0.873%
85	19.604	2765	2768	2772	rVB4	64530	85010	9.60%	1.006%
86	19.921	2818	2822	2828	rVB2	76196	124658	14.08%	1.475%
87	20.109	2850	2854	2860	rVB	723191	885345	100.00%	10.474%
88	21.413	3073	3076	3081	rVB4	92393	130461	14.74%	1.543%
89	21.672	3117	3120	3127	rVB	132153	178159	20.12%	2.108%
90	21.801	3138	3142	3147	rVB	186065	308535	34.85%	3.650%
91	25.162	3707	3714	3722	rVB	101833	296582	33.50%	3.509%
92	26.936	4014	4016	4017	rBV2	18982	12490	1.41%	0.148%
93	32.459	4954	4956	4959	rBV4	12632	13437	1.52%	0.159%
94	32.489	4959	4961	4964	rVB4	14904	12704	1.43%	0.150%




Sum of corrected areas: 8453015

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
Data File : BG048717.D
Acq On : 15 Apr 2021 20:26
Operator : CG/JU
Sample : M1998-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-4C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

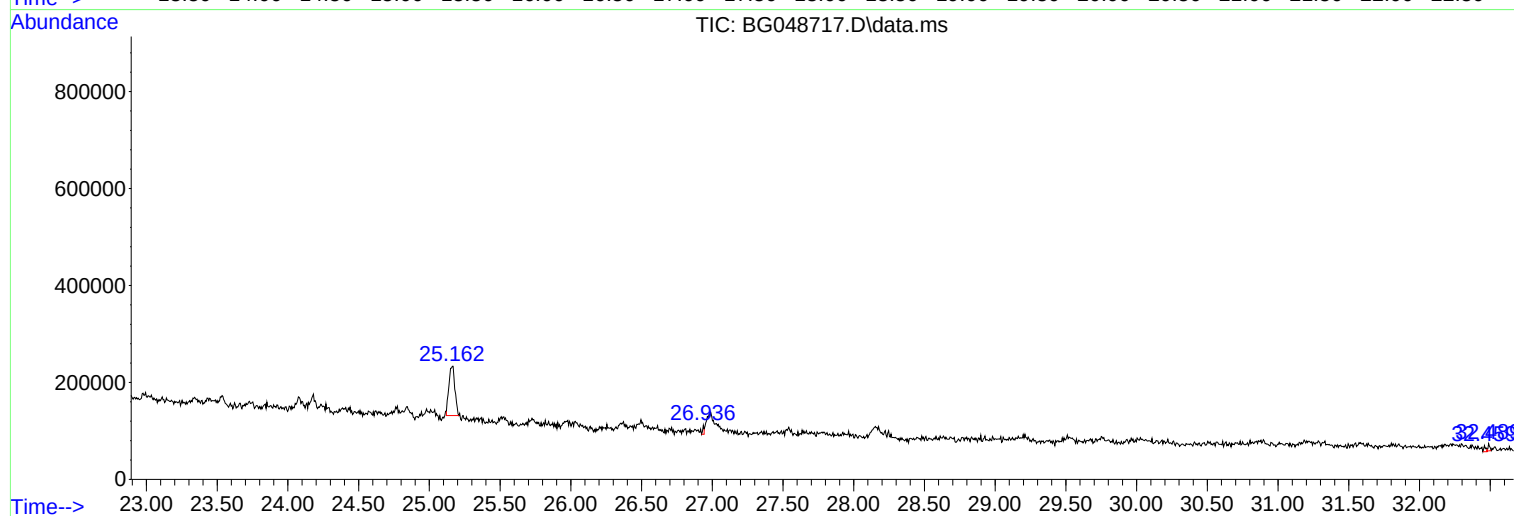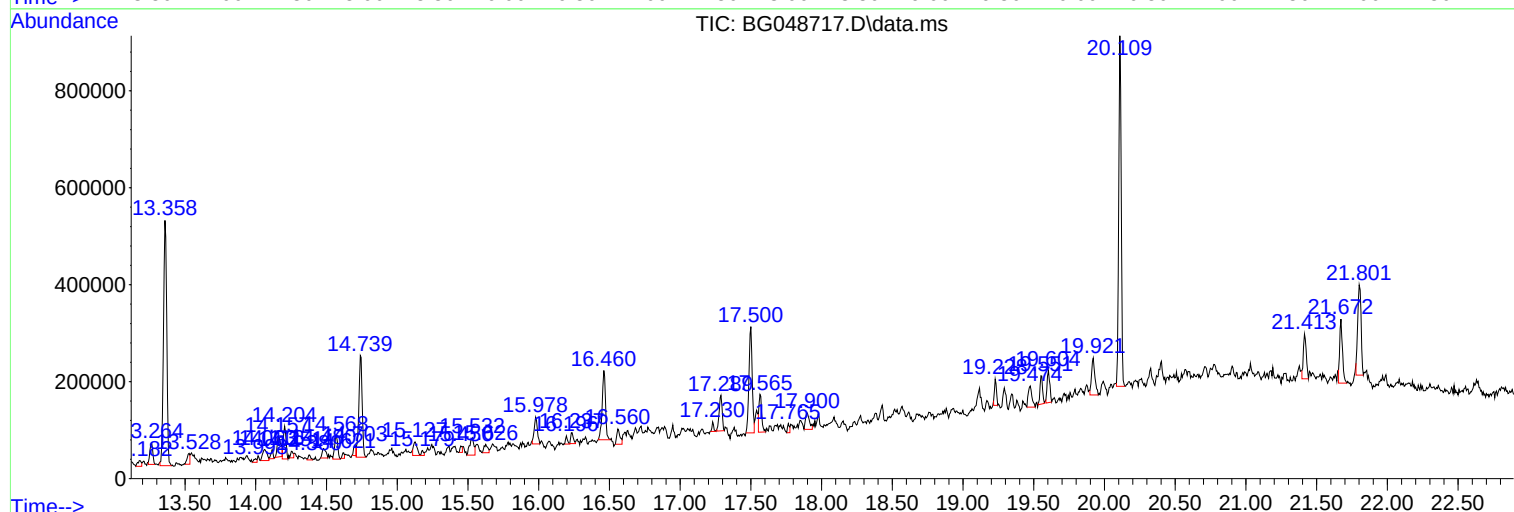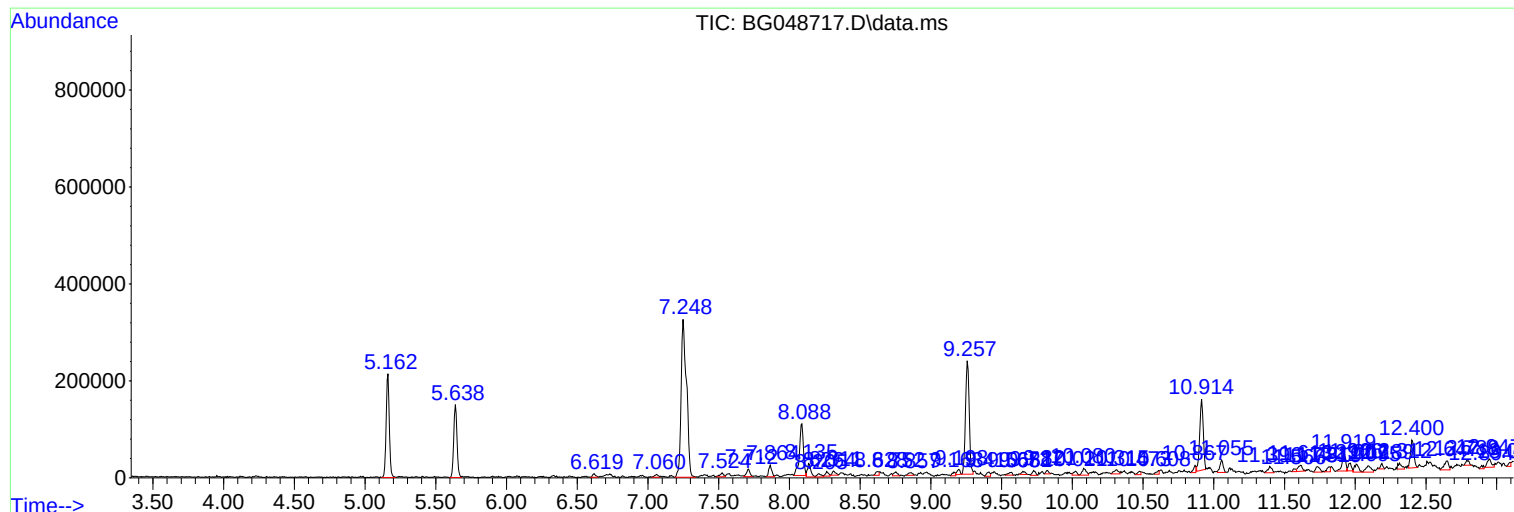

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
Data File : BG048717.D
Acq On : 15 Apr 2021 20:26
Operator : CG/JU
Sample : M1998-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-4C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
Data File : BG048717.D
Acq On : 15 Apr 2021 20:26
Operator : CG/JU
Sample : M1998-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-4C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
