


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048700.D
 Acq On : 15 Apr 2021 8:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 12:19:56 2021

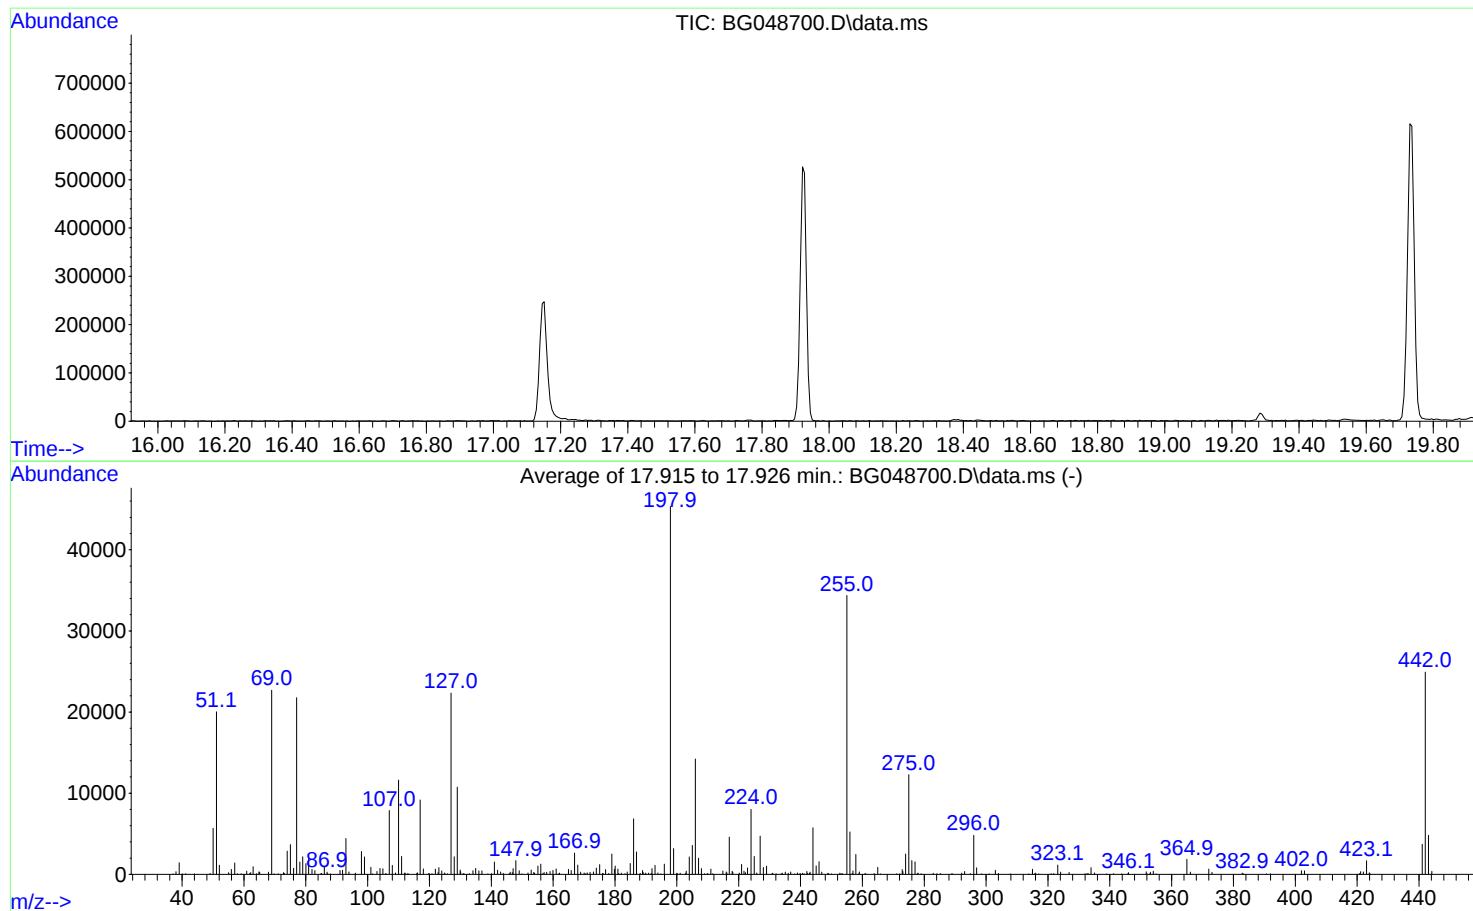




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	20042	PASS
68	69	0.00	2	1.2	276	PASS
69	198	0.00	100	50.1	22704	PASS
70	69	0.00	2	0.2	51	PASS
127	198	10	80	49.3	22347	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45331	PASS
199	198	5	9	7.0	3170	PASS
275	198	10	60	27.1	12279	PASS
365	198	1	100	4.1	1850	PASS
441	198	0.01	100	8.2	3711	PASS
442	198	50	100	55.0	24920	PASS
443	442	15	24	19.3	4816	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048700.D
 Acq On : 15 Apr 2021 8:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 15 09:55:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 15 01:59:11 2021
 Response via : Initial Calibration

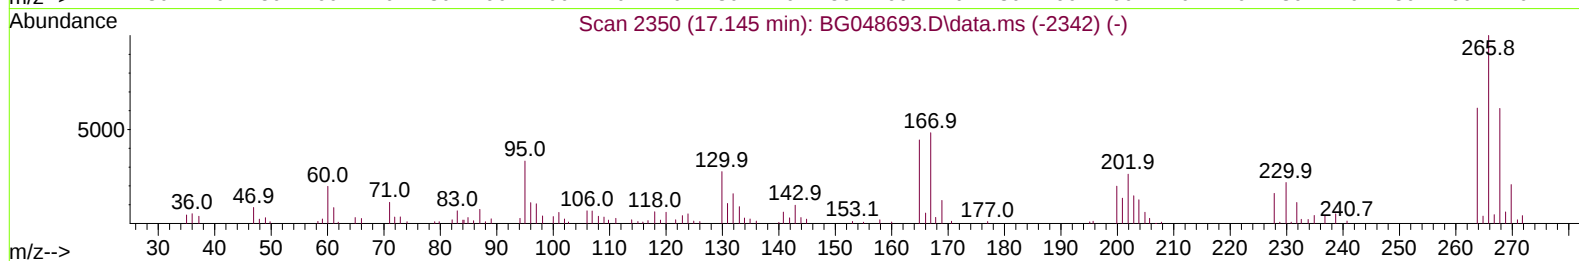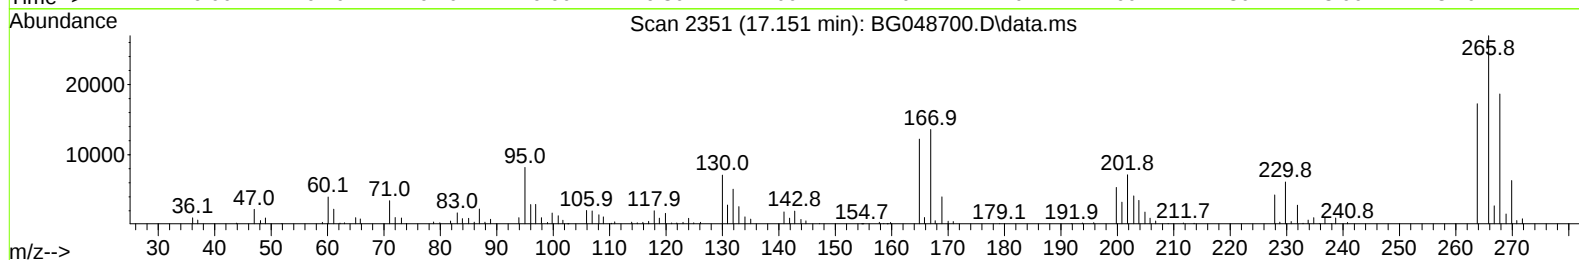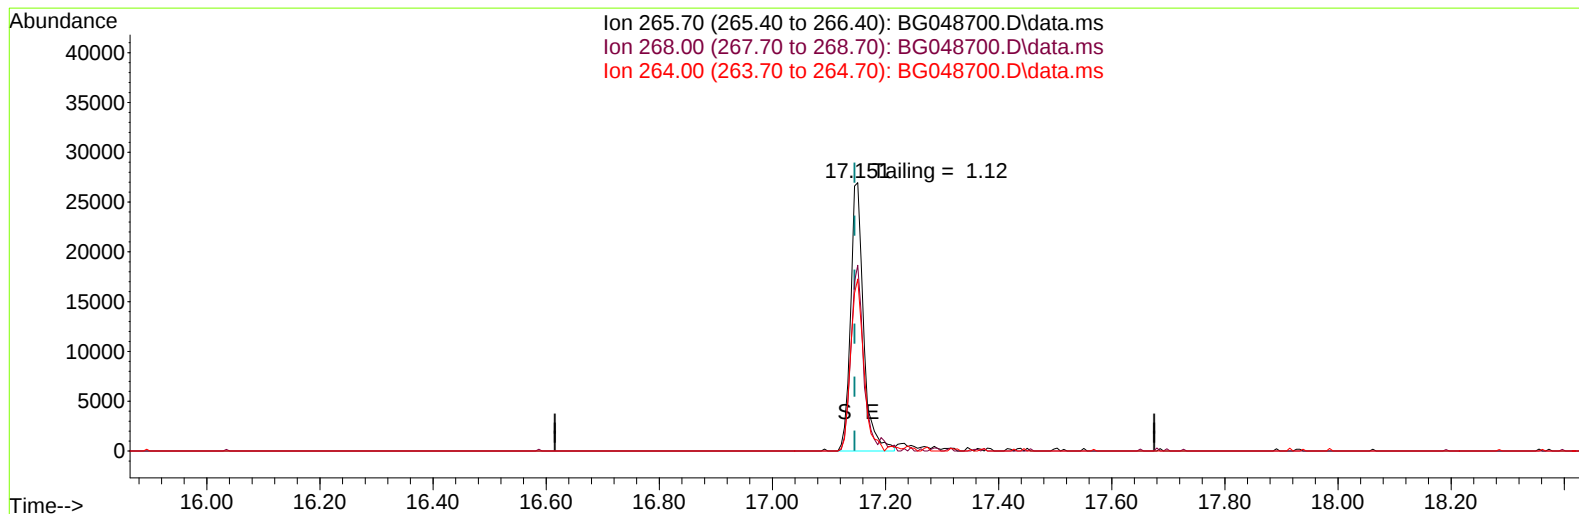

TIC: BG048700.D\data.ms

(70) Pentachlorophenol (C)

17.151min (+ 0.006) 100607.71 ng




response 43125

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	69.22
264.00	61.30	64.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041521\
 Data File : BG048700.D
 Acq On : 15 Apr 2021 8:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 15 09:55:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 15 01:59:11 2021
 Response via : Initial Calibration

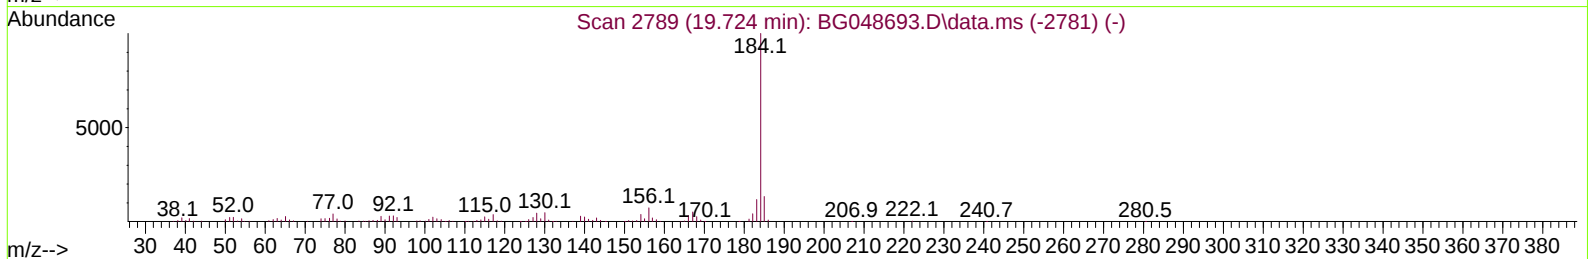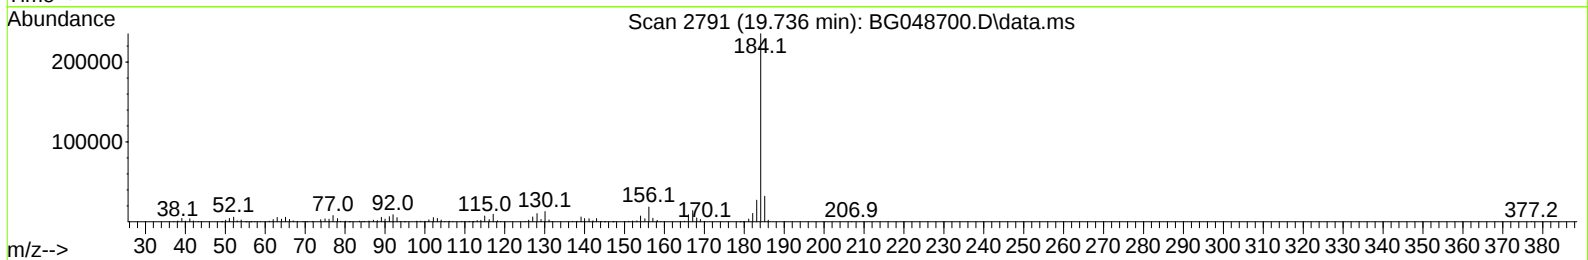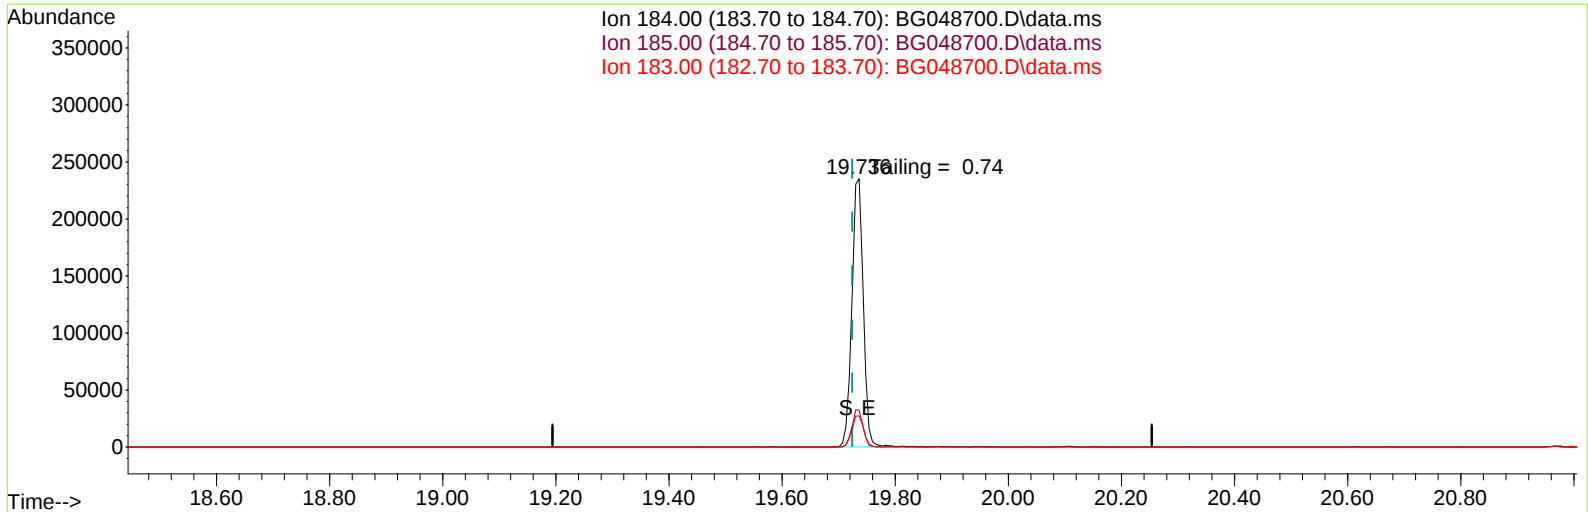

TIC: BG048700.D\data.ms

(77) Benzidine

19.736min (+ 0.012) 7019.08 ng

response 329378

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.72
183.00	11.70	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/15/2021	BNA_G	BG048700.D
Compound Name	Response	Retention Time
DDT	184955	20.97
DDD	4048	20.523
DDE	595	20.018
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4643	189598	2.45