


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041522\
 Data File : BG053160.D
 Acq On : 15 Apr 2022 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

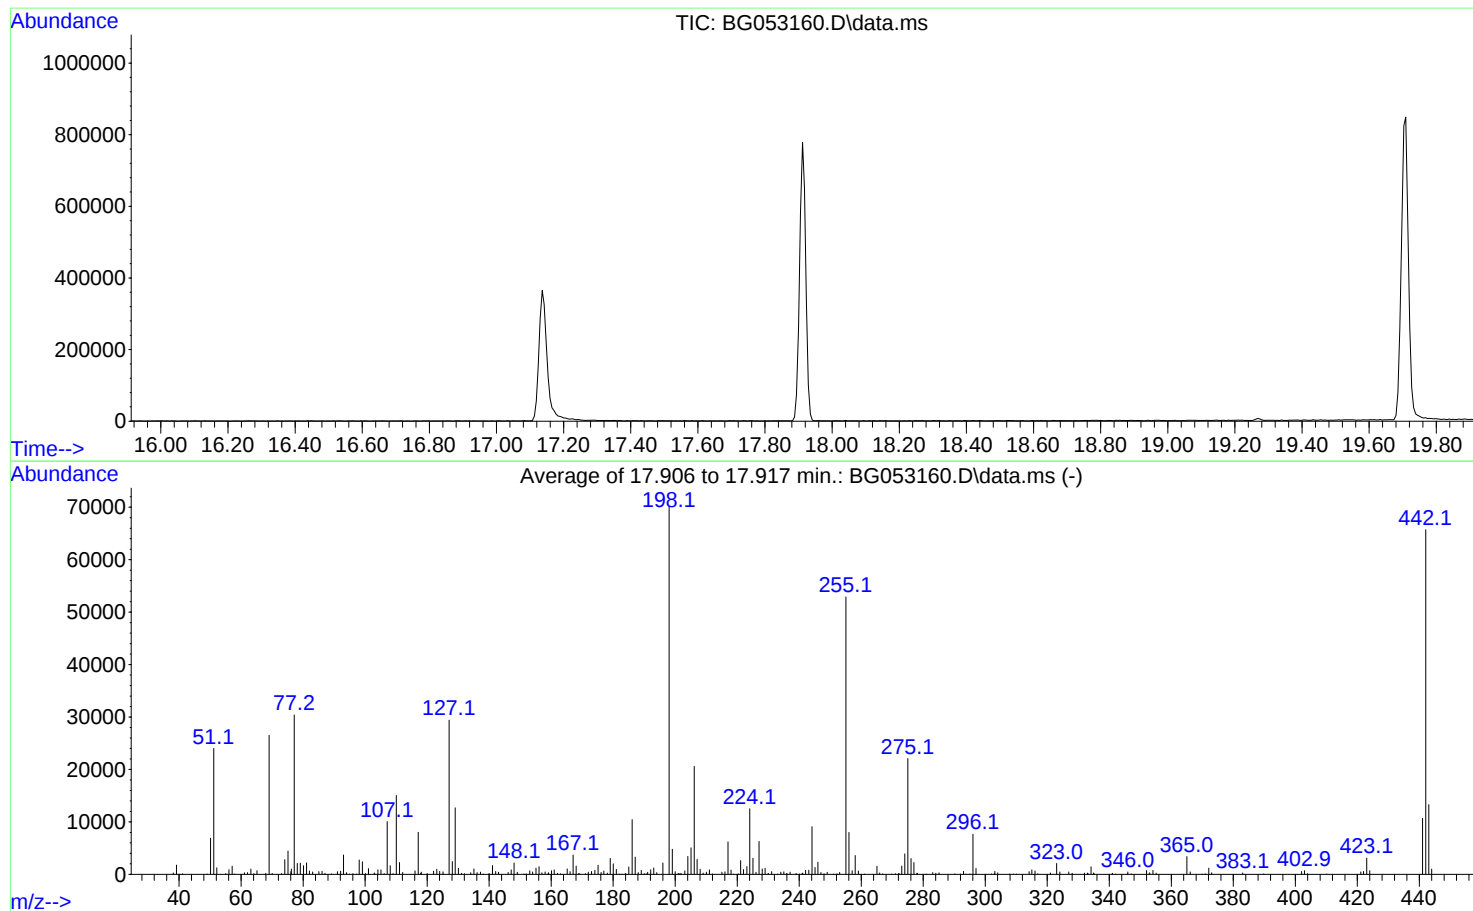

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	24011	PASS
68	69	0.00	2	0.7	173	PASS
69	198	0.00	100	37.8	26504	PASS
70	69	0.00	2	0.7	174	PASS
127	198	10	80	41.9	29400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70139	PASS
199	198	5	9	6.8	4798	PASS
275	198	10	60	31.5	22083	PASS
365	198	1	100	4.8	3391	PASS
441	198	0.01	100	15.2	10675	PASS
442	442	50	100	100.0	65707	PASS
443	442	15	24	20.2	13293	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/15/2022	BNA_G	<u>BG053160.D</u>
Compound Name	Response	Retention Time
DDT	273823	20.943
DDD	5059	20.496
DDE	1046	19.991
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6105	279928	2.18

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041522\
Data File : BG053160.D
Acq On : 15 Apr 2022 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 08:32:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

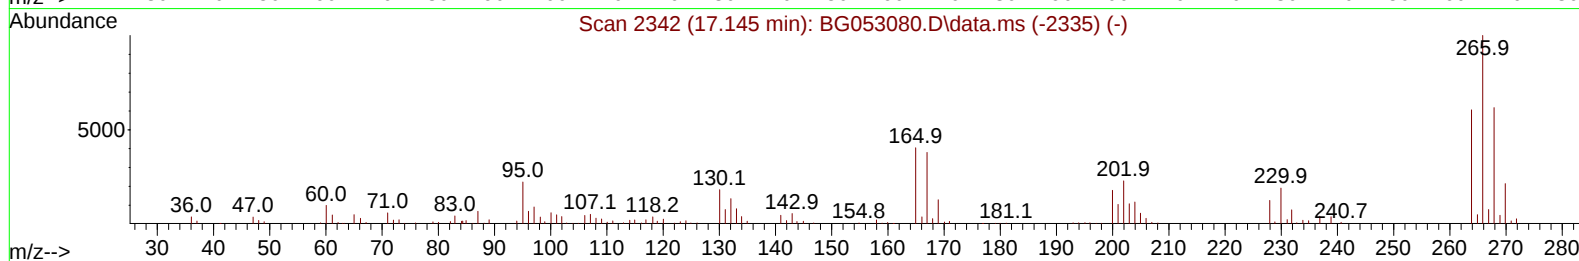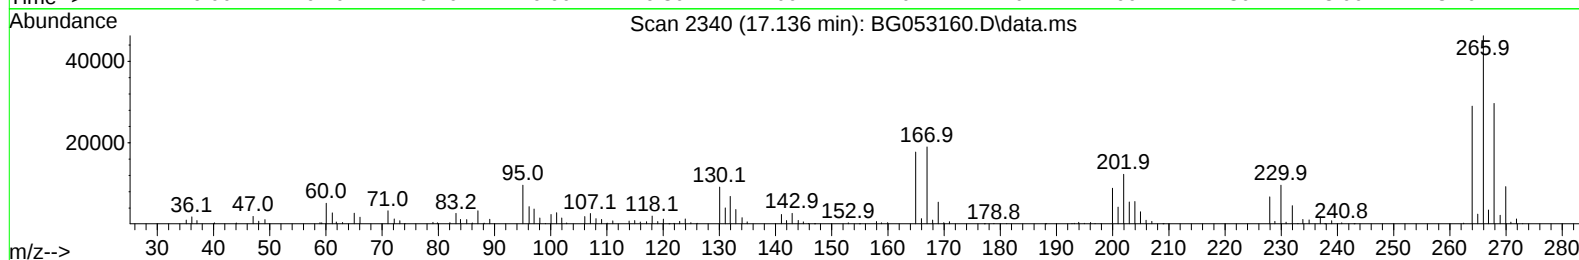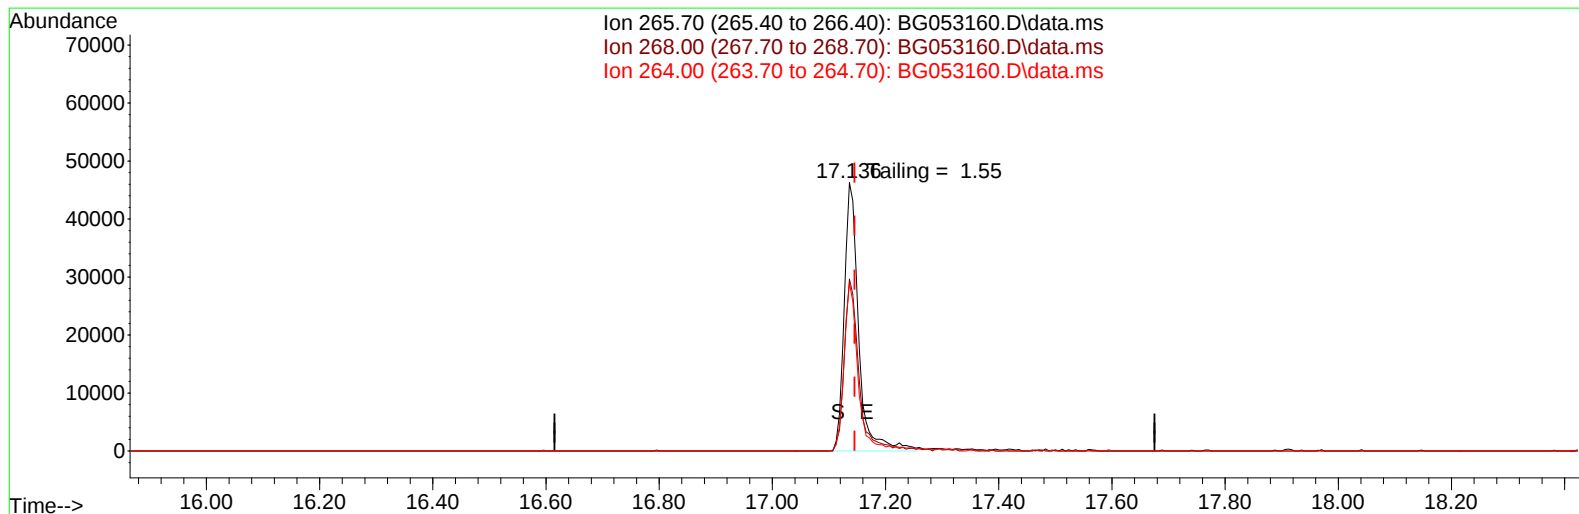

TIC: BG053160.D\data.ms

(70) Pentachlorophenol (C)

17.136min (-0.009) 178747.99 ng




response 79980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.09
264.00	56.60	62.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041522\
 Data File : BG053160.D
 Acq On : 15 Apr 2022 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 19 08:32:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 08 15:31:24 2022
 Response via : Initial Calibration

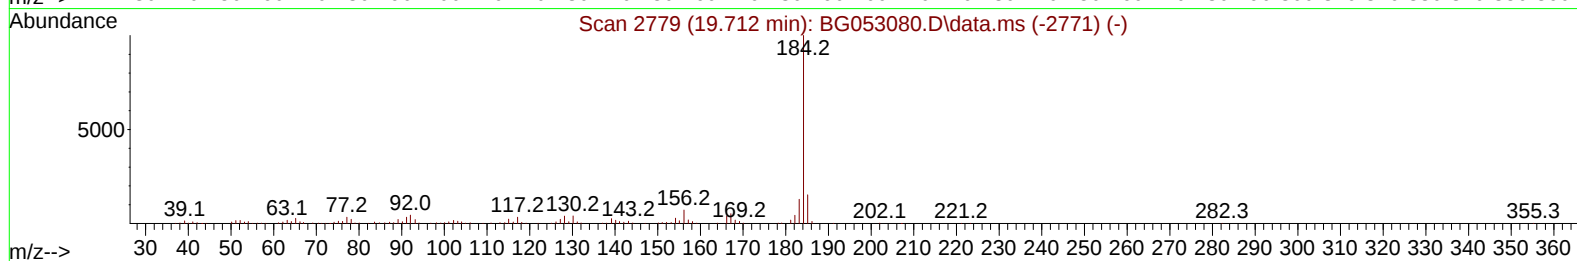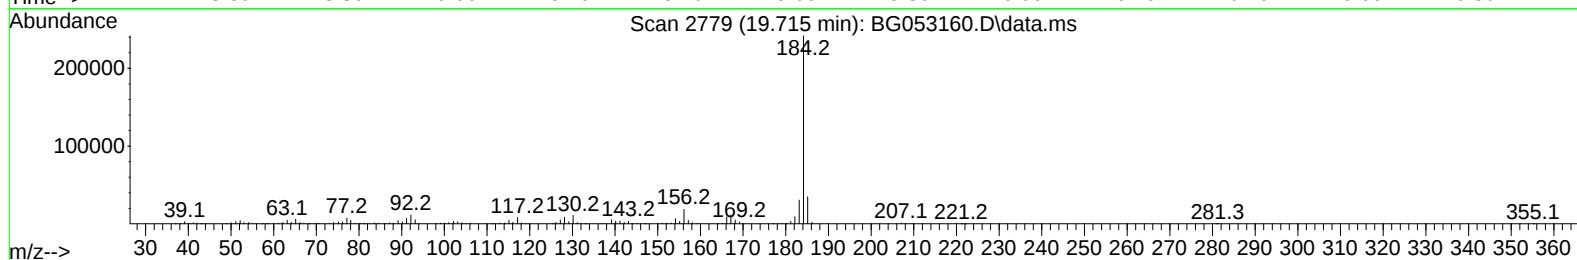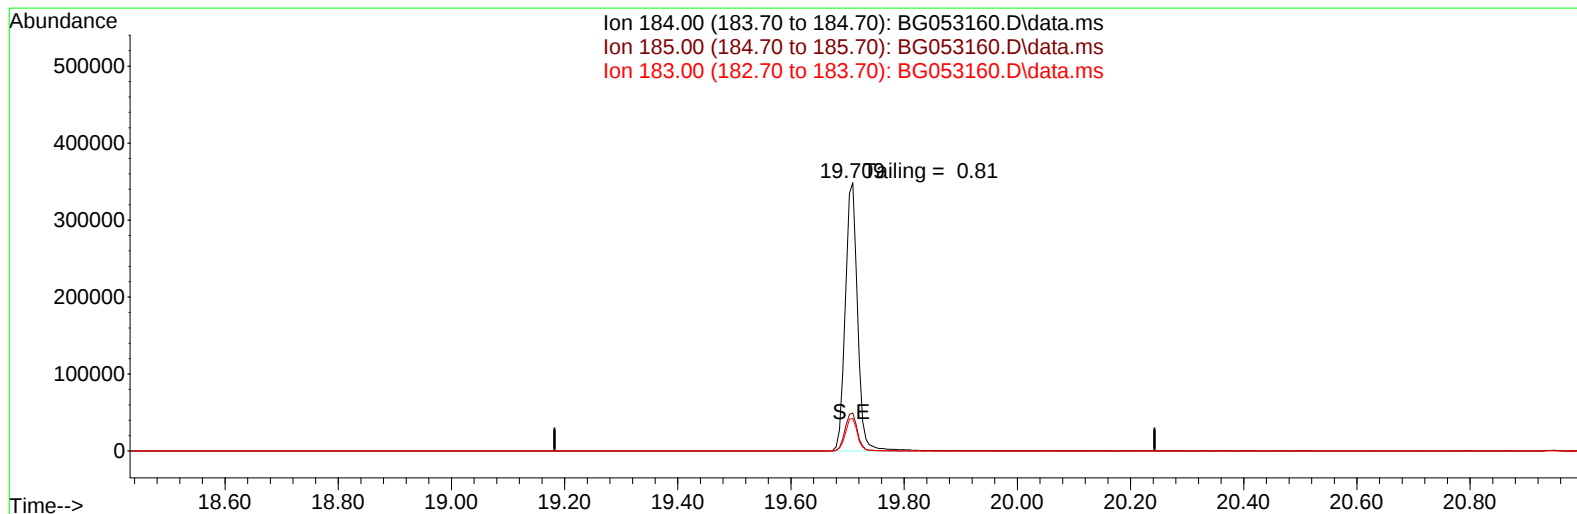

TIC: BG053160.D\data.ms

(77) Benzidine

19.712min (-19.712) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.40	0.00#
183.00	11.80	0.00#
0.00	0.00	0.00