
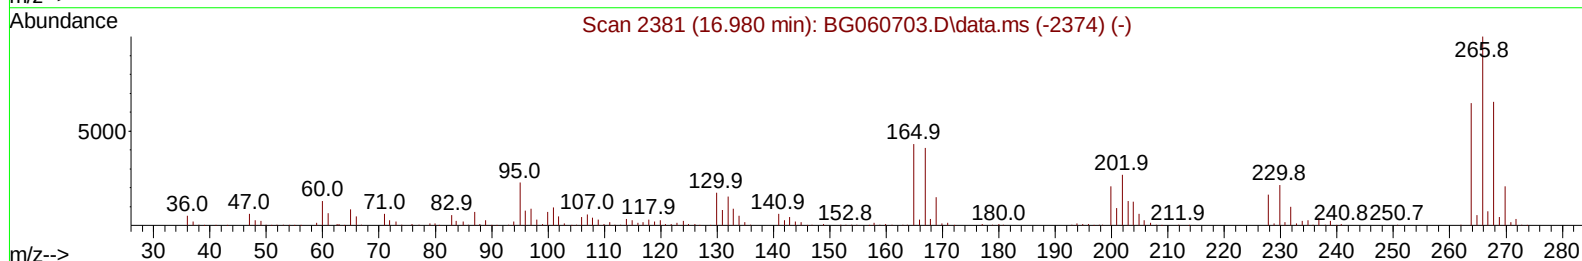
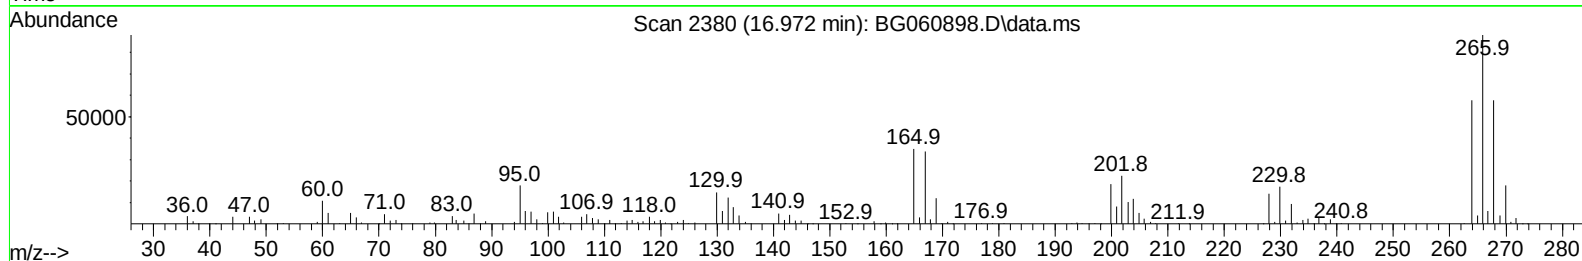


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060898.D
Acq On : 15 Apr 2024 10:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 03:52:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

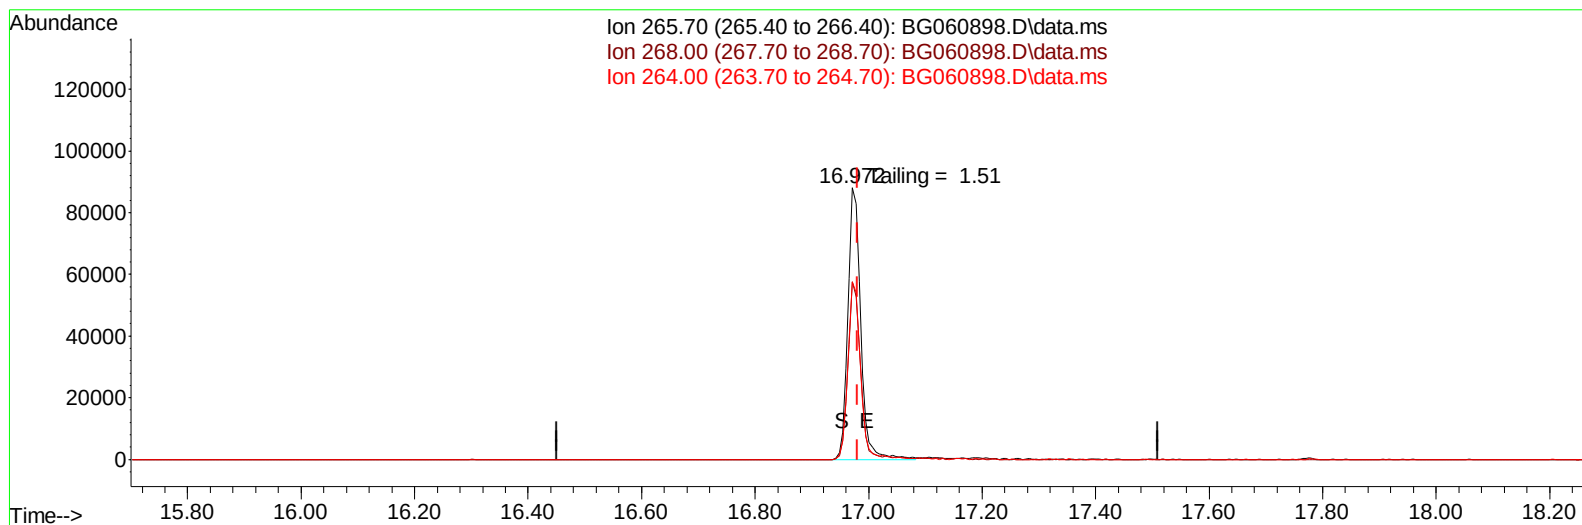




TIC: BG060898.D\data.ms

(70) Pentachlorophenol (C)**16.972min (-0.009) 20970.05 ng****response 138419**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.40
264.00	64.70	65.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060898.D
Acq On : 15 Apr 2024 10:39
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 03:52:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

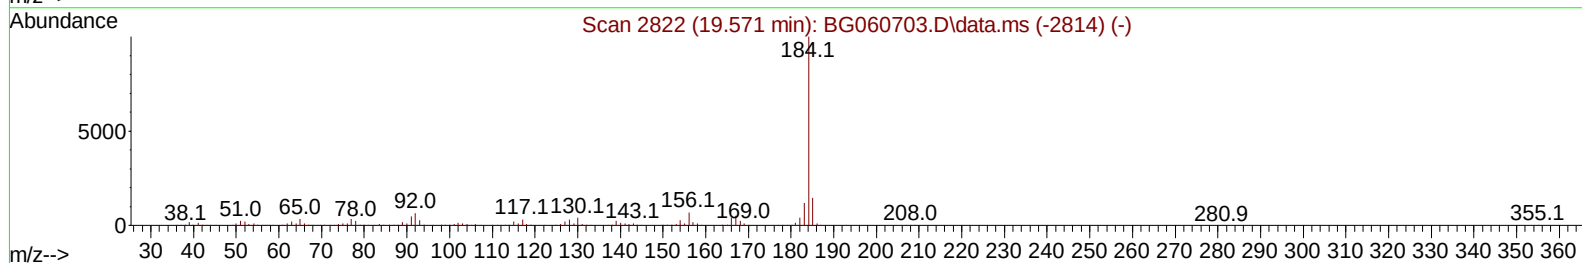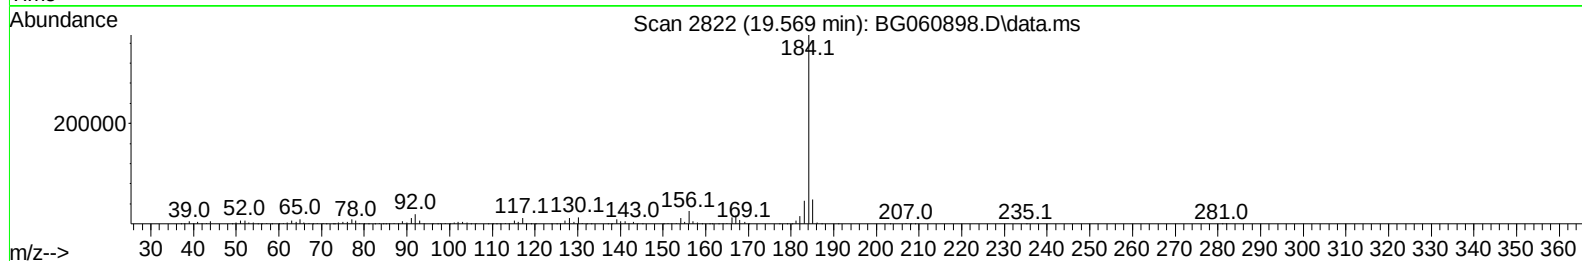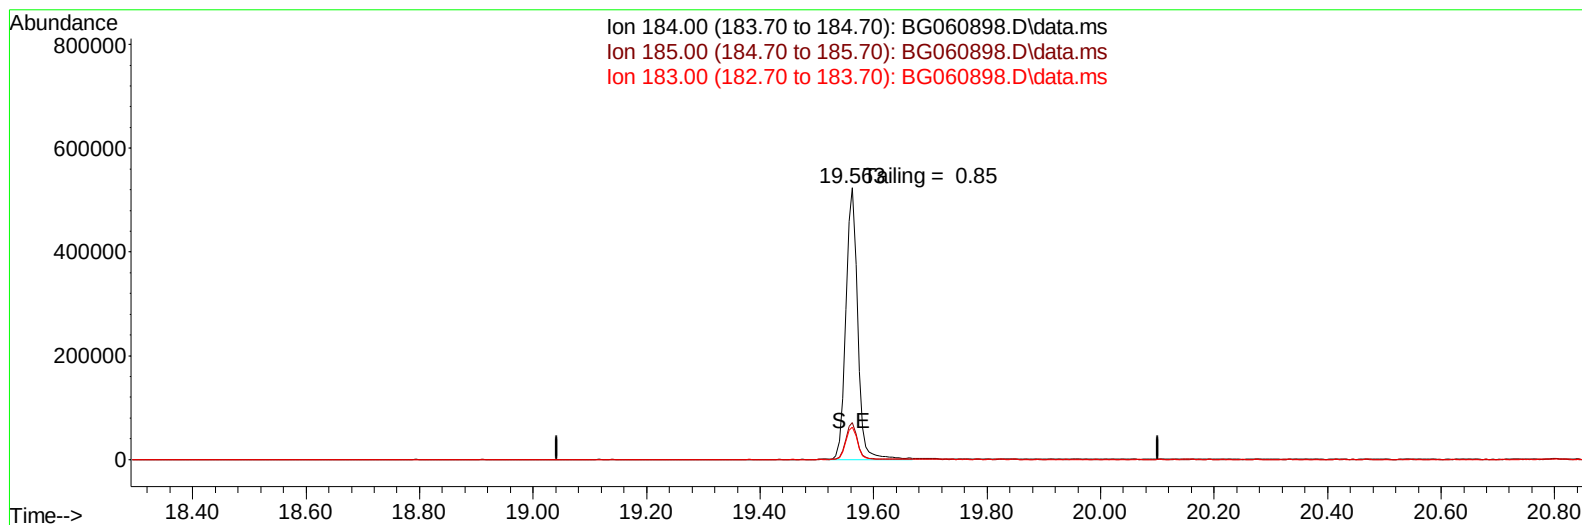

TIC: BG060898.D\data.ms

(77) Benzidine

19.571min (-19.571) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.70	0.00#
183.00	11.90	0.00#
0.00	0.00	0.00