

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
 Data File : BG060906.D
 Acq On : 15 Apr 2024 18:31
 Operator : MA/JU
 Sample : P2091-01DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OR-02-041124DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.096	12	18	27	rBV6	22404	70607	2.68%	0.256%
2	3.185	27	33	41	rVB6	12291	29136	1.11%	0.106%
3	5.535	427	433	441	rBV	83183	137645	5.23%	0.499%
4	7.109	694	701	709	rVB	80395	144281	5.48%	0.523%
5	7.950	837	844	851	rBV	257680	420488	15.97%	1.523%
6	9.101	1034	1040	1046	rBV	55367	96635	3.67%	0.350%
7	10.746	1312	1320	1325	rBV	324781	586429	22.27%	2.124%
8	10.793	1325	1328	1334	rVB	78616	123687	4.70%	0.448%
9	12.403	1596	1602	1609	rBV	76592	123902	4.70%	0.449%
10	12.621	1629	1639	1648	rVB	51612	85655	3.25%	0.310%
11	13.196	1730	1737	1744	rBV	131234	198589	7.54%	0.719%
12	13.414	1768	1774	1780	rBV2	19811	30216	1.15%	0.109%
13	13.743	1822	1830	1831	rBV	26448	40355	1.53%	0.146%
14	13.901	1849	1857	1861	rBV	41289	72876	2.77%	0.264%
15	13.954	1861	1866	1871	rVB	29073	43472	1.65%	0.157%
16	14.136	1892	1897	1900	rBV2	20045	30880	1.17%	0.112%
17	14.301	1917	1925	1931	rBV	25344	41605	1.58%	0.151%
18	14.577	1962	1972	1978	rBV	526977	836285	31.75%	3.029%
19	14.642	1978	1983	1990	rVB	176835	281375	10.68%	1.019%
20	14.789	2000	2008	2018	rBV6	13103	34232	1.30%	0.124%
21	14.977	2034	2040	2046	rVV	147969	227274	8.63%	0.823%
22	15.059	2046	2054	2060	rVB	17351	30246	1.15%	0.110%
23	15.194	2070	2077	2083	rBV5	15511	26957	1.02%	0.098%
24	15.623	2144	2150	2160	rVB	292290	432892	16.44%	1.568%
25	15.787	2175	2178	2183	rVB2	31865	46571	1.77%	0.169%
26	15.923	2196	2201	2208	rVB	48277	80454	3.05%	0.291%
27	16.064	2216	2225	2234	rBV3	159922	276551	10.50%	1.002%
28	16.299	2261	2265	2276	rVB10	15157	35519	1.35%	0.129%
29	16.628	2309	2321	2326	rBV3	47074	111278	4.23%	0.403%
30	16.681	2326	2330	2335	rVB4	20947	34447	1.31%	0.125%
31	16.775	2342	2346	2351	rVB4	20174	36597	1.39%	0.133%
32	16.863	2351	2361	2364	rBV6	17990	47053	1.79%	0.170%
33	17.057	2390	2394	2400	rBV2	24838	51823	1.97%	0.188%
34	17.145	2404	2409	2419	rVB	85955	140204	5.32%	0.508%
35	17.327	2434	2440	2443	rBV	636266	1019727	38.72%	3.694%
36	17.368	2443	2447	2453	rVV	1562312	2220958	84.33%	8.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
 Data File : BG060906.D
 Acq On : 15 Apr 2024 18:31
 Operator : MA/JU
 Sample : P2091-01DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OR-02-041124DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.456	2453	2462	2468	rVV	570178	853710	32.41%	3.093%
38	17.515	2468	2472	2477	rVV5	22112	37601	1.43%	0.136%
39	17.721	2498	2507	2512	rBV	97459	171123	6.50%	0.620%
40	17.844	2524	2528	2533	rBV	28860	40233	1.53%	0.146%
41	17.903	2535	2538	2544	rVB4	19931	32567	1.24%	0.118%
42	18.008	2549	2556	2559	rVV	63816	89401	3.39%	0.324%
43	18.050	2559	2563	2568	rVB2	14884	28244	1.07%	0.102%
44	18.202	2583	2589	2593	rBV	143160	233640	8.87%	0.846%
45	18.249	2593	2597	2603	rVB	199445	315683	11.99%	1.144%
46	18.332	2604	2611	2616	rBV	104891	166609	6.33%	0.604%
47	18.396	2616	2622	2626	rVV2	281358	498515	18.93%	1.806%
48	18.431	2626	2628	2635	rVB	88696	118878	4.51%	0.431%
49	18.537	2643	2646	2653	rVB4	16508	27312	1.04%	0.099%
50	18.702	2669	2674	2678	rBV	114379	160639	6.10%	0.582%
51	18.737	2678	2680	2685	rVB6	24333	30172	1.15%	0.109%
52	18.948	2713	2716	2721	rVB	31138	38875	1.48%	0.141%
53	19.001	2721	2725	2727	rBV	31701	40065	1.52%	0.145%
54	19.031	2727	2730	2735	rVB2	33851	48405	1.84%	0.175%
55	19.113	2739	2744	2746	rBV2	71663	106213	4.03%	0.385%
56	19.148	2746	2750	2753	rVV	210631	260386	9.89%	0.943%
57	19.184	2753	2756	2759	rVB2	159541	186478	7.08%	0.676%
58	19.254	2764	2768	2776	rBV5	39332	87114	3.31%	0.316%
59	19.313	2776	2778	2783	rVB2	36920	43844	1.66%	0.159%
60	19.383	2783	2790	2797	rBV	1797805	2618006	99.40%	9.484%
61	19.618	2827	2830	2834	rVB	50395	70772	2.69%	0.256%
62	19.742	2841	2851	2859	rBV	1413591	2633717	100.00%	9.541%
63	19.818	2860	2864	2870	rVB2	65322	113559	4.31%	0.411%
64	19.918	2877	2881	2882	rBV	95029	108164	4.11%	0.392%
65	19.947	2882	2886	2889	rVB	219877	295866	11.23%	1.072%
66	20.071	2900	2907	2912	rBV3	94491	247747	9.41%	0.897%
67	20.200	2925	2929	2930	rBV4	55275	67791	2.57%	0.246%
68	20.235	2931	2935	2940	rVB	329956	452853	17.19%	1.640%
69	20.335	2947	2952	2956	rBV	341292	455713	17.30%	1.651%
70	20.394	2956	2962	2966	rVV2	131092	219112	8.32%	0.794%
71	20.535	2982	2986	2989	rBV	59512	84544	3.21%	0.306%
72	20.576	2989	2993	2997	rVV2	67939	105157	3.99%	0.381%
73	21.175	3091	3095	3098	rBV	86962	127265	4.83%	0.461%
74	21.216	3099	3102	3106	rVV	98995	129898	4.93%	0.471%
75	21.263	3106	3110	3115	rVB2	97191	178308	6.77%	0.646%
76	21.575	3156	3163	3169	rBV4	986891	2421488	91.94%	8.772%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060906.D
Acq On : 15 Apr 2024 18:31
Operator : MA/JU
Sample : P2091-01DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-041124DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.634	3169	3173	3182	rVB	634290	1059682	40.24%	3.839%
78	21.780	3194	3198	3204	rBV	155935	229870	8.73%	0.833%
79	21.980	3229	3232	3241	rVB3	90585	158026	6.00%	0.572%
80	23.737	3523	3531	3538	rBV2	401471	1320334	50.13%	4.783%
81	24.430	3643	3649	3662	rVB	232402	675707	25.66%	2.448%
82	24.571	3666	3673	3682	rVV	366006	929734	35.30%	3.368%
83	24.724	3691	3699	3706	rBV2	385754	1039618	39.47%	3.766%


Sum of corrected areas: 27605539

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060906.D
Acq On : 15 Apr 2024 18:31
Operator : MA/JU
Sample : P2091-01DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-041124DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

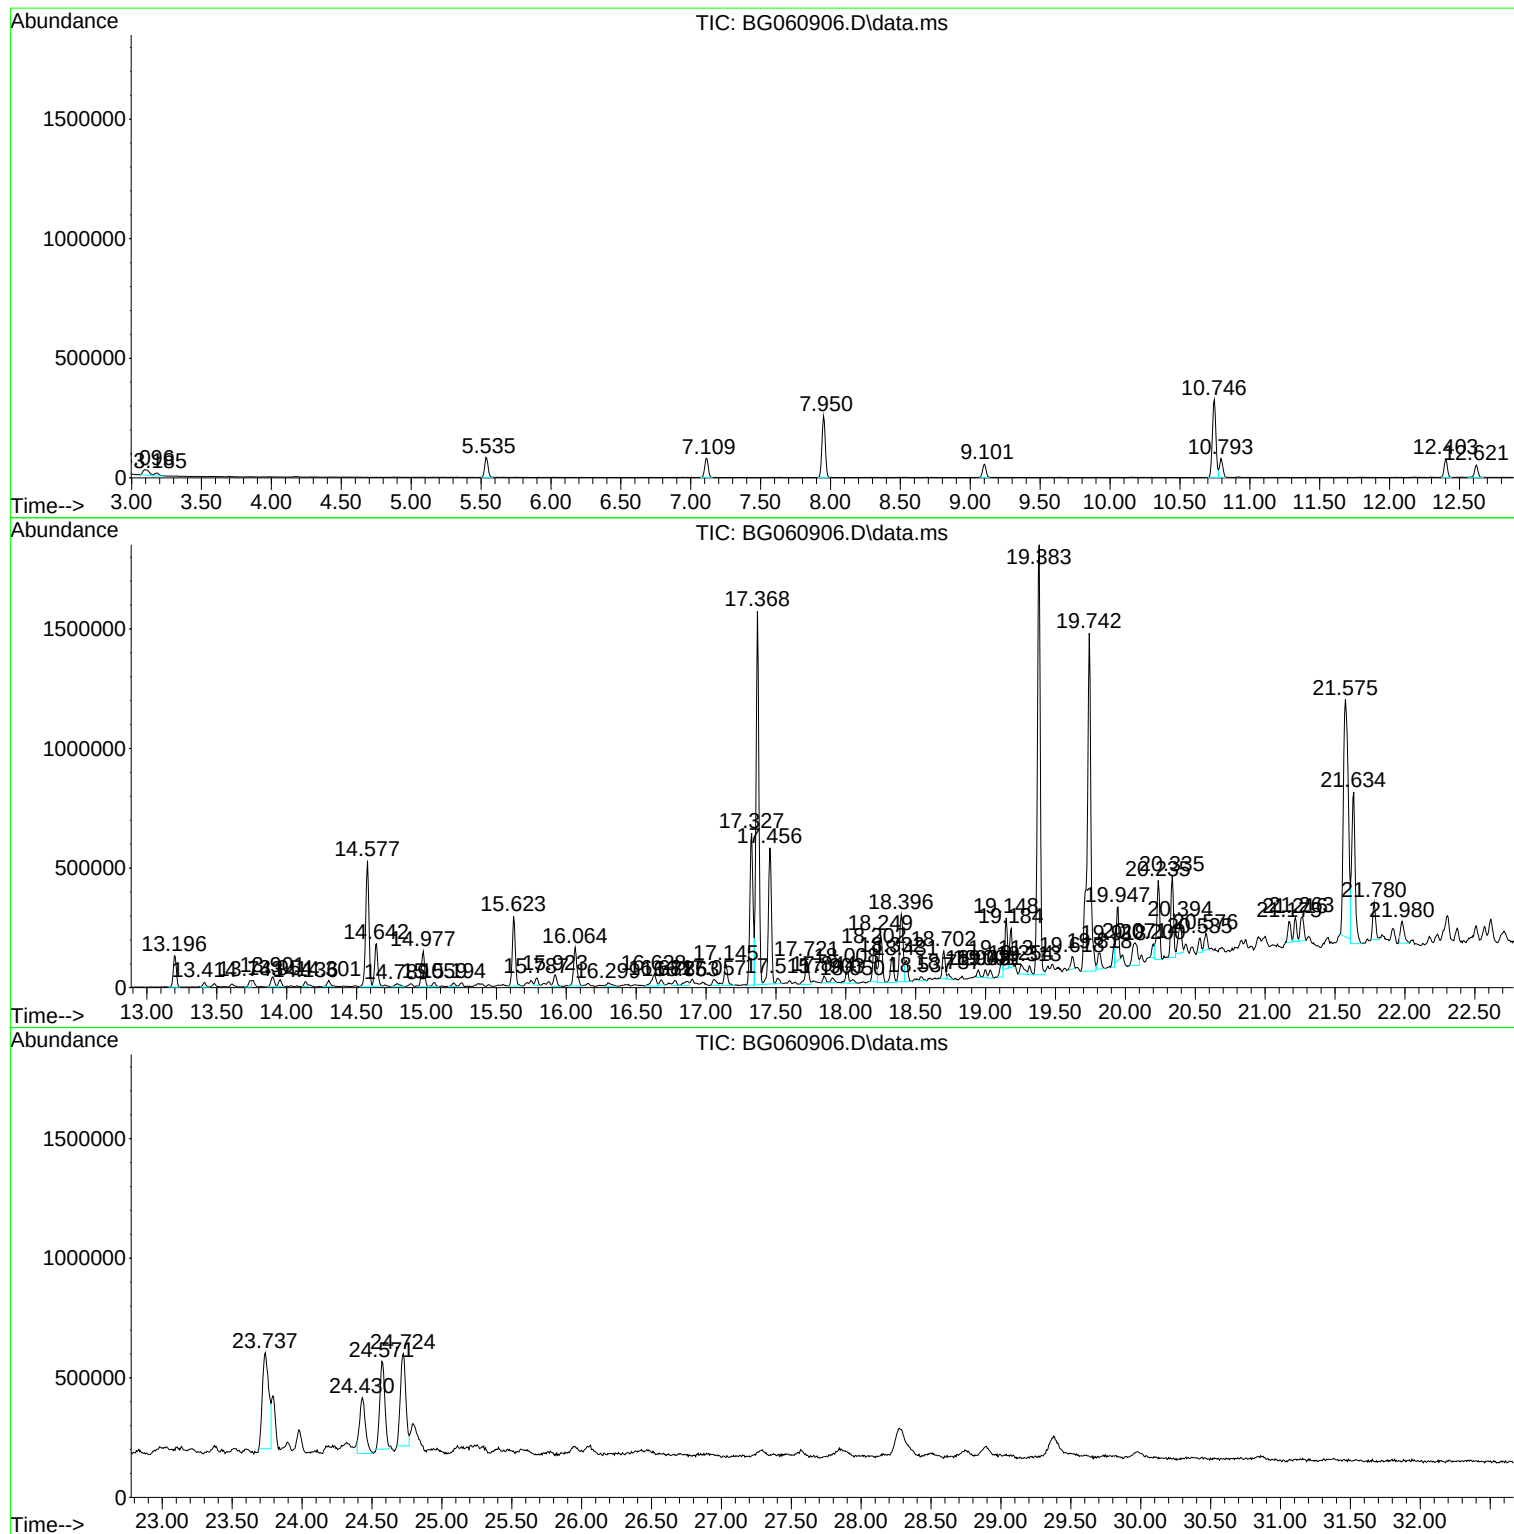

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060906.D
Acq On : 15 Apr 2024 18:31
Operator : MA/JU
Sample : P2091-01DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-041124DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060906.D
Acq On : 15 Apr 2024 18:31
Operator : MA/JU
Sample : P2091-01DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OR-02-041124DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------