


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060898.D
Acq On : 15 Apr 2024 10:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

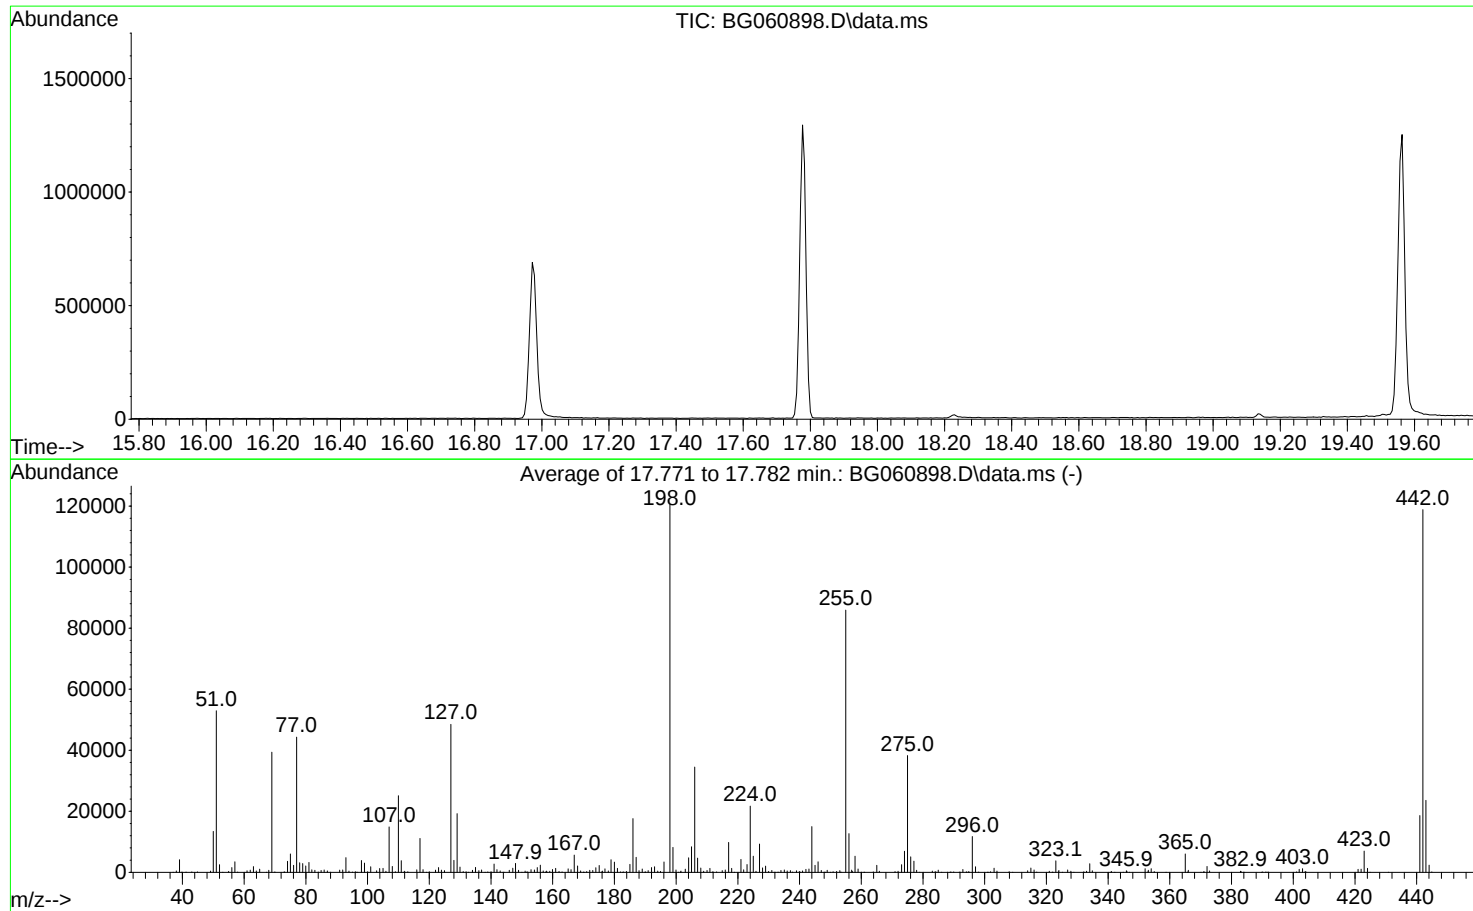




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	52947	PASS
68	69	0.00	2	1.7	684	PASS
69	198	0.00	100	32.7	39365	PASS
70	69	0.00	2	0.4	173	PASS
127	198	10	80	40.2	48504	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120509	PASS
199	198	5	9	6.8	8156	PASS
275	198	10	60	31.7	38240	PASS
365	198	1	100	5.0	6053	PASS
441	198	0.01	100	15.4	18592	PASS
442	442	50	100	100.0	118843	PASS
443	442	15	24	19.9	23608	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060898.D
Acq On : 15 Apr 2024 10:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 16 03:52:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

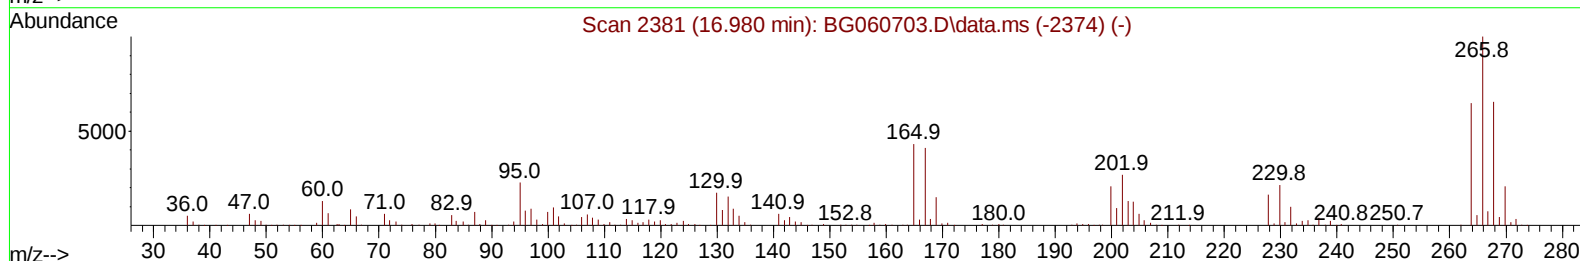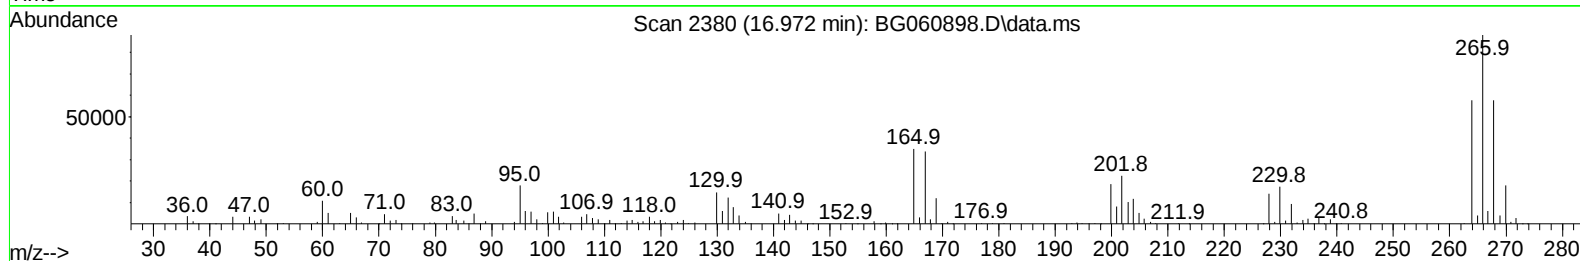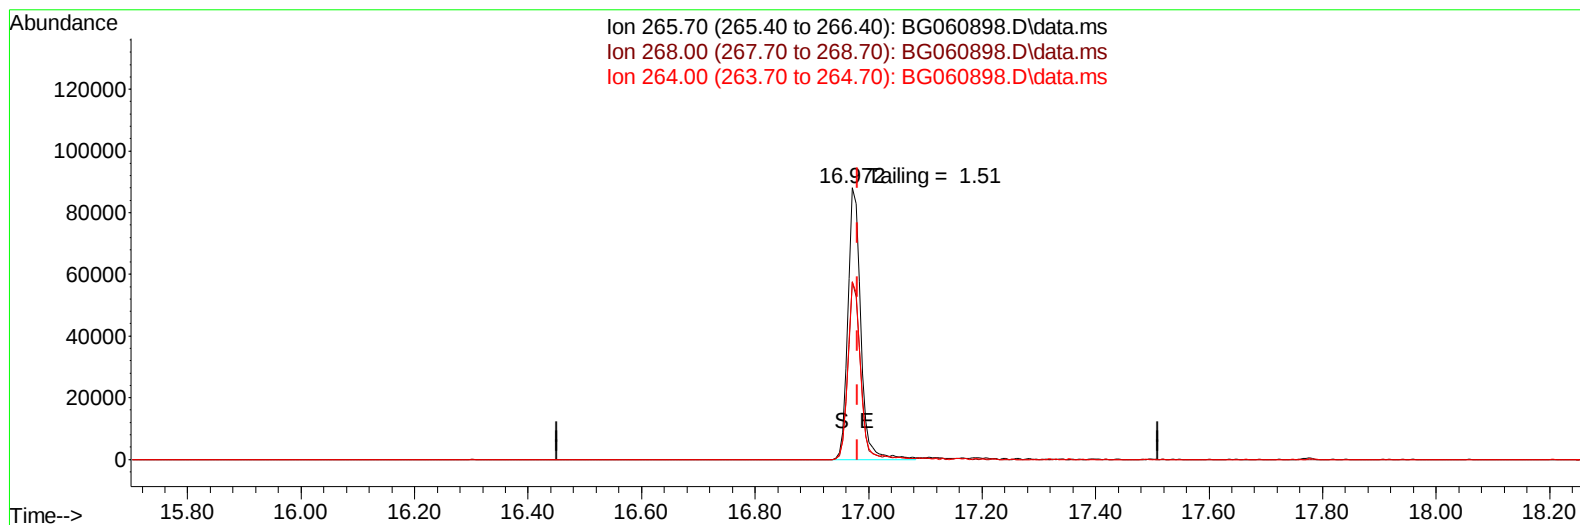

TIC: BG060898.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.009) 20970.05 ng




response 138419

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.40
264.00	64.70	65.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041524\
Data File : BG060898.D
Acq On : 15 Apr 2024 10:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 16 03:52:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

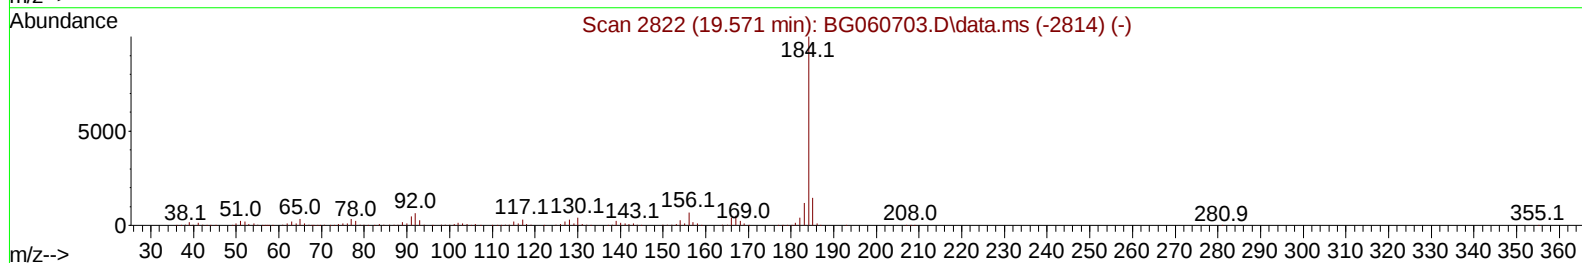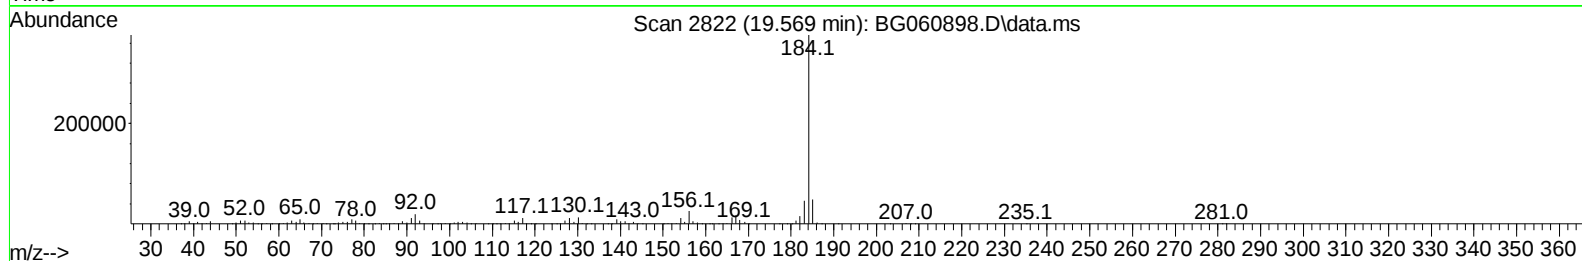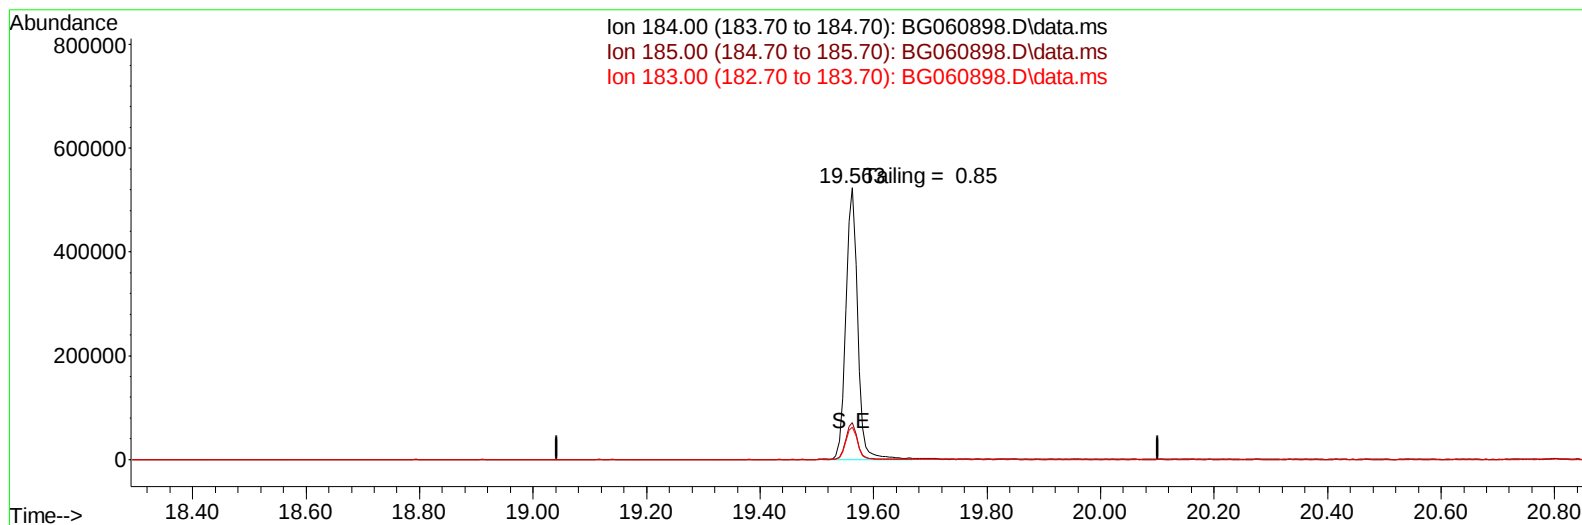

TIC: BG060898.D\data.ms

(77) Benzidine

19.571min (-19.571) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.70	0.00#
183.00	11.90	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/15/2024	BNA_G	<u>BG060898.D</u>
Compound Name	Response	Retention Time
DDT	410098	20.802
DDD	15413	20.362
DDE	3115	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18528	428626	4.32

Instrument :
BNA_G
ClientSampleId :
DFTPP