


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041615\
 Data File : BG016473.D
 Acq On : 17 Apr 2015 2:46
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 17 03:57:14 2015

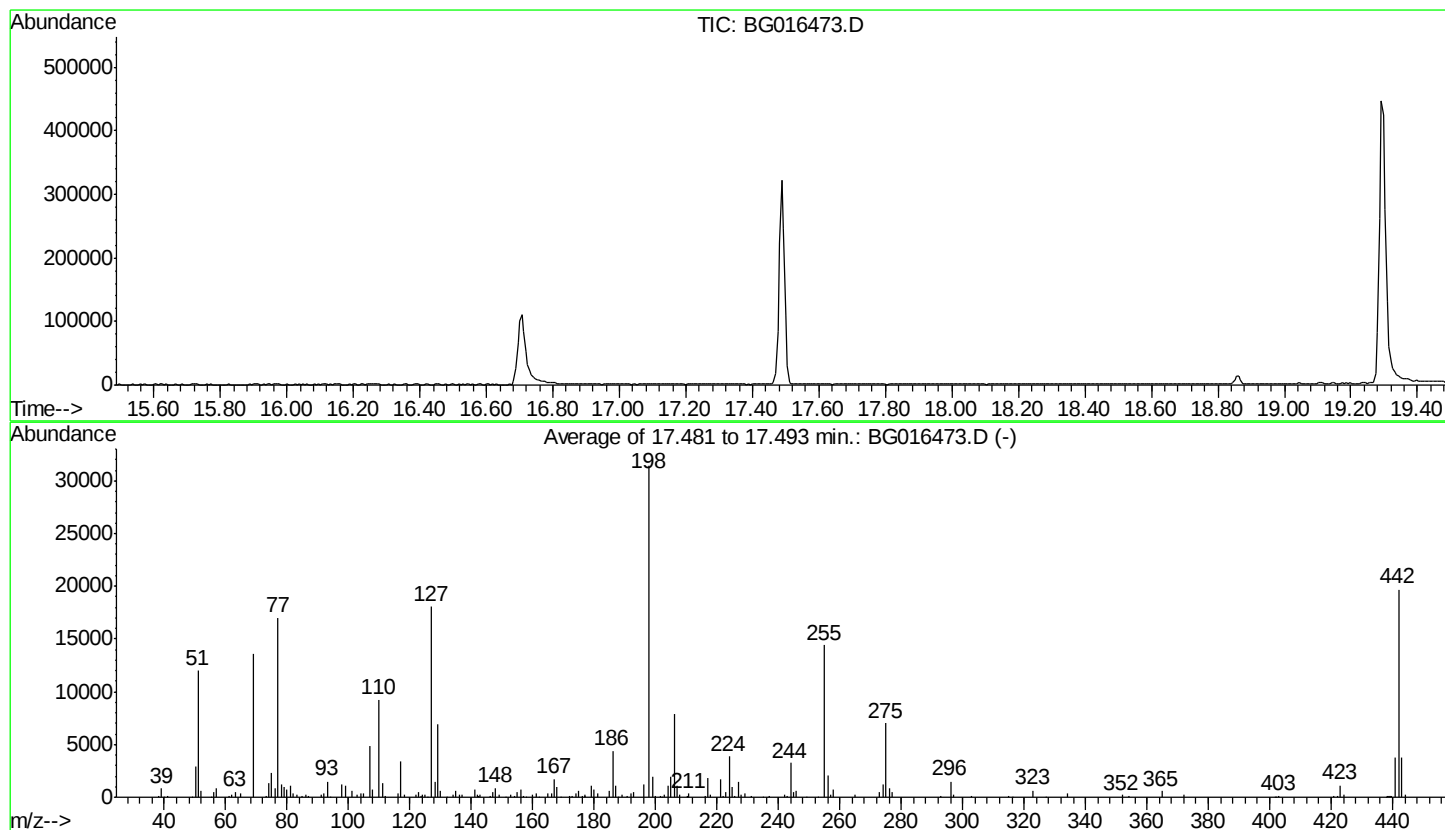

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	11963	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.1	13534	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.5	18070	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31434	PASS
199	198	5	9	6.4	1998	PASS
275	198	10	60	22.2	6987	PASS
365	198	1	100	1.8	572	PASS
441	442	0.01	24	19.0	3742	PASS
442	198	50	100	62.6	19672	PASS
443	442	15	24	18.9	3727	PASS