
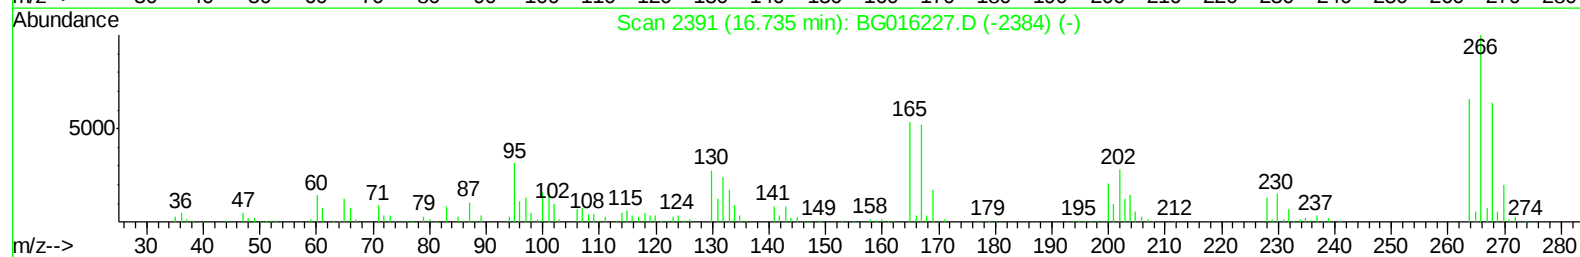
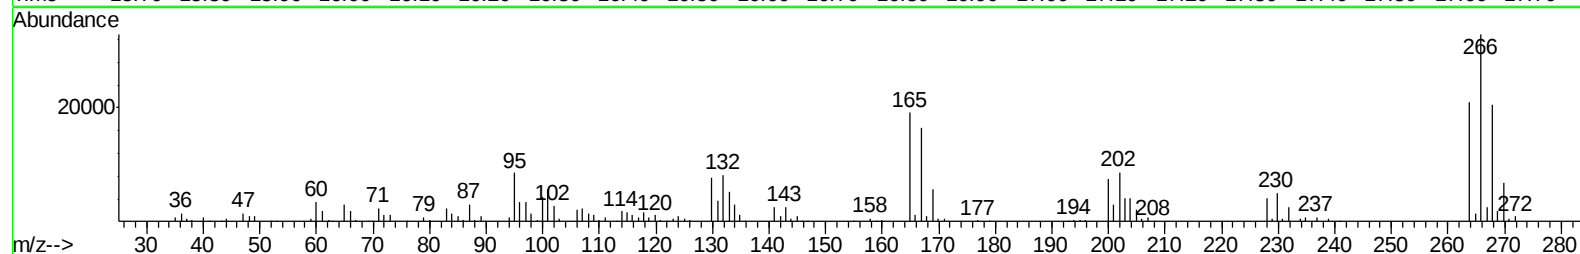


Data Path : Z:\HPCHEM1\BNA_G\Data\BG041615\
Data File : BG016456.D
Acq On : 16 Apr 2015 13:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 08:49:00 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 14:00:56 2015
Response via : Initial Calibration

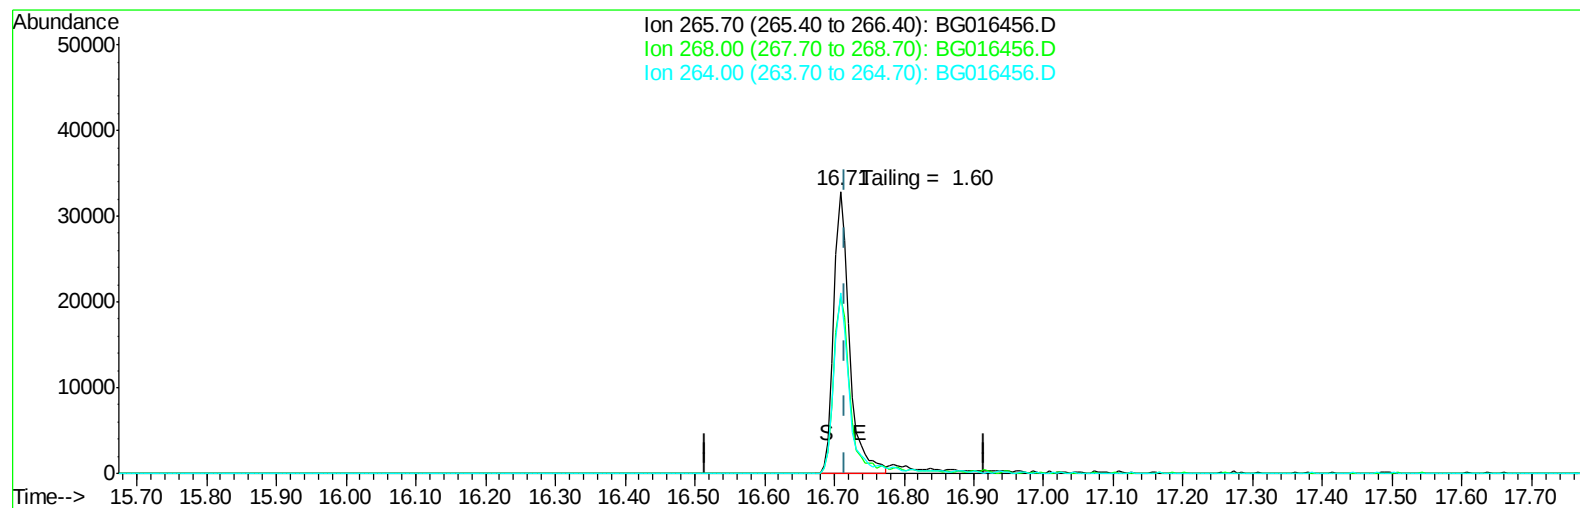

TIC: BG016456.D

(69) Pentachlorophenol (C)




16.708min (-0.007) 161020.18ng

response 51403

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.76
264.00	66.00	63.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG041615\
Data File : BG016456.D
Acq On : 16 Apr 2015 13:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 08:49:00 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 14 14:00:56 2015
Response via : Initial Calibration

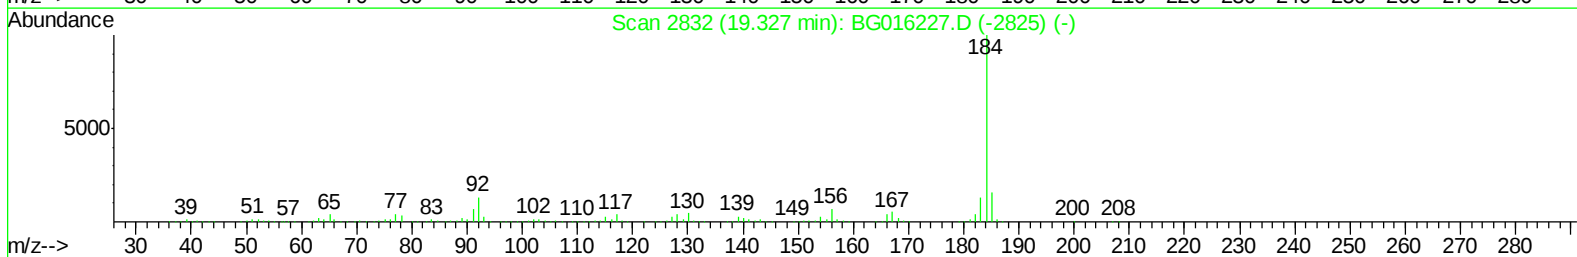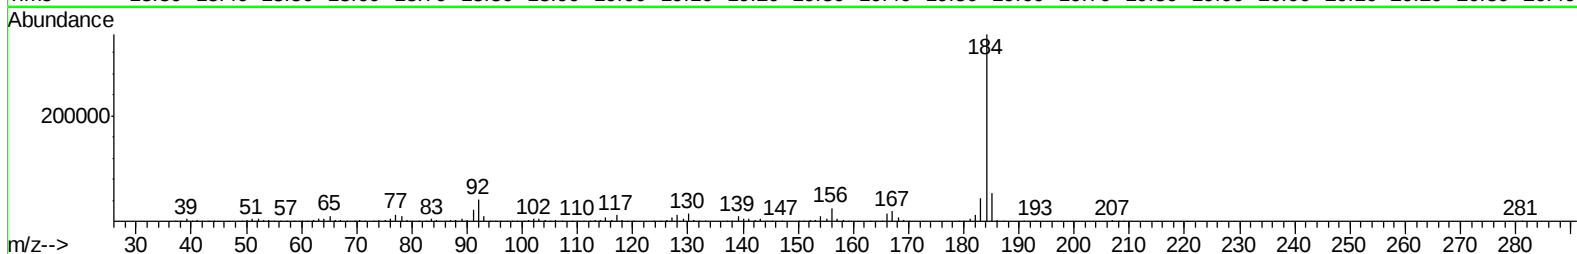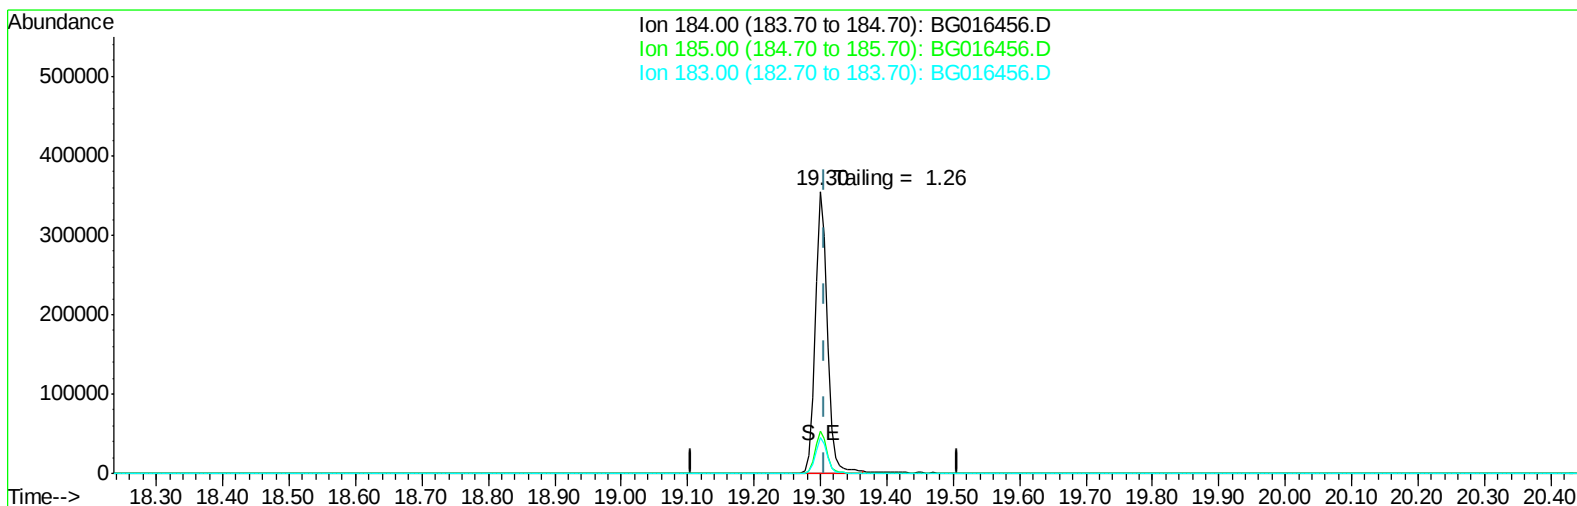

TIC: BG016456.D

(76) Benzidine

19.299min (-0.007) 167089.99ng

response 460580

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.79
183.00	13.00	12.70
0.00	0.00	0.00