
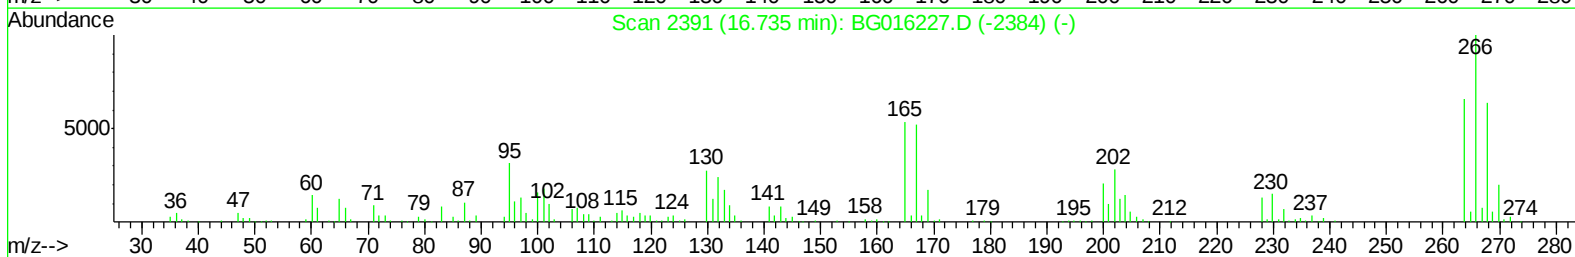
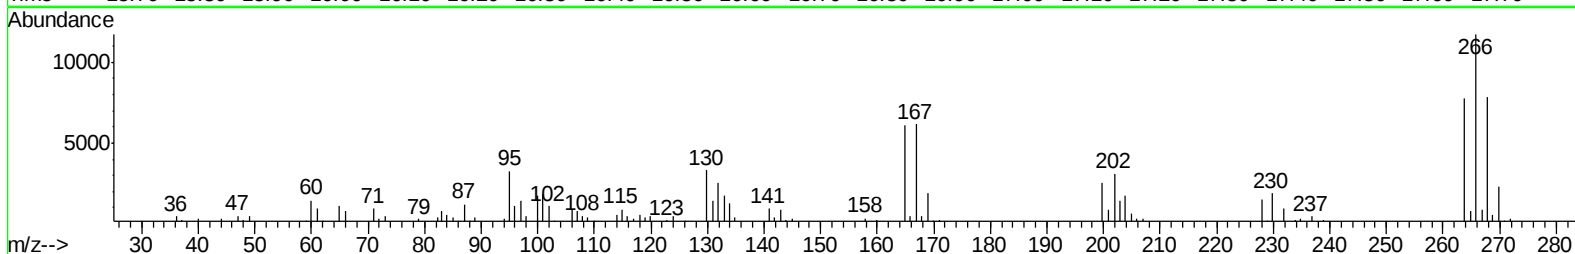


Data Path : Z:\HPCHEM1\BNA\_G\Data\BG041615\  
Data File : BG016473.D  
Acq On : 17 Apr 2015 2:46  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 08:56:30 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG040615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 14 14:00:56 2015  
Response via : Initial Calibration

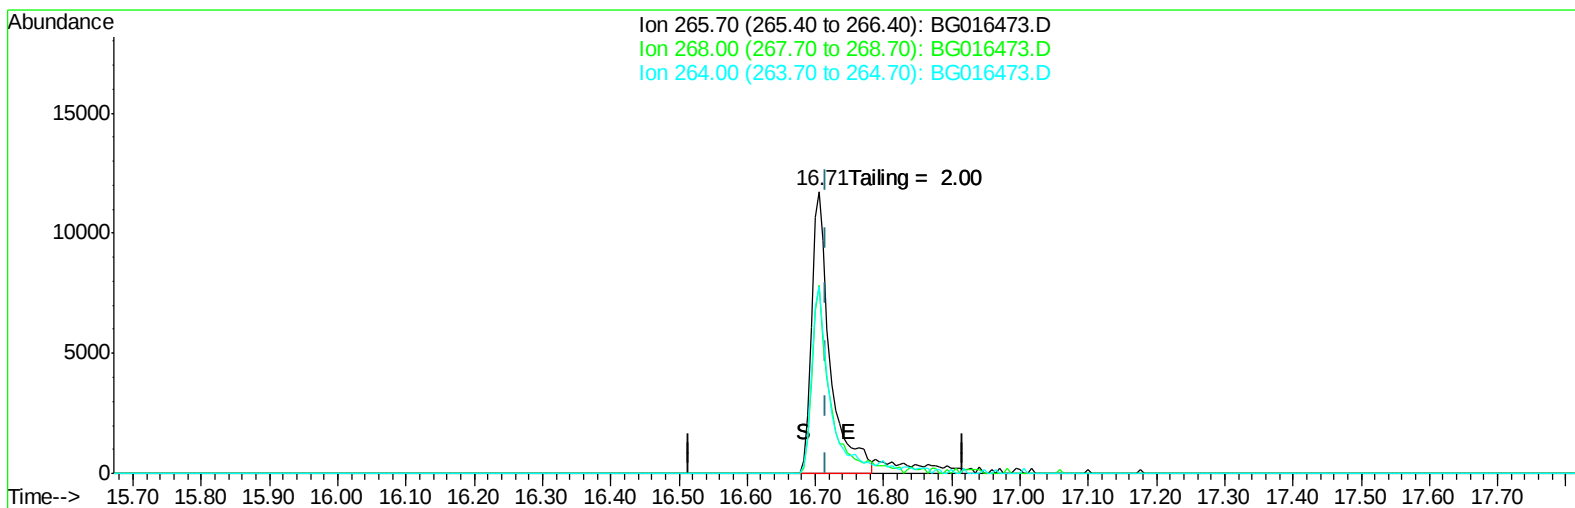

TIC: BG016473.D

(69) Pentachlorophenol (C)




16.706min (-0.010) 0.00ng

response 23287

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.60 | 66.82 |
| 264.00 | 66.00 | 66.48 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\Data\BG041615\  
Data File : BG016473.D  
Acq On : 17 Apr 2015 2:46  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 08:56:30 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG040615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 14 14:00:56 2015  
Response via : Initial Calibration

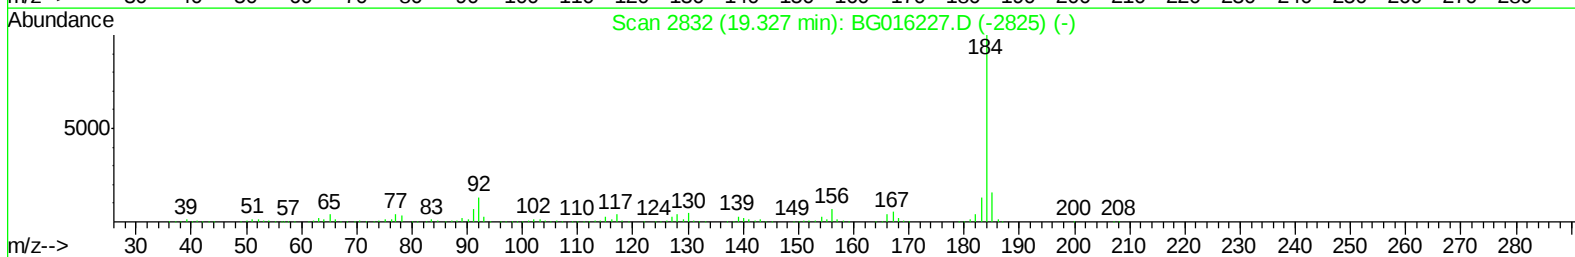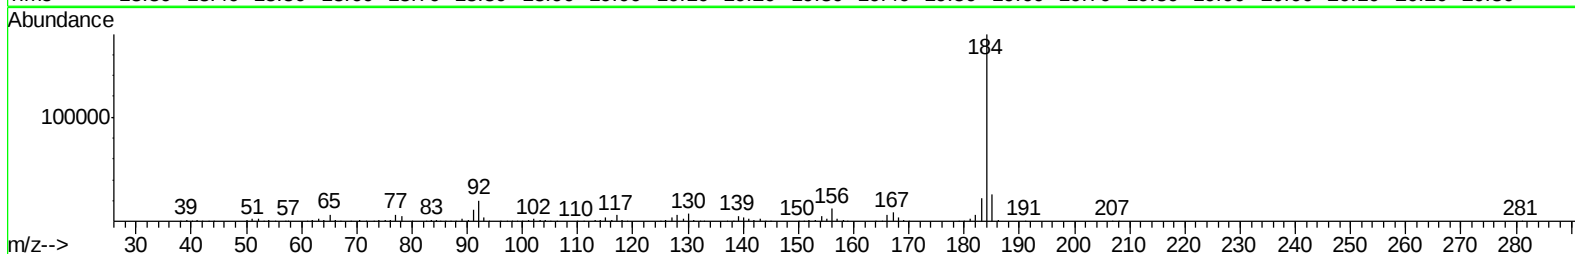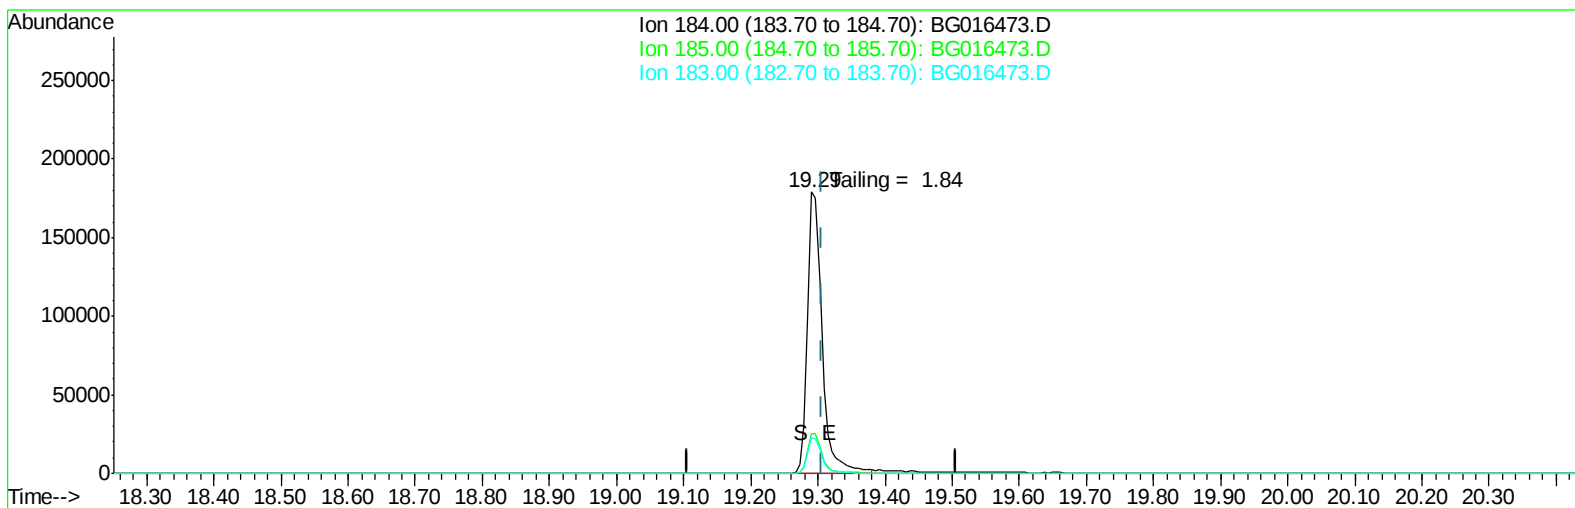

TIC: BG016473.D

(76) Benzidine

19.291min (-0.016) 22640.60ng

response 269796

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 14.31 |
| 183.00 | 13.00 | 12.67 |
| 0.00   | 0.00  | 0.00  |