
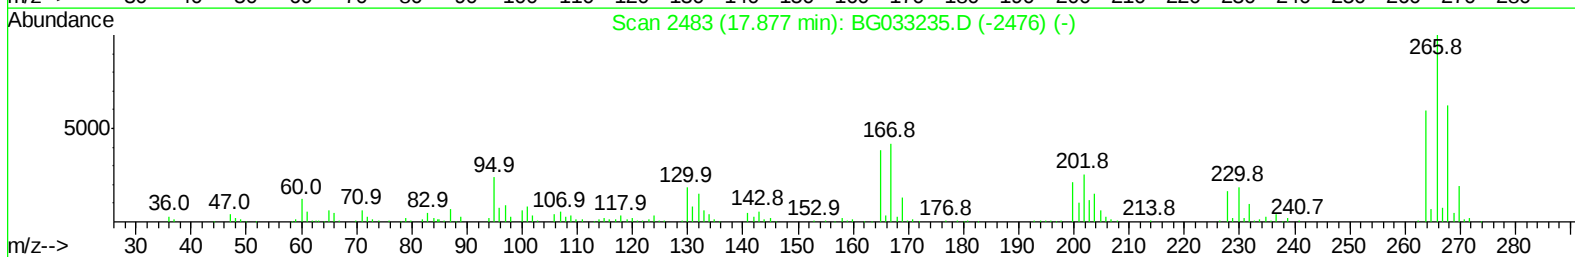
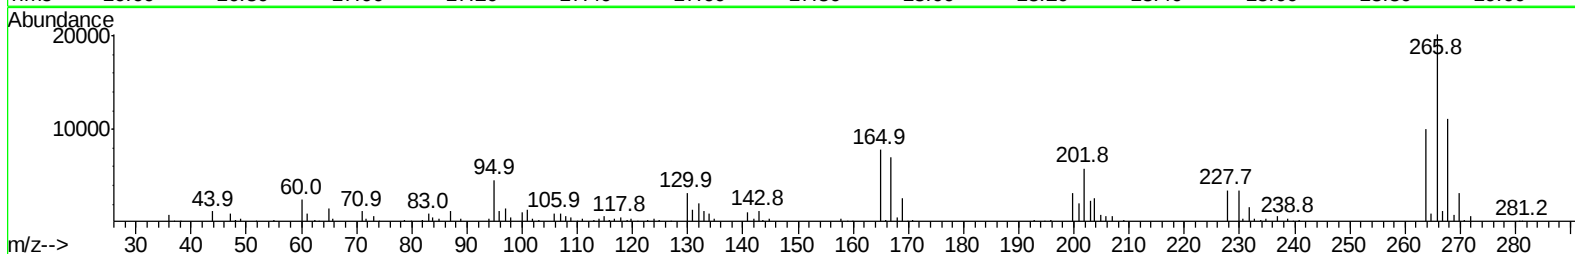


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033808.D
Acq On : 16 Apr 2018 9:56
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:52:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 16 11:44:01 2018
Response via : Initial Calibration

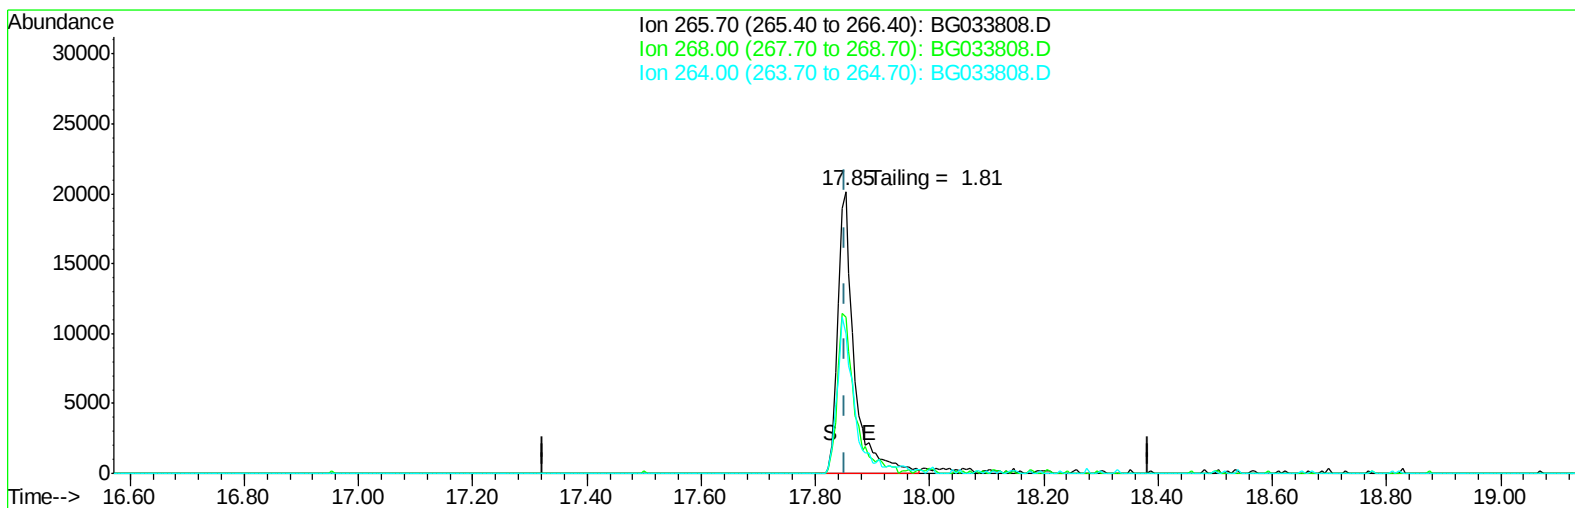

TIC: BG033808.D

(69) Pentachlorophenol (C)




17.852min (-0.001) 15175.49ng

response 40407

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.46
264.00	62.00	49.51#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033808.D
Acq On : 16 Apr 2018 9:56
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:52:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 16 11:44:01 2018
Response via : Initial Calibration

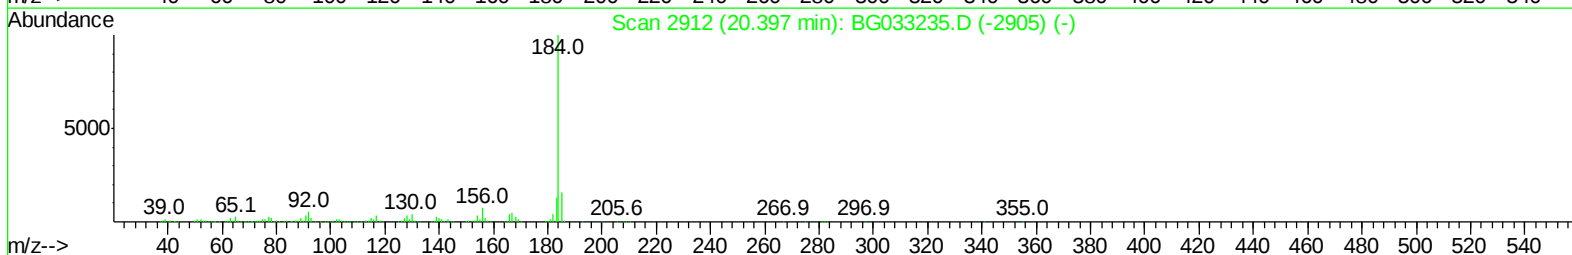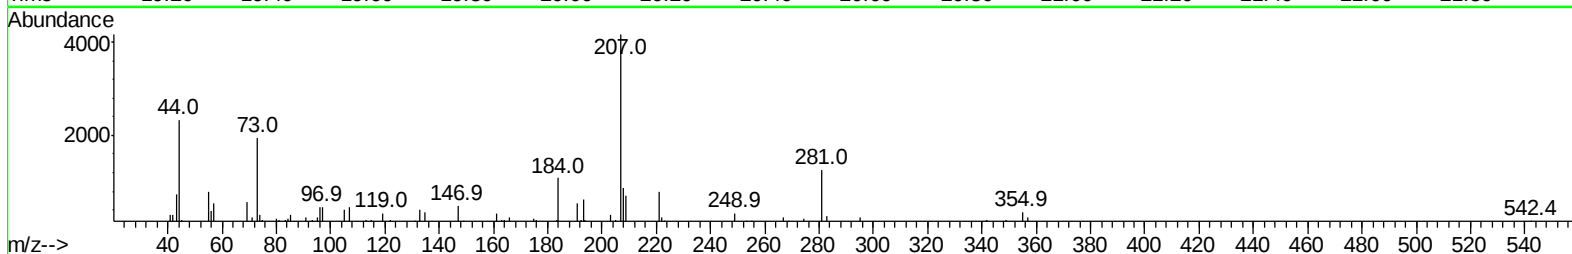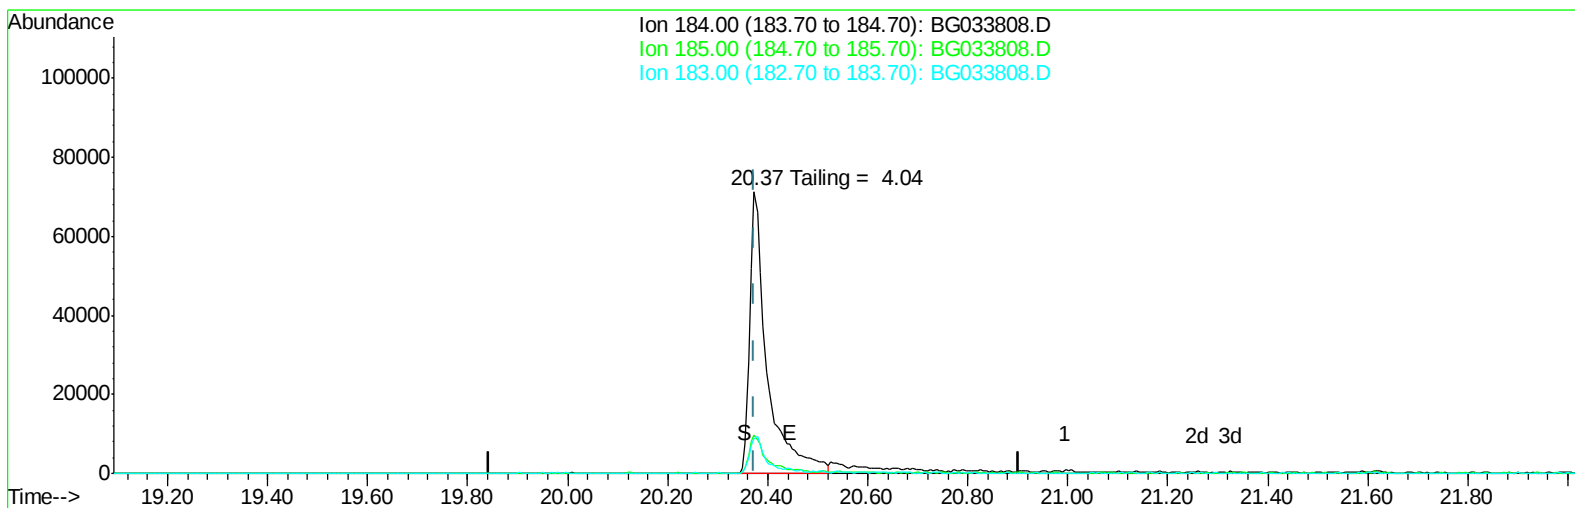

TIC: BG033808.D

(76) Benzidine

20.996min (+0.622) 444.64ng

response 832

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	16.04#
0.00	0.00	0.00