
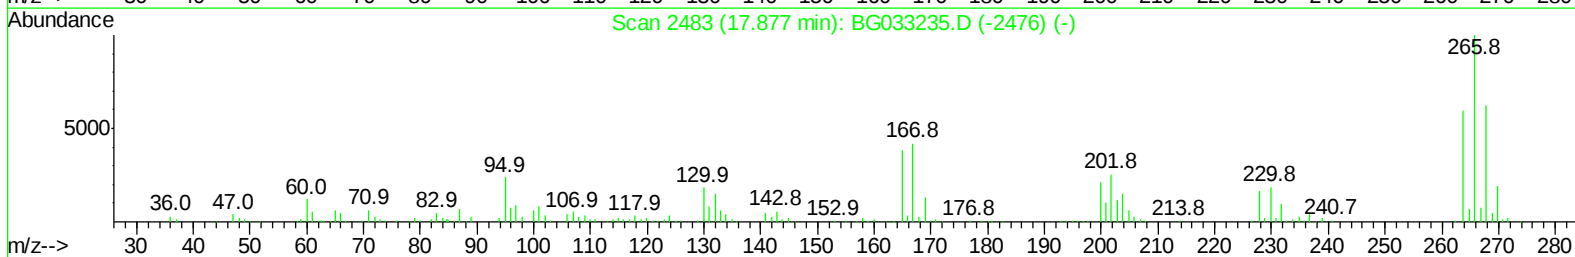
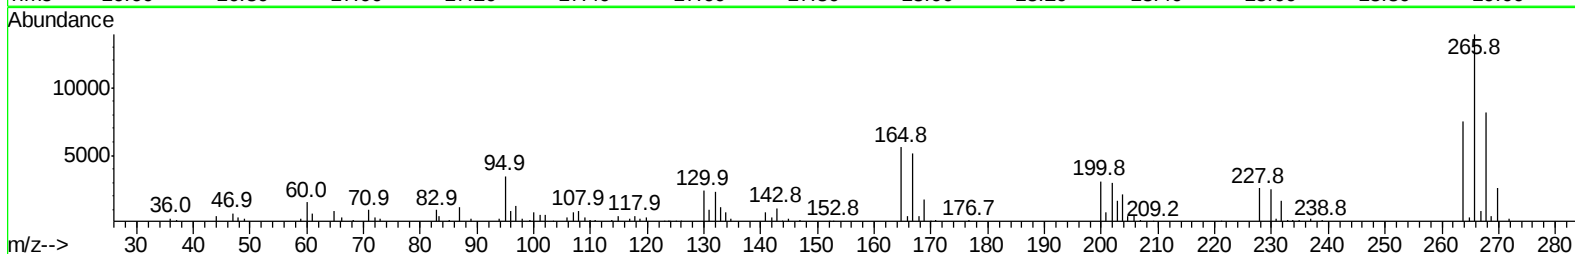


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033827.D
Acq On : 16 Apr 2018 23:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:55:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 16 11:44:01 2018
Response via : Initial Calibration

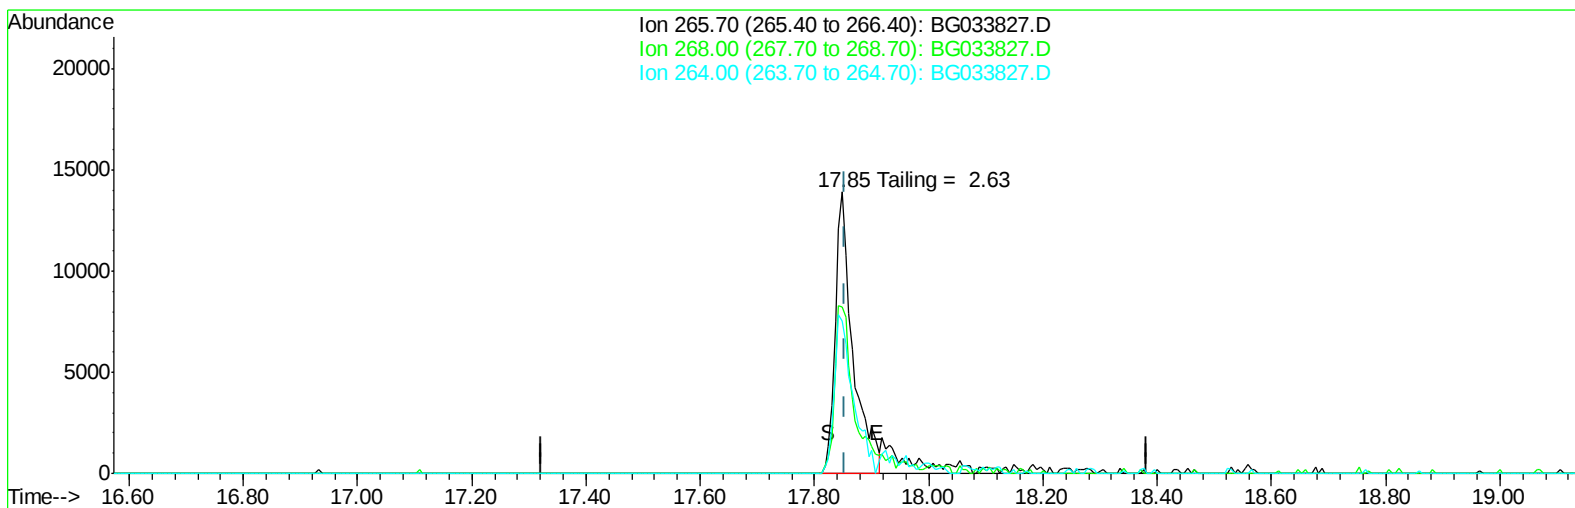

TIC: BG033827.D

(69) Pentachlorophenol (C)




17.848min (-0.005) 27154.55ng

response 29568

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.85
264.00	62.00	53.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033827.D
Acq On : 16 Apr 2018 23:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 05:55:58 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 16 11:44:01 2018
Response via : Initial Calibration

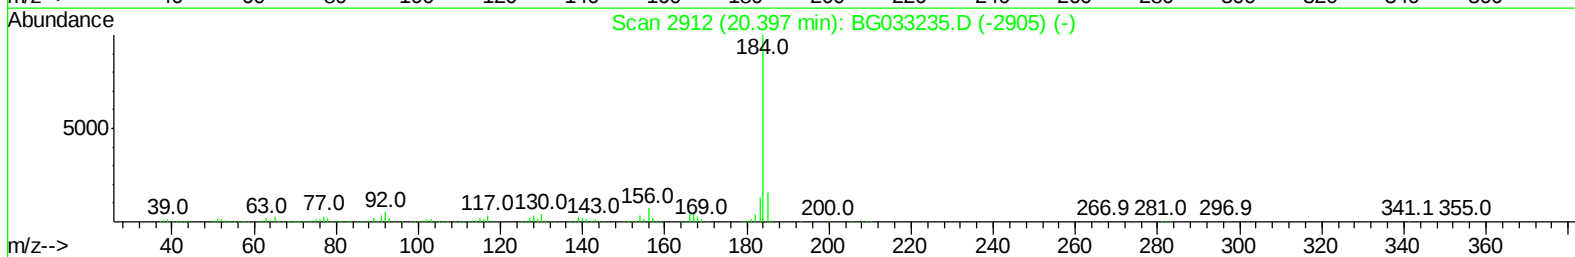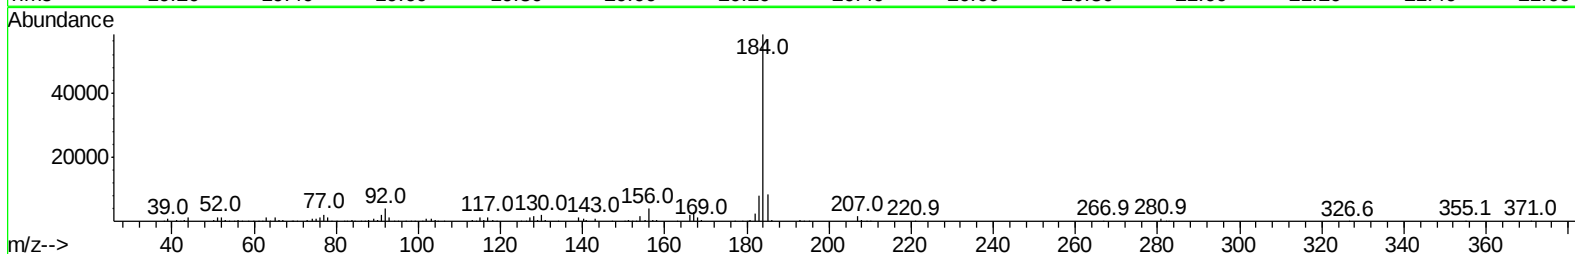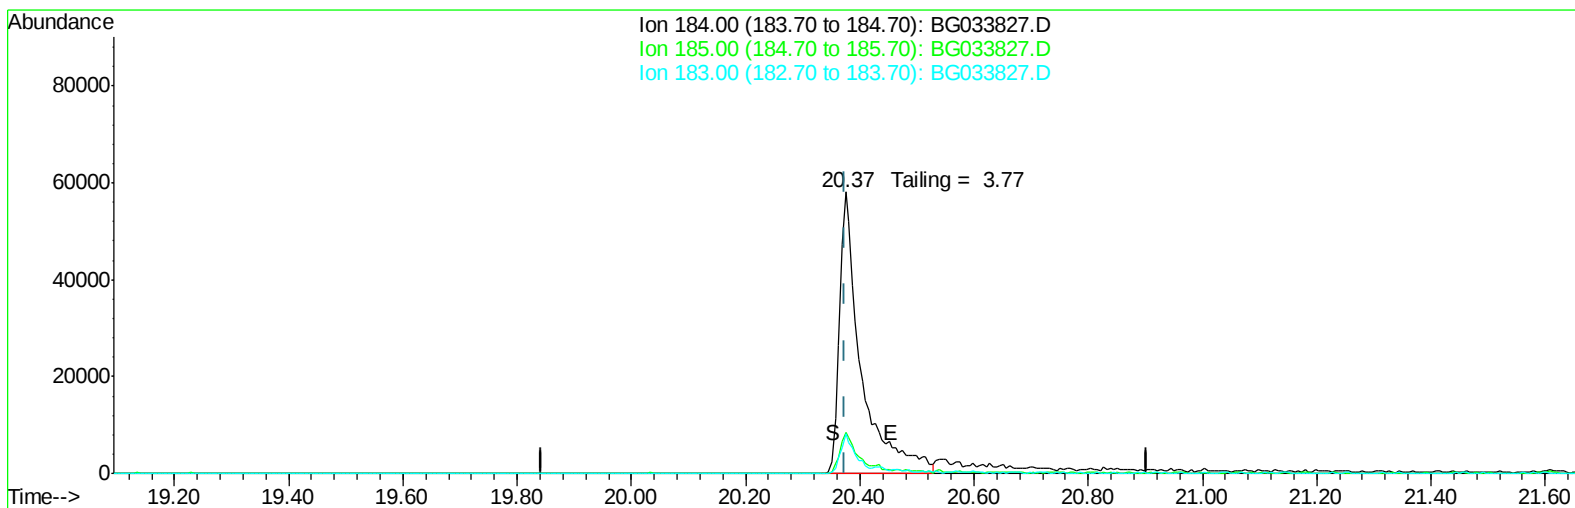

TIC: BG033827.D

(76) Benzidine

20.375min (+0.000) 104657.86ng

response 153261

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.71
183.00	13.30	14.01
0.00	0.00	0.00