

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
 Data File : BG033829.D
 Acq On : 17 Apr 2018 00:24
 Operator : SJ/JU
 Sample : J2391-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 041218-DBRI-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	23	31	39	rBV2	51280	98913	2.57%	0.820%
2	6.296	504	512	525	rBV3	42570	172179	4.48%	1.428%
3	8.370	859	865	877	rBV3	135664	434478	11.31%	3.603%
4	8.858	941	948	959	rBV2	45232	138705	3.61%	1.150%
5	9.181	996	1003	1023	rBV	309934	819274	21.32%	6.794%
6	10.062	1145	1153	1173	rBV2	163983	641479	16.69%	5.320%
7	11.737	1428	1438	1457	rBV2	75634	249362	6.49%	2.068%
8	14.093	1832	1839	1862	rBV	858832	1889274	49.16%	15.668%
9	15.468	2067	2073	2086	rBV3	204817	423172	11.01%	3.509%
10	16.948	2318	2325	2344	rBV	543411	1229197	31.98%	10.194%
11	18.206	2530	2539	2551	rBV2	313282	645995	16.81%	5.357%
12	20.720	2961	2967	2982	rBV	2576171	3843066	100.00%	31.871%
13	22.548	3271	3278	3288	rBV	377856	783176	20.38%	6.495%
14	26.314	3909	3919	3931	rBV3	202505	689830	17.95%	5.721%


Sum of corrected areas: 12058100

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033829.D
Acq On : 17 Apr 2018 00:24
Operator : SJ/JU
Sample : J2391-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-DBRI-F-U-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

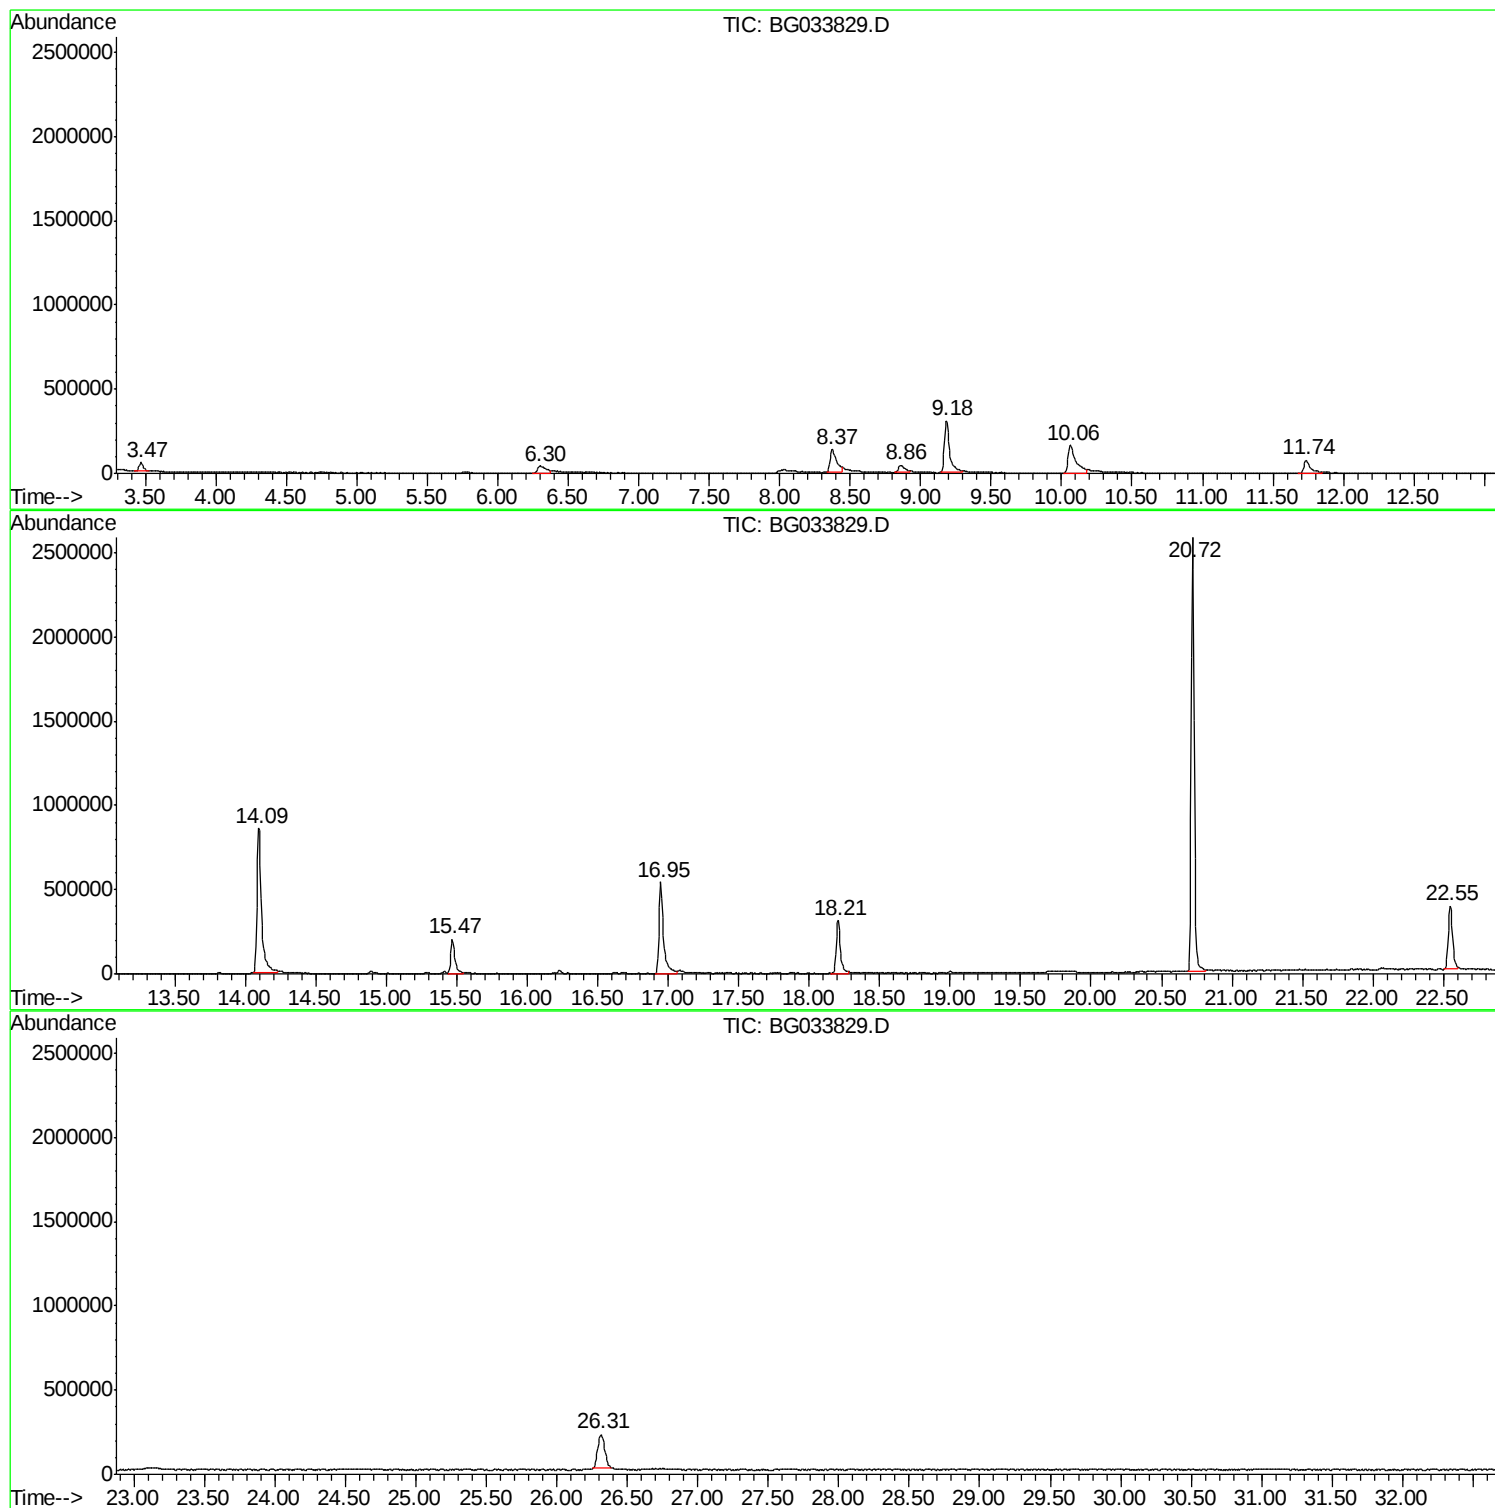

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033829.D
Acq On : 17 Apr 2018 00:24
Operator : SJ/JU
Sample : J2391-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-DBRI-F-U-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.37 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.37	62.65 ng	434478	1,4-Dichlorobenzene-d4	8.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	25
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22

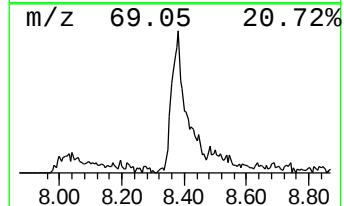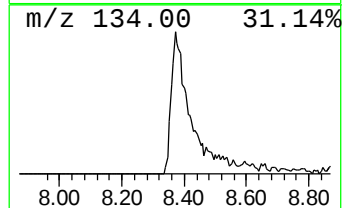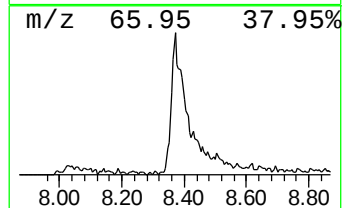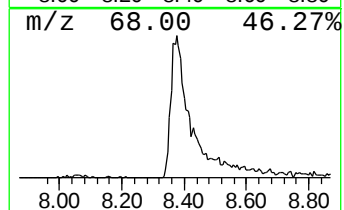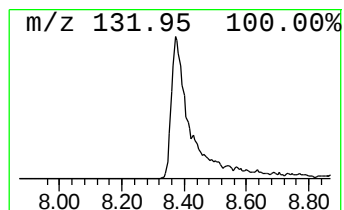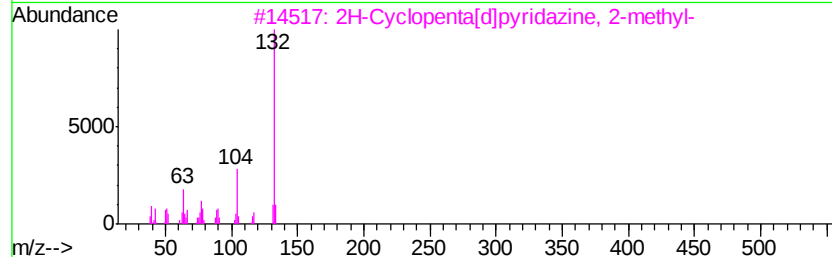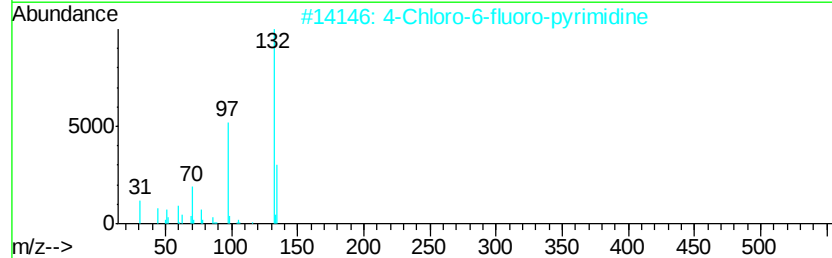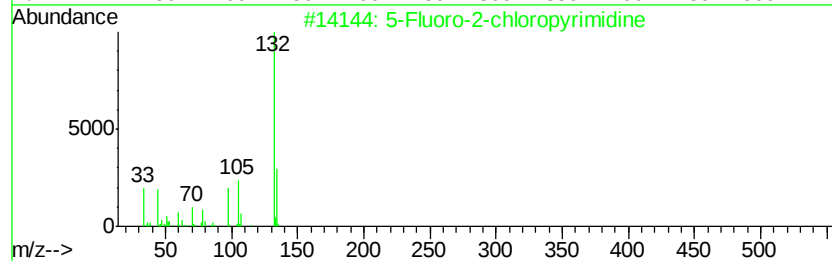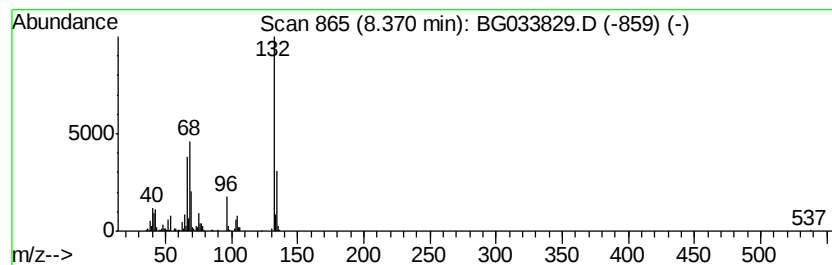

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041618\
Data File : BG033829.D
Acq On : 17 Apr 2018 00:24
Operator : SJ/JU
Sample : J2391-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-DBRI-F-U-M

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.37	8.37	62.6	ng	434478	1	8.86	138705	20.0