

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
 Data File : BG033836.D
 Acq On : 17 Apr 2018 4:47
 Operator : SJ/JU
 Sample : J2391-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 041218-JETB-E-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.464	26	30	43	rVB	52843	116220	2.80%	0.873%
2	6.302	505	513	524	rBV7	33851	141850	3.42%	1.066%
3	8.370	858	865	885	rBV2	135275	506555	12.21%	3.806%
4	8.858	940	948	960	rBV4	43673	152073	3.67%	1.143%
5	9.181	995	1003	1023	rBV2	334873	878420	21.17%	6.601%
6	10.062	1146	1153	1176	rBV2	170260	706564	17.03%	5.309%
7	11.737	1430	1438	1462	rBV	86331	291667	7.03%	2.192%
8	14.093	1833	1839	1860	rBV	926958	2013636	48.53%	15.131%
9	14.892	1967	1975	1988	rBV3	24764	61218	1.48%	0.460%
10	15.468	2067	2073	2091	rBV2	232471	500661	12.07%	3.762%
11	16.948	2317	2325	2344	rBV	601381	1381683	33.30%	10.382%
12	17.083	2344	2348	2355	rVB5	21437	45854	1.11%	0.345%
13	18.206	2532	2539	2550	rBV	329856	714065	17.21%	5.366%
14	20.720	2961	2967	2987	rBV	2737443	4149299	100.00%	31.178%
15	22.548	3271	3278	3292	rBV2	401499	849399	20.47%	6.383%
16	26.314	3908	3919	3936	rBV2	223181	799044	19.26%	6.004%


Sum of corrected areas: 13308208

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033836.D
Acq On : 17 Apr 2018 4:47
Operator : SJ/JU
Sample : J2391-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-JETB-E-U-S

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

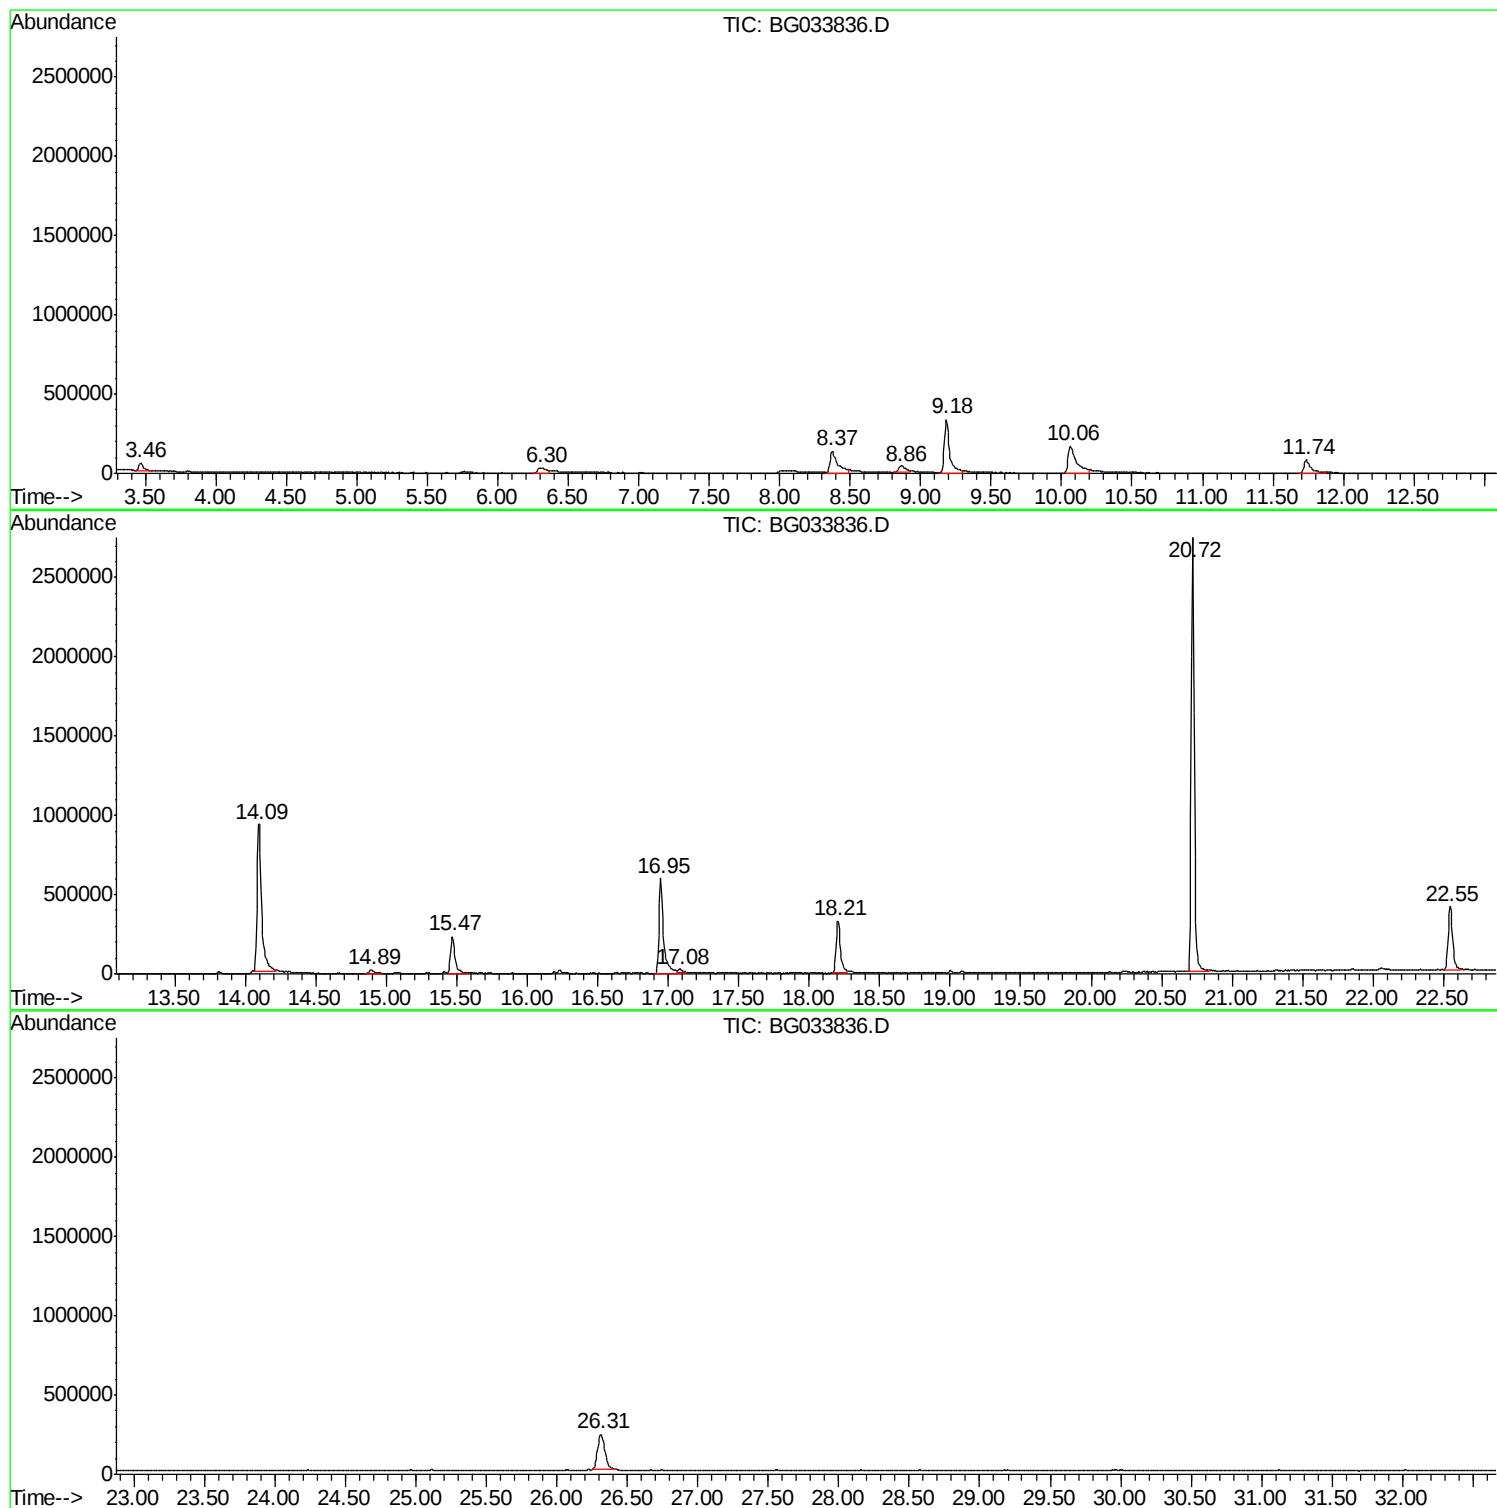

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033836.D
Acq On : 17 Apr 2018 4:47
Operator : SJ/JU
Sample : J2391-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-JETB-E-U-S










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.37 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.37	66.62 ng	506555	1,4-Dichlorobenzene-d4	8.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	14
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

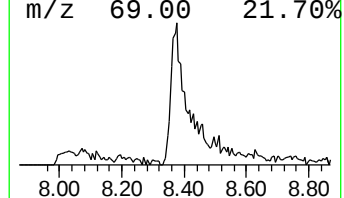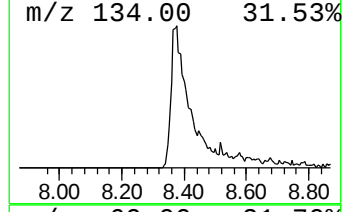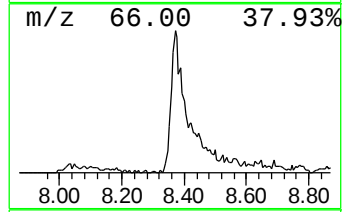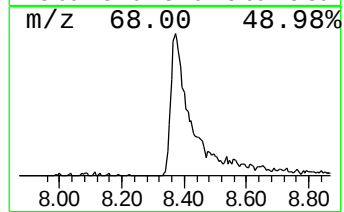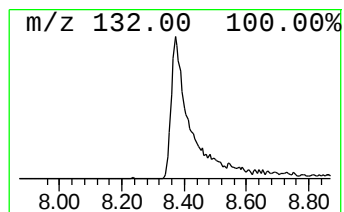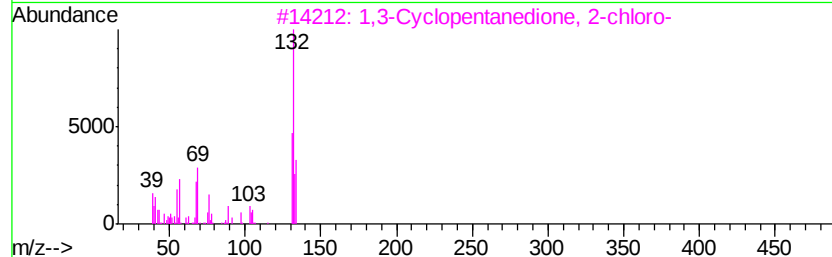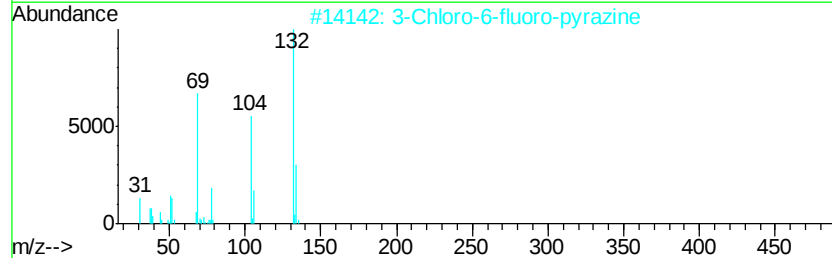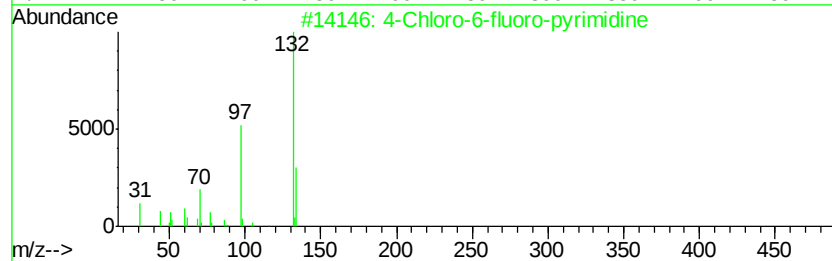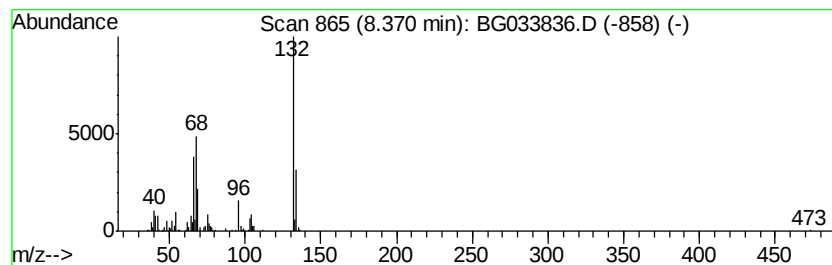

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041618\
Data File : BG033836.D
Acq On : 17 Apr 2018 4:47
Operator : SJ/JU
Sample : J2391-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-JETB-E-U-S

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.37	8.37	66.6	ng	506555	1	8.87	152073	20.0