

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
 Data File : BG033837.D
 Acq On : 17 Apr 2018 5:25
 Operator : SJ/JU
 Sample : J2391-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 041218-SIDI-E-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.464	25	30	40	rVB2	53495	106488	2.99%	0.921%
2	6.302	506	513	530	rBV4	31290	153726	4.32%	1.330%
3	8.018	797	805	808	rBV5	15743	40916	1.15%	0.354%
4	8.376	858	866	882	rBV2	110365	412265	11.59%	3.566%
5	8.858	942	948	960	rBV4	35021	122989	3.46%	1.064%
6	9.181	994	1003	1020	rBV	279201	742414	20.87%	6.423%
7	10.062	1146	1153	1184	rBV	139046	634369	17.83%	5.488%
8	11.737	1432	1438	1448	rBV2	64626	195389	5.49%	1.690%
9	14.099	1833	1840	1861	rBV	796577	1815007	51.01%	15.702%
10	14.892	1968	1975	1984	rBV3	20812	48837	1.37%	0.422%
11	15.468	2067	2073	2089	rBV2	198982	422275	11.87%	3.653%
12	16.948	2317	2325	2344	rBV	496880	1174507	33.01%	10.161%
13	17.083	2344	2348	2358	rVB3	27472	57952	1.63%	0.501%
14	18.206	2530	2539	2552	rBV	294185	643850	18.10%	5.570%
15	20.720	2961	2967	2981	rBV	2410385	3558023	100.00%	30.780%
16	22.548	3271	3278	3290	rBV2	357687	757627	21.29%	6.554%
17	26.314	3909	3919	3933	rBV2	196036	672804	18.91%	5.820%


Sum of corrected areas: 11559438

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033837.D
Acq On : 17 Apr 2018 5:25
Operator : SJ/JU
Sample : J2391-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-SIDI-E-D-M

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

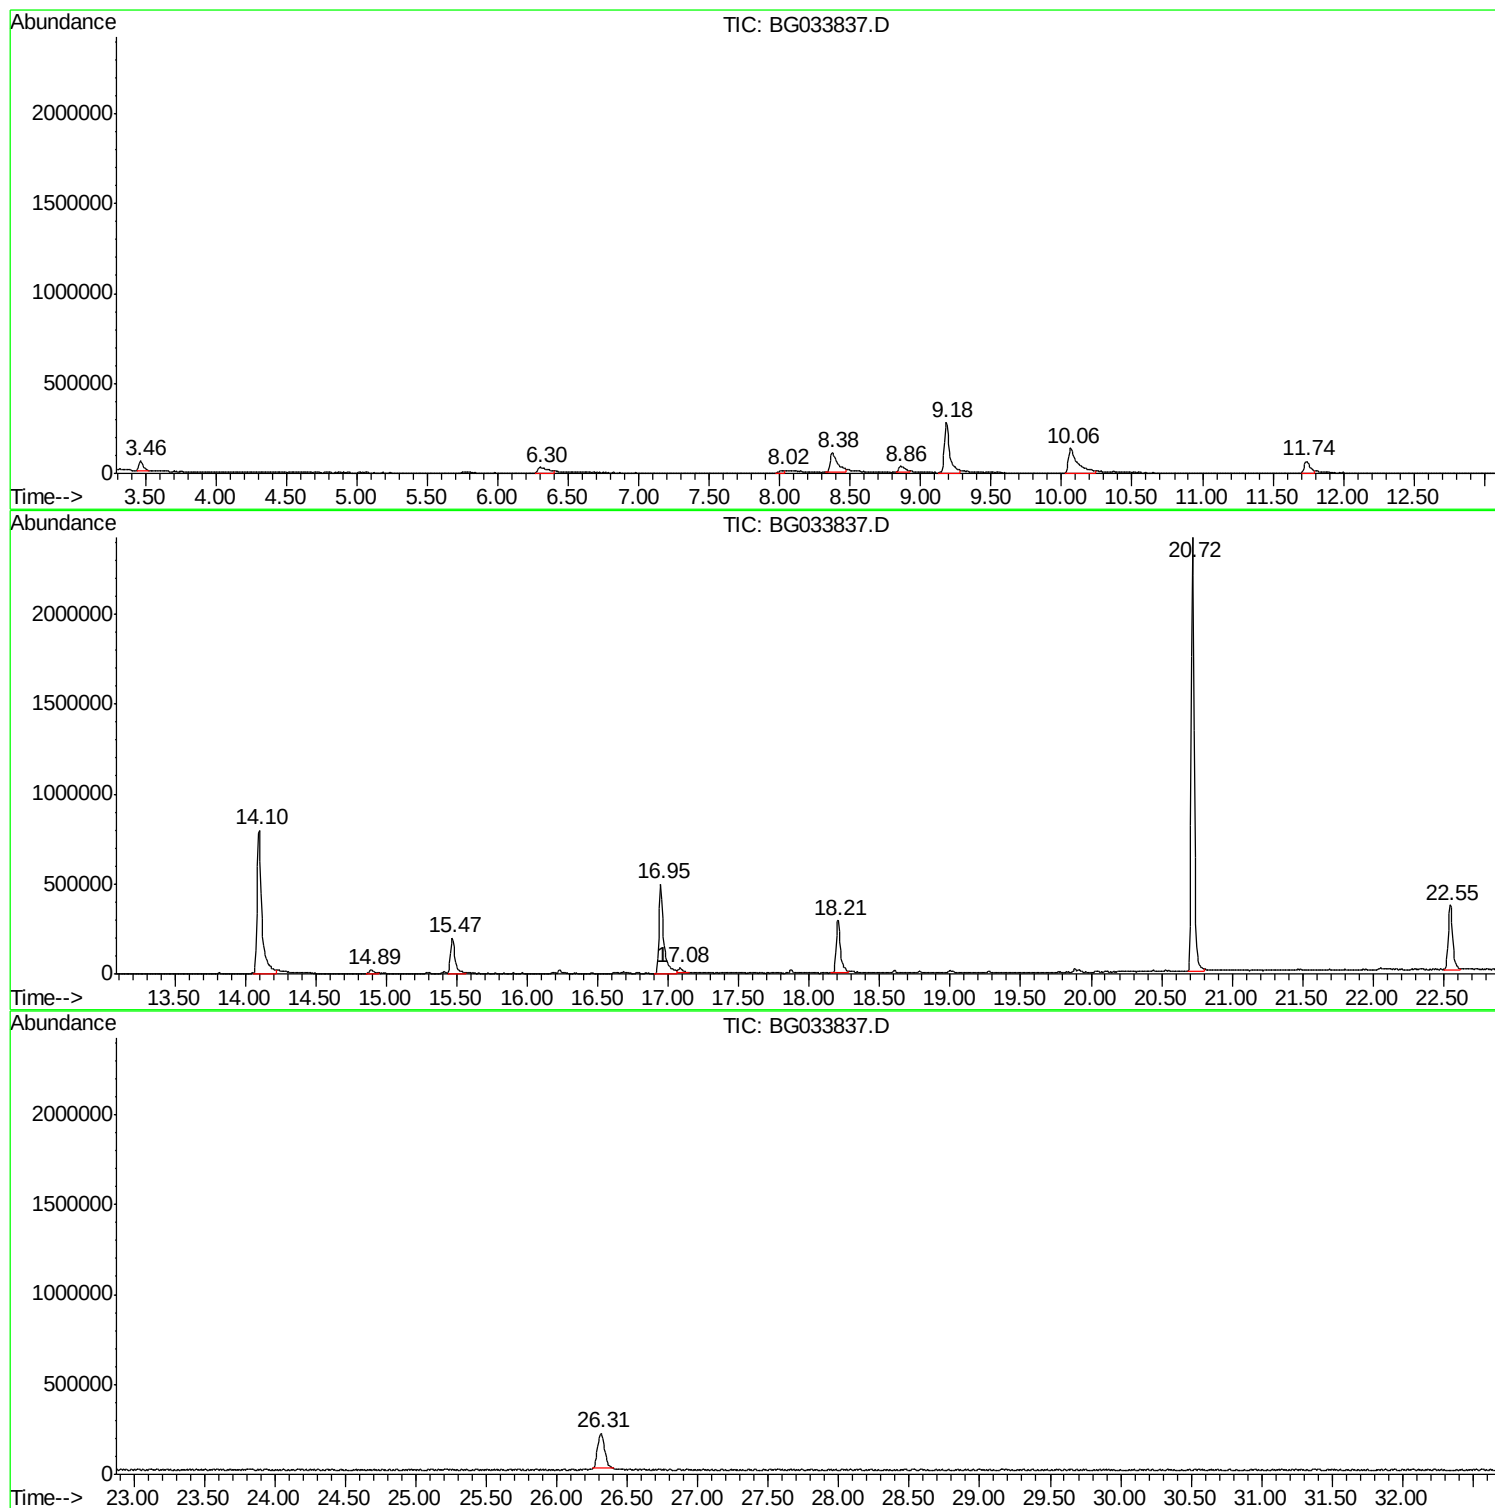

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041618\
Data File : BG033837.D
Acq On : 17 Apr 2018 5:25
Operator : SJ/JU
Sample : J2391-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-SIDI-E-D-M










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.38 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.38	67.04 ng	412265	1,4-Dichlorobenzene-d4	8.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		5-Aminoindole	132	C8H8N2	005192-03-0	16

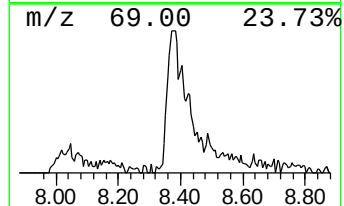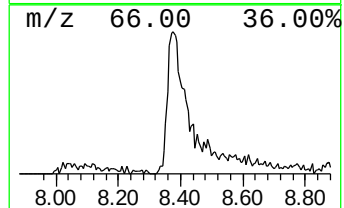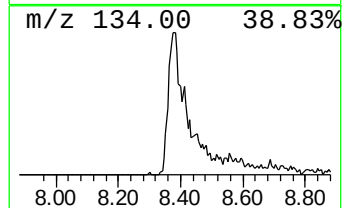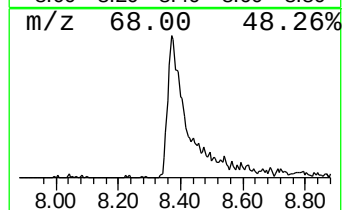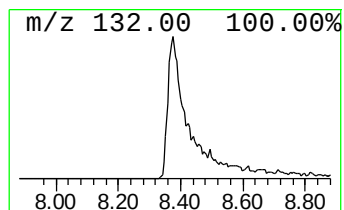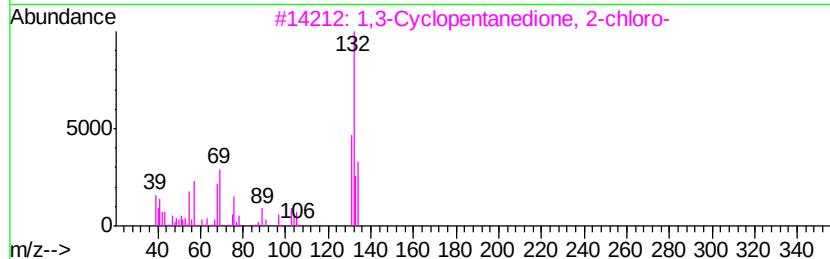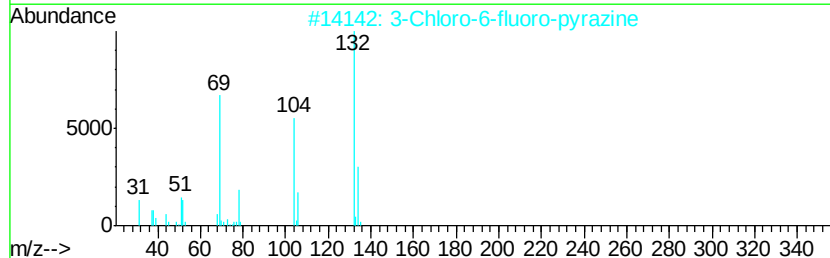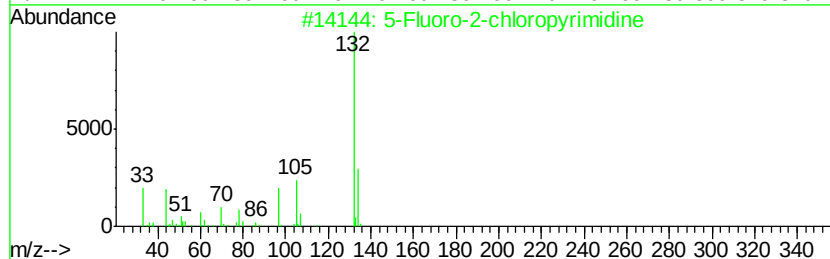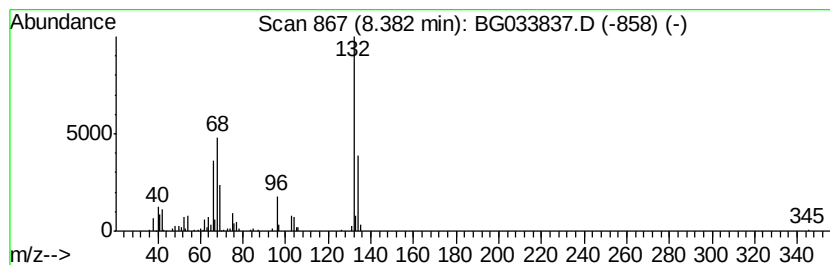

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041618\
Data File : BG033837.D
Acq On : 17 Apr 2018 5:25
Operator : SJ/JU
Sample : J2391-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
041218-SIDI-E-D-M

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.38	8.38	67.0	ng	412265	1	8.86	122989	20.0