


Data Path : Z:\HPCHEM1\BNA G\Data\BG041618\
 Data File : BG033808.D
 Acq On : 16 Apr 2018 9:56
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 16 11:44:01 2018

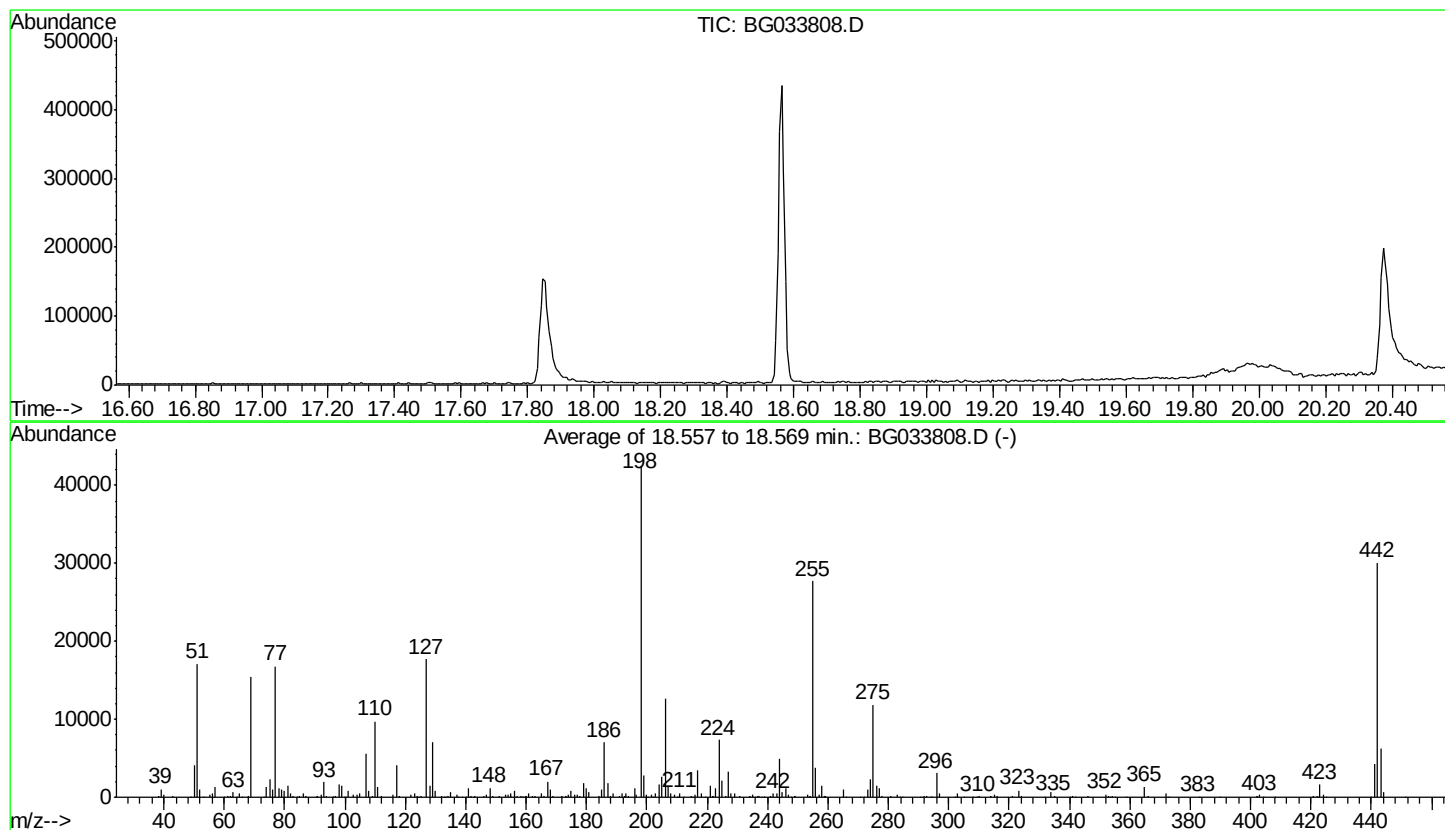

AutoFind: Scans 2599, 2600, 2601; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	17073	PASS
68	69	0.00	2	0.6	93	PASS
69	198	0.00	100	36.3	15414	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.6	17684	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42517	PASS
199	198	5	9	6.5	2743	PASS
275	198	10	60	28.0	11891	PASS
365	198	1	100	3.3	1396	PASS
441	443	0.01	100	69.2	4298	PASS
442	198	50	100	70.8	30106	PASS
443	442	15	24	20.6	6207	PASS