


Data Path : Z:\HPCHEM1\BNA G\Data\BG041618\
 Data File : BG033827.D
 Acq On : 16 Apr 2018 23:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 16 11:44:01 2018

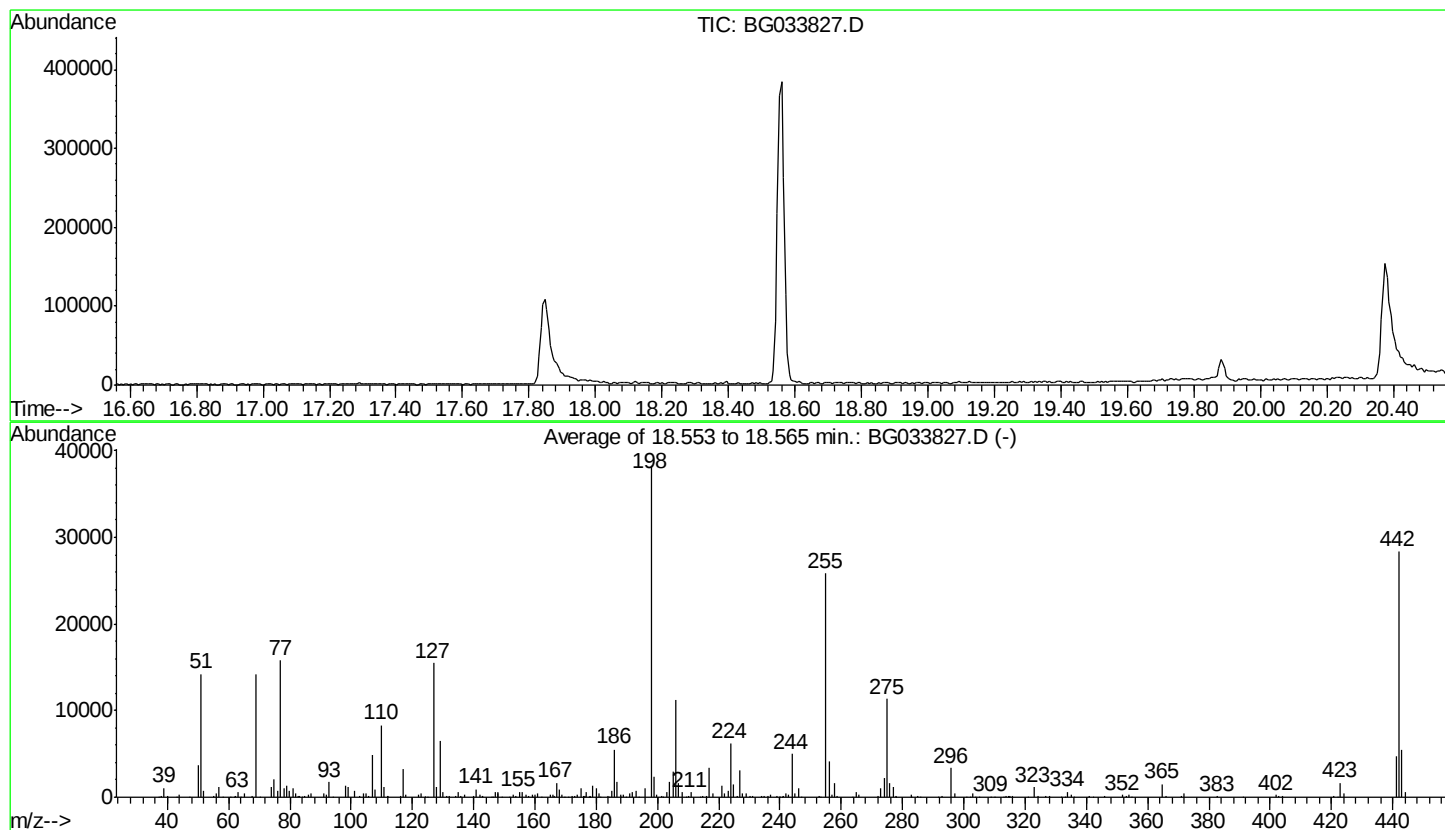

AutoFind: Scans 2598, 2599, 2600; Background Corrected with Scan 2591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	14202	PASS
68	69	0.00	2	1.5	212	PASS
69	198	0.00	100	37.2	14246	PASS
70	69	0.00	2	0.4	53	PASS
127	198	10	80	40.4	15480	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38272	PASS
199	198	5	9	6.3	2415	PASS
275	198	10	60	29.6	11325	PASS
365	198	1	100	4.0	1517	PASS
441	443	0.01	100	87.6	4747	PASS
442	198	50	100	74.1	28346	PASS
443	442	15	24	19.1	5420	PASS