
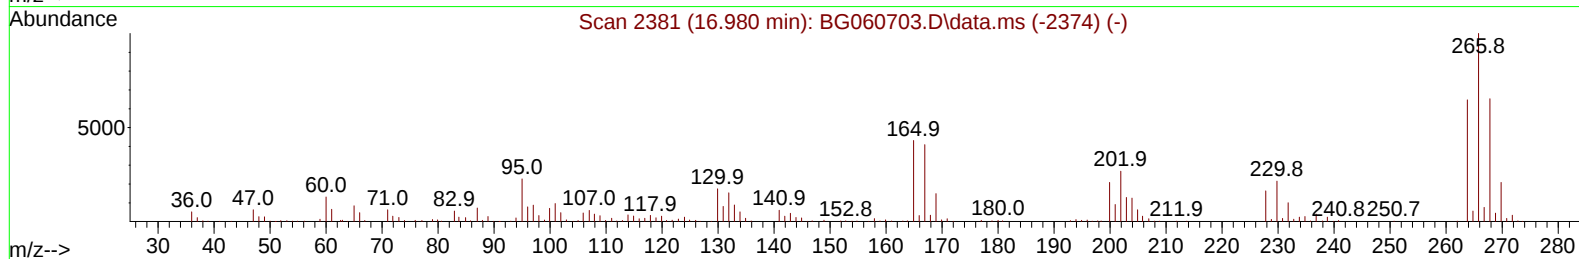
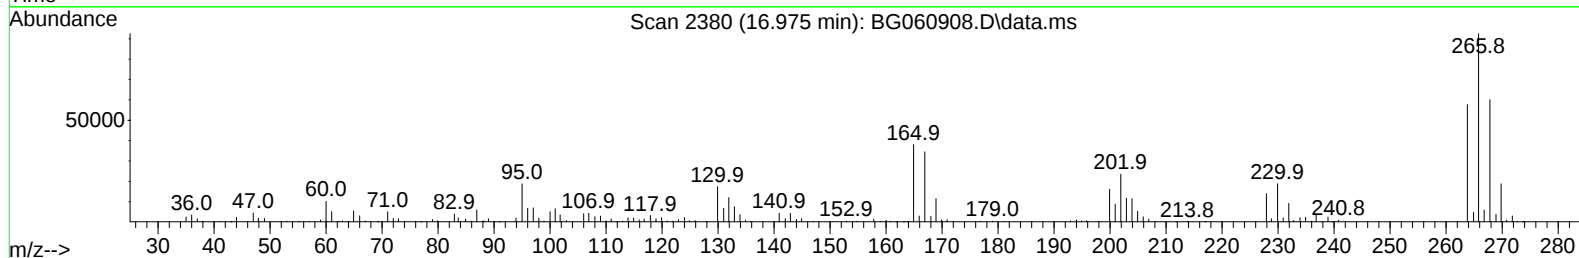


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041624\
Data File : BG060908.D
Acq On : 16 Apr 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 12:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

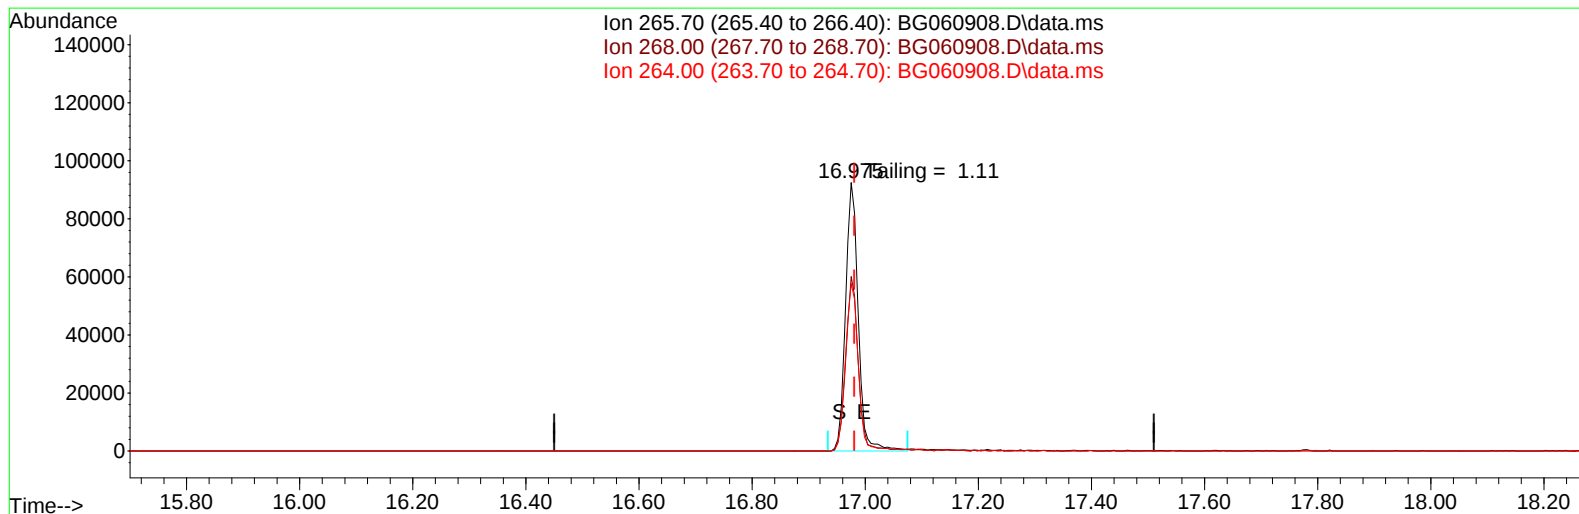

TIC: BG060908.D\data.ms

(70) Pentachlorophenol (C)




16.975min (-0.005) 257380.43 ng

response 144302

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.97
264.00	64.70	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041624\
Data File : BG060908.D
Acq On : 16 Apr 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 12:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

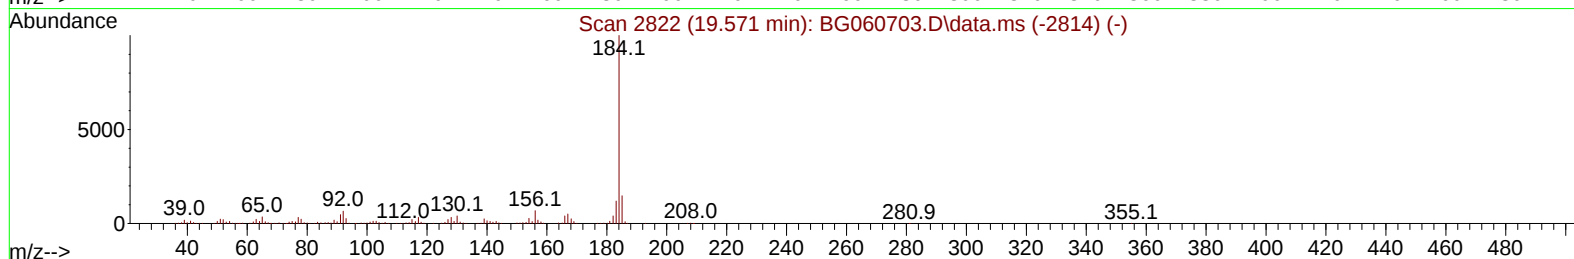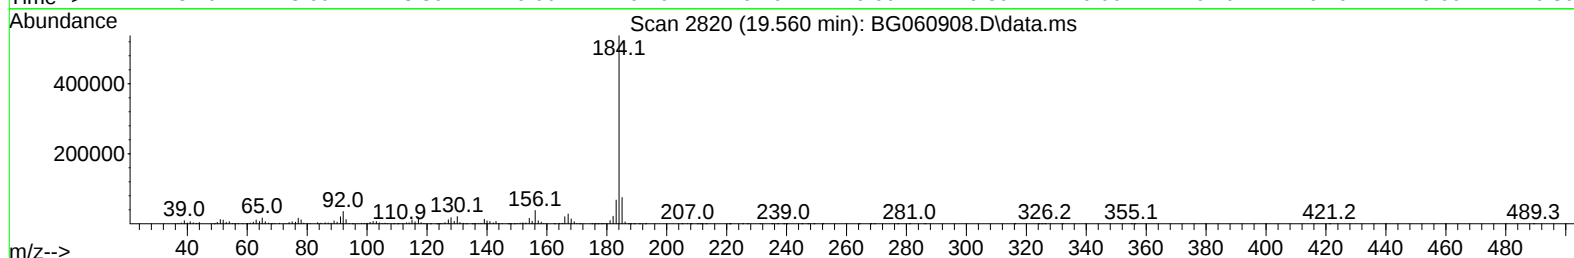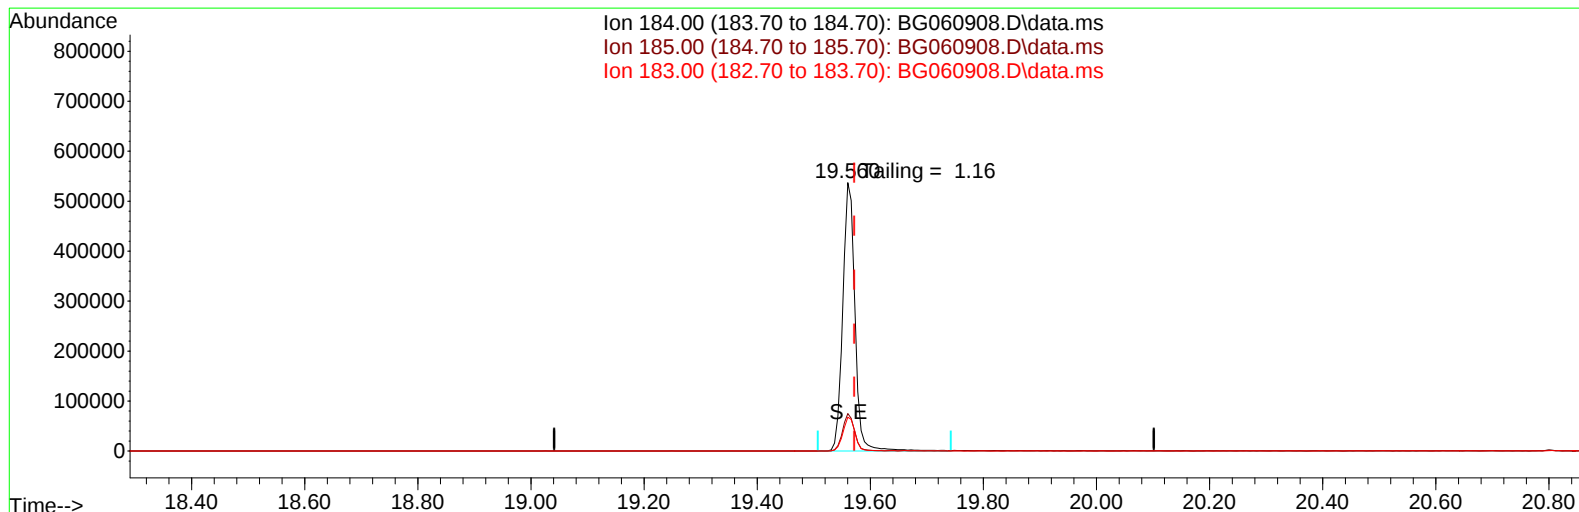

TIC: BG060908.D\data.ms

(77) Benzidine**19.560min (-0.011) 78325.93 ng****response 806434**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.97
183.00	11.90	12.59
0.00	0.00	0.00