
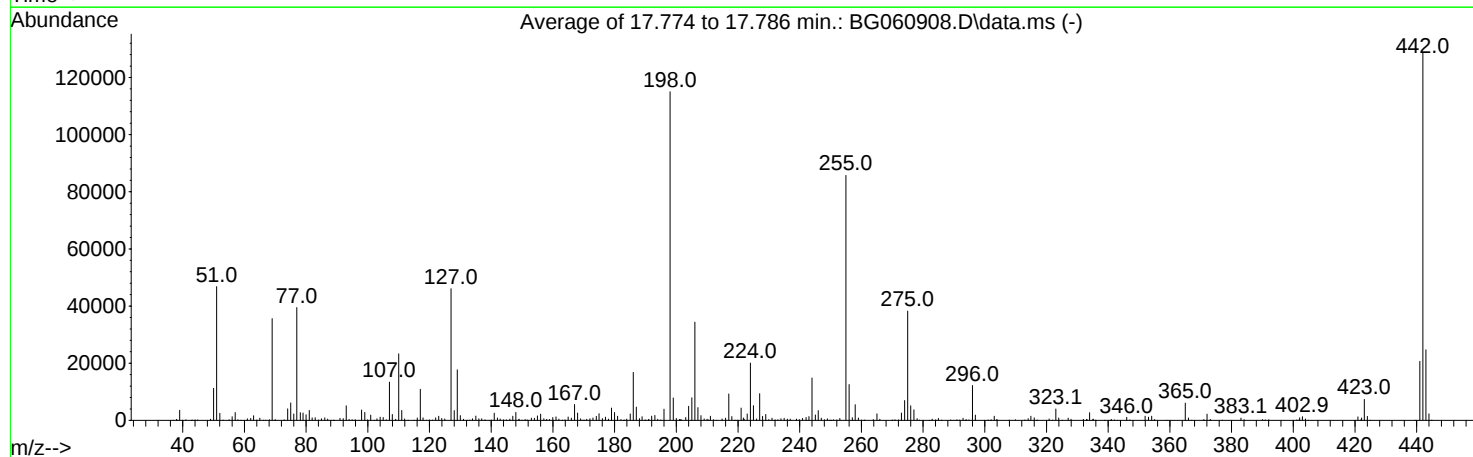


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041624\  
Data File : BG060908.D  
Acq On : 16 Apr 2024 10:50  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG032924.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sat Mar 30 03:12:26 2024

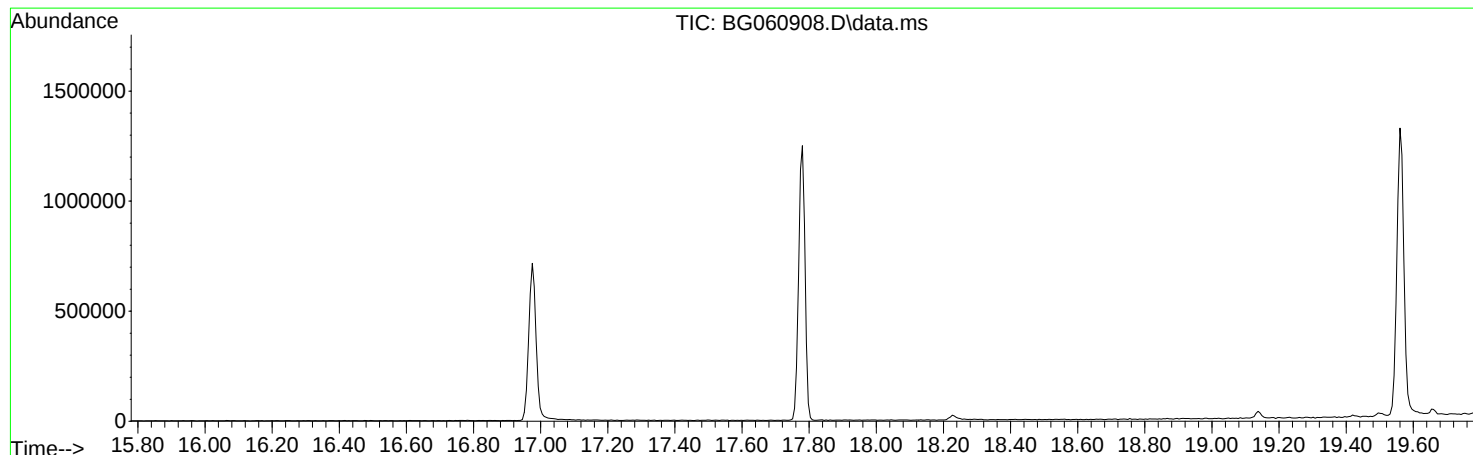




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.7         | 46821      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.6          | 215        | PASS                |
| 69             | 198             | 0.00            | 100             | 31.0         | 35624      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 156        | PASS                |
| 127            | 198             | 10              | 80              | 40.1         | 46099      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 115029     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 7824       | PASS                |
| 275            | 198             | 10              | 60              | 33.3         | 38256      | PASS                |
| 365            | 198             | 1               | 100             | 5.2          | 6025       | PASS                |
| 441            | 198             | 0.01            | 100             | 17.9         | 20643      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 128741     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 24691      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041624\  
Data File : BG060908.D  
Acq On : 16 Apr 2024 10:50  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Apr 16 12:00:53 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG032924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Mar 30 03:12:26 2024  
Response via : Initial Calibration

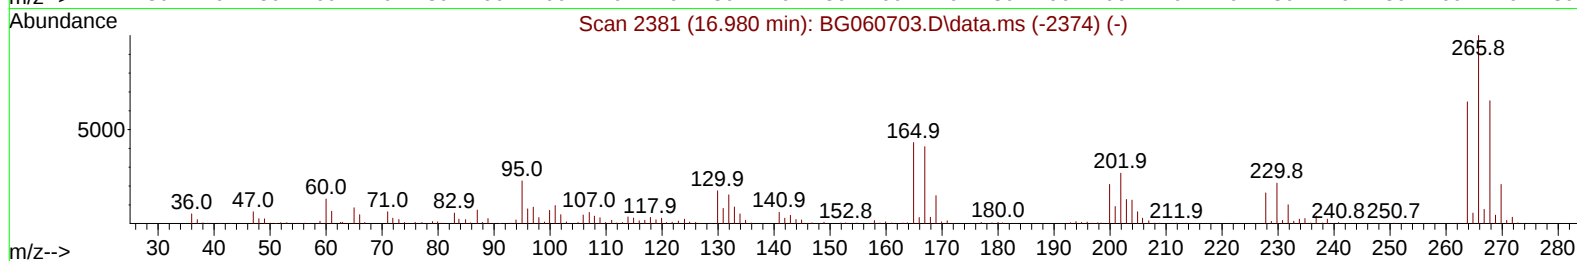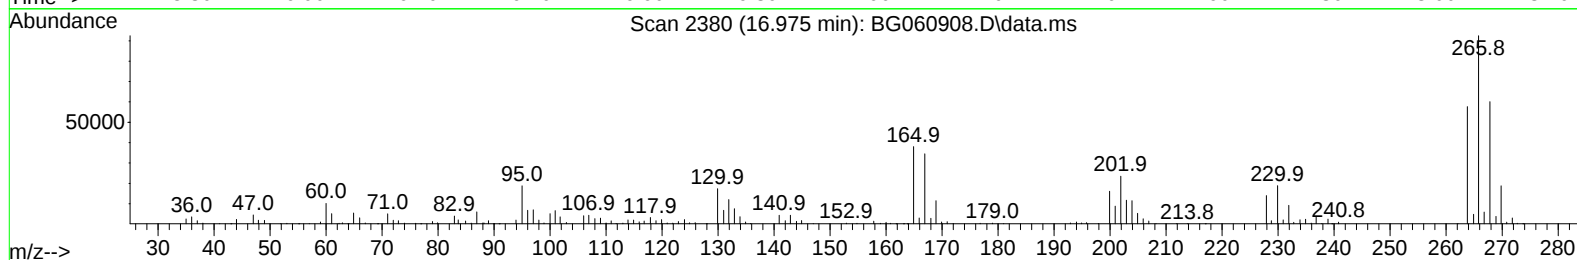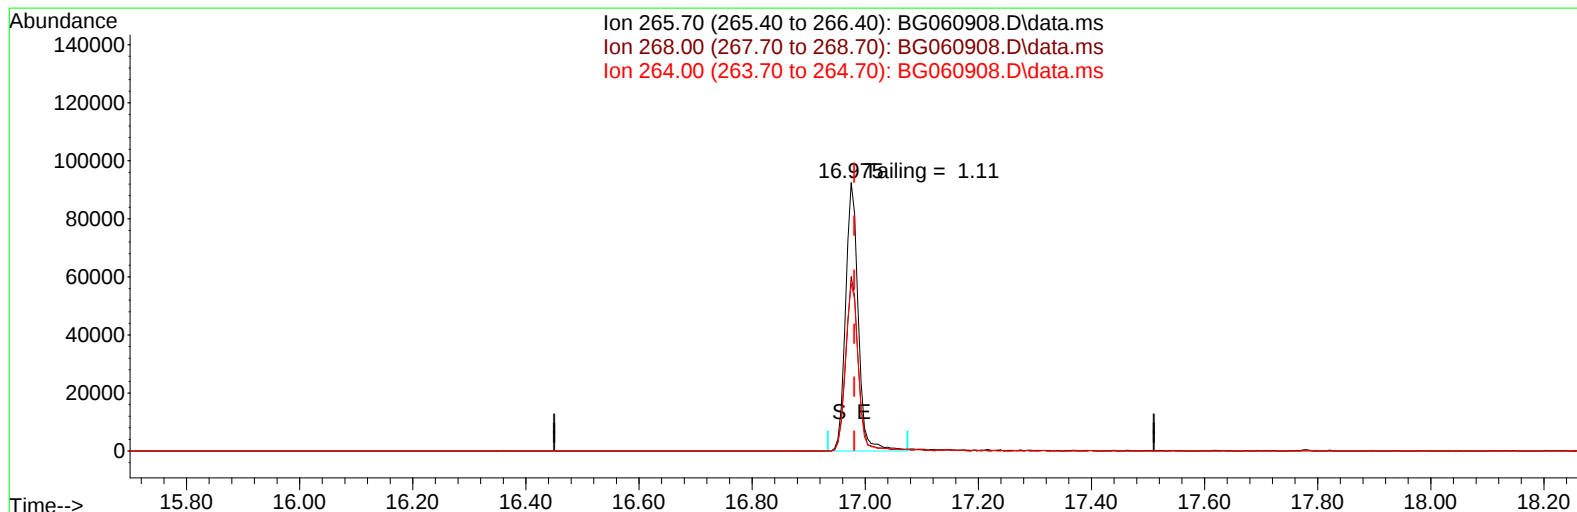

TIC: BG060908.D\data.ms

**(70) Pentachlorophenol (C)**

16.975min (-0.005) 257380.43 ng




response 144302

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.30  | 64.97  |
| 264.00 | 64.70  | 62.35  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041624\  
Data File : BG060908.D  
Acq On : 16 Apr 2024 10:50  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Apr 16 12:00:53 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG032924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Mar 30 03:12:26 2024  
Response via : Initial Calibration

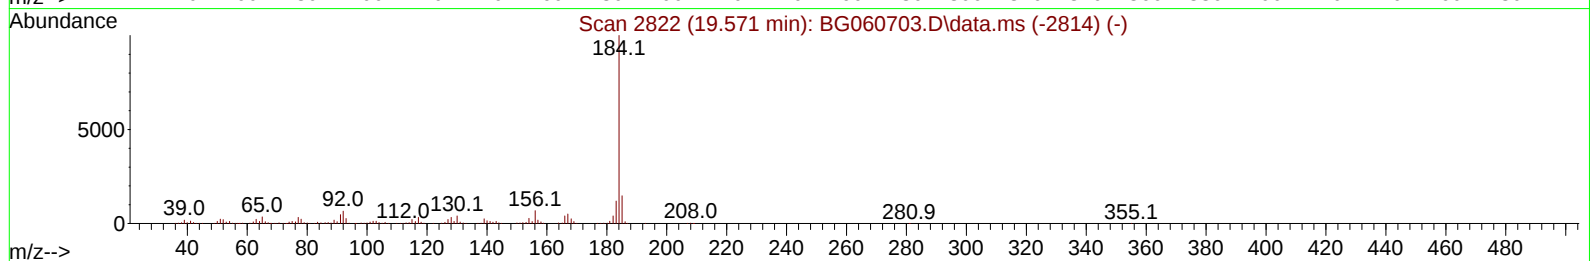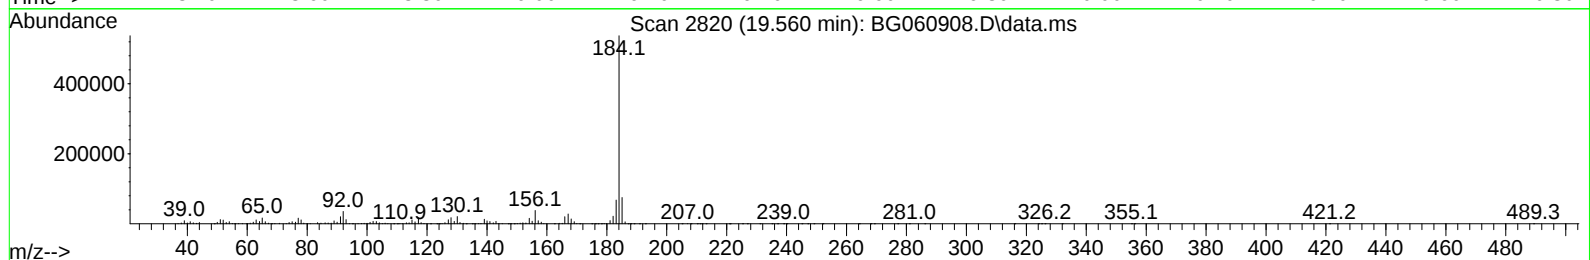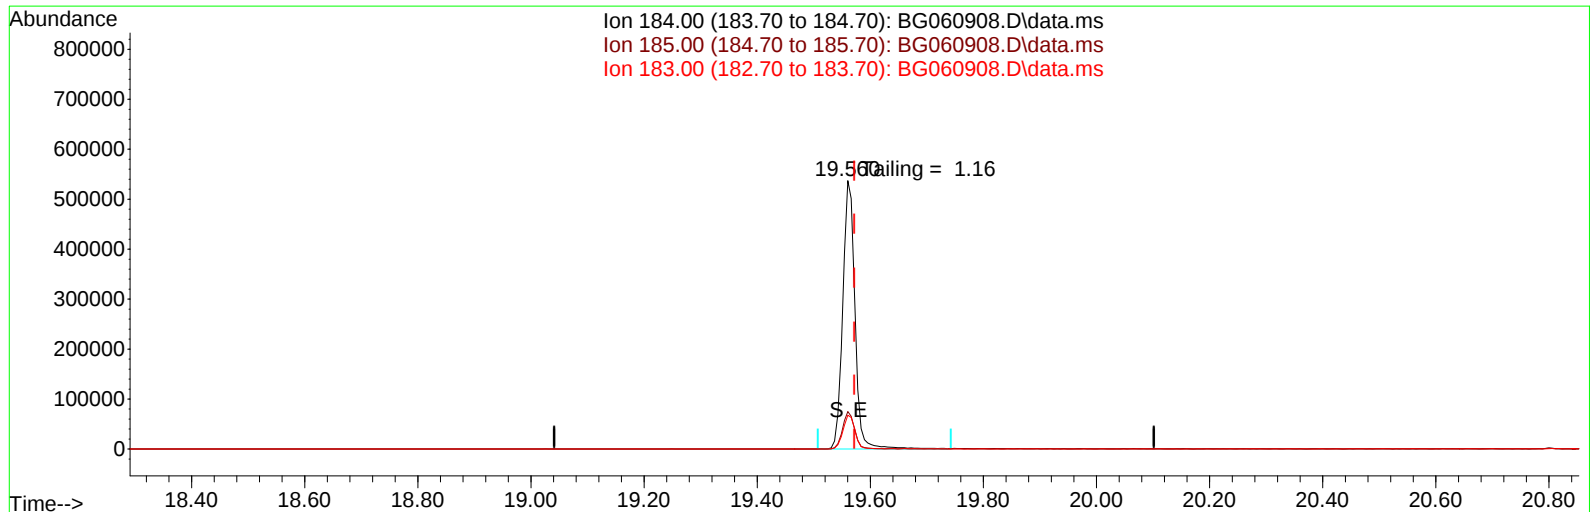

TIC: BG060908.D\data.ms

**(77) Benzidine**

**19.560min (-0.011) 78325.93 ng**

**response 806434**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 13.97  |
| 183.00 | 11.90  | 12.59  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/16/2024     | BNA_G            | <u>BG060908.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 421374           | 20.8               |
| DDD           | 16904            | 20.359             |
| DDE           | 2480             | 19.854             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 19384         | 440758           | 4.40               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP