

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
 Data File : BG016539.D
 Acq On : 19 Apr 2015 2:02
 Operator : TP/IZ
 Sample : G1868-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 P5-28(15-20)

Quant Time: Apr 20 04:13:33 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 20 03:57:28 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	78605	20.00	ng	0.00
21) Naphthalene-d8	10.44	136	348042	20.00	ng	0.00
38) Acenaphthene-d10	14.30	164	195115	20.00	ng	0.00
63) Phenanthrene-d10	17.04	188	391004	20.00	ng	0.00
75) Chrysene-d12	21.23	240	338617	20.00	ng	0.00
86) Perylene-d12	23.45	264	321261	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	461015	92.56	ng	0.00
7) Phenol-d6	6.85	99	662134	88.56	ng	0.00
23) Nitrobenzene-d5	8.81	82	339143	56.45	ng	0.00
41) 2,4,6-Tribromophenol	15.79	330	121997	92.45	ng	0.00
44) 2-Fluorobiphenyl	12.92	172	718793	62.72	ng	0.00
78) Terphenyl-d14	19.67	244	800519	55.33	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.76	163	30967	2.17	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016539.D
Acq On : 19 Apr 2015 2:02
Operator : TP/IZ
Sample : G1868-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
P5-28(15-20)

Quant Time: Apr 20 04:13:33 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

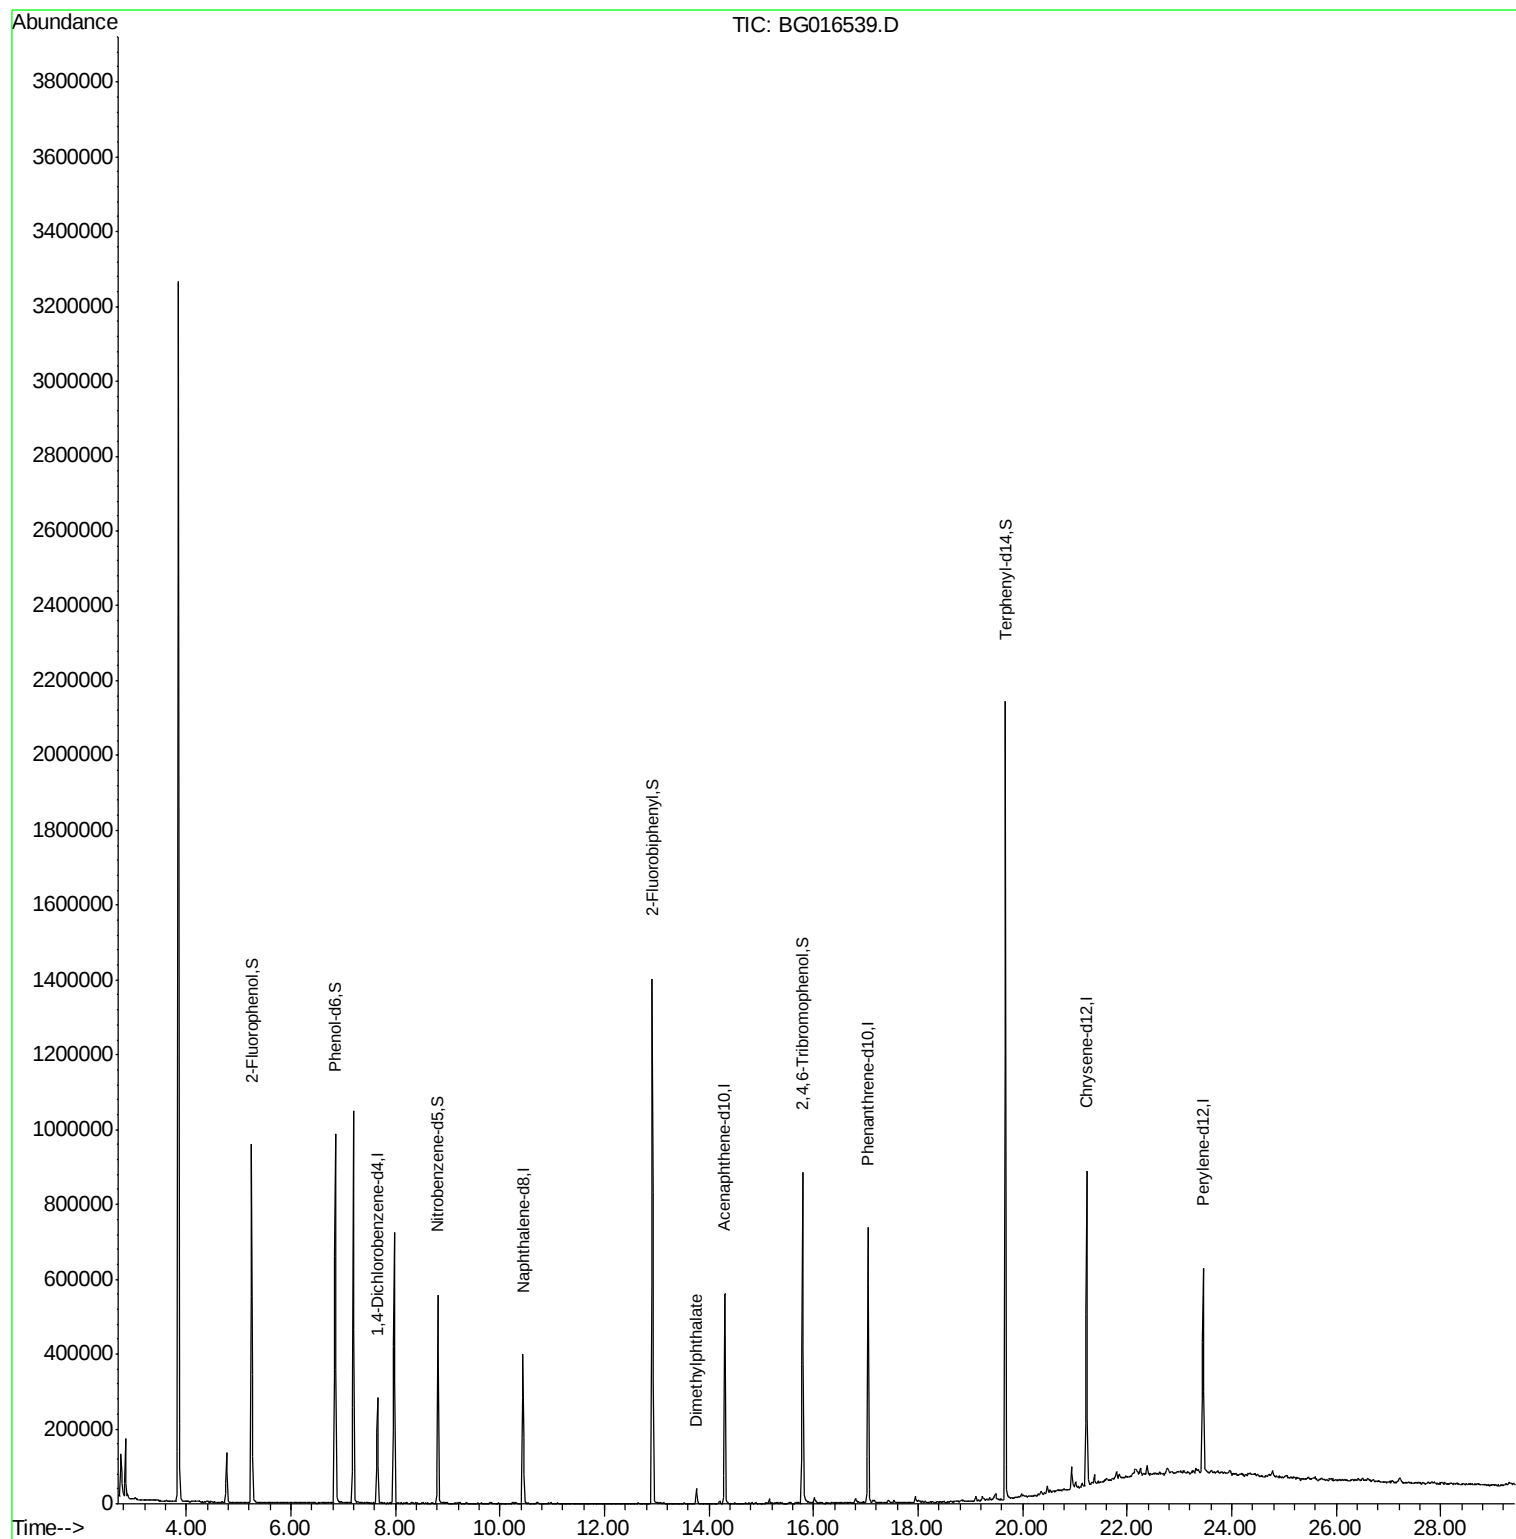



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.66 min Scan# 846

Delta R.T. 0.00 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02

Instrument :

BNA_G

ClientSampleId :

P5-28(15-20)


Tgt Ion:152 Resp: 78605

Ion Ratio Lower Upper

152 100

150 156.0 130.1 195.1



115 54.3 50.5 75.7

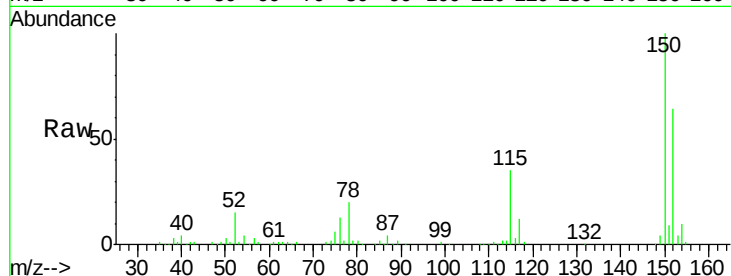

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

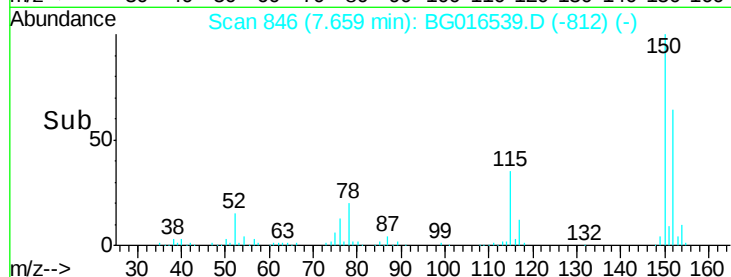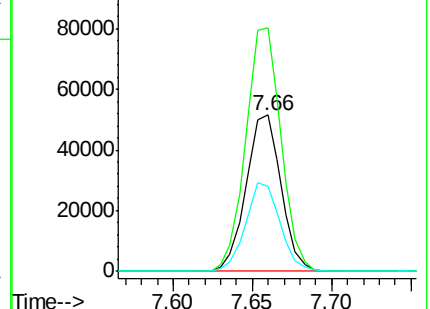

#5

2-Fluorophenol

Concen: 92.56 ng

RT: 5.25 min Scan# 436

Delta R.T. 0.00 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02


Tgt Ion:112 Resp: 461015

Ion Ratio Lower Upper

112 100

64 51.5 44.5 66.7



63 24.6 21.4 32.0

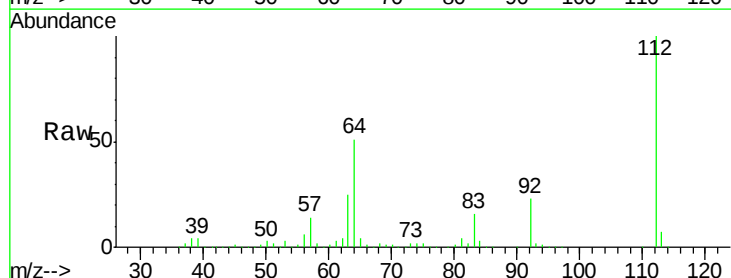


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

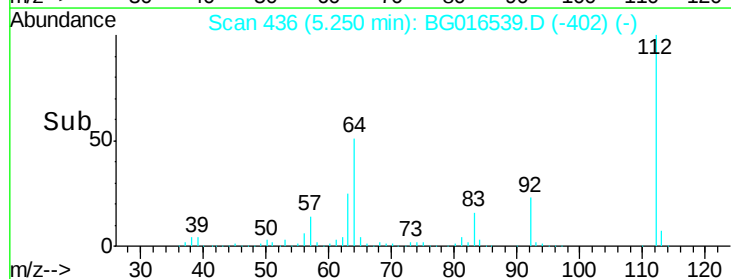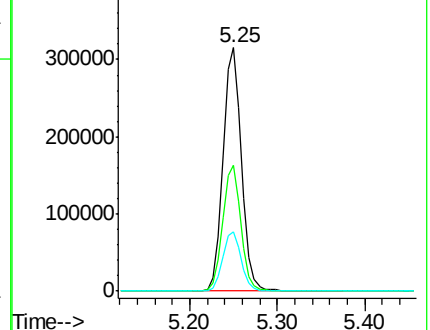

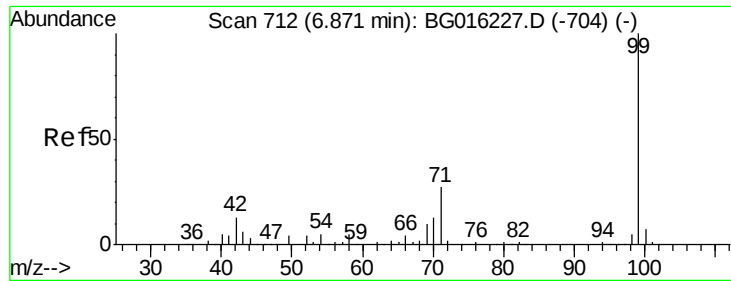

#7

Phenol-d6

Concen: 88.56 ng

RT: 6.85 min Scan# 708

Delta R.T. 0.00 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02

Instrument :

BNA_G

ClientSampleId :

P5-28(15-20)


Tgt Ion: 99 Resp: 662134

Ion Ratio Lower Upper



99 100

42 12.1 10.0 15.0

71 25.9 21.5 32.3

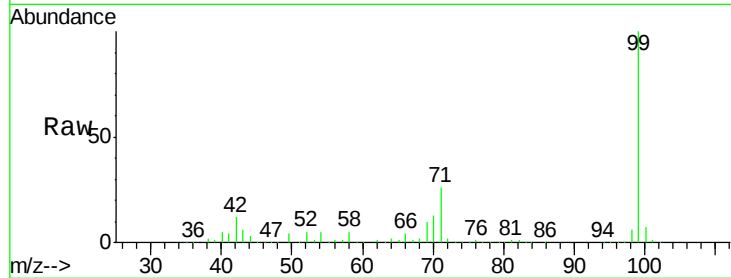

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

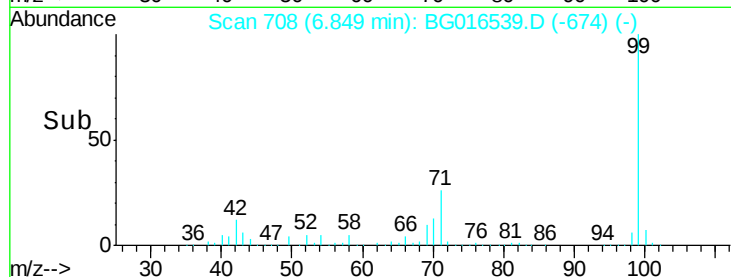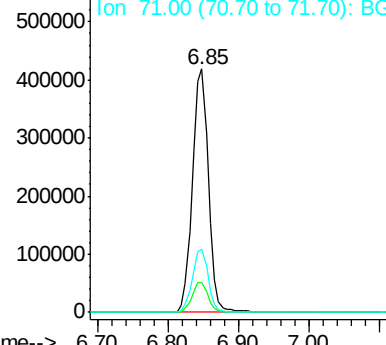

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.44 min Scan# 1320

Delta R.T. 0.00 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02

Tgt Ion: 136 Resp: 348042


Ion Ratio Lower Upper

136 100



137 10.9 8.7 13.1

54 6.7 6.3 9.5

68 7.3 6.5 9.7

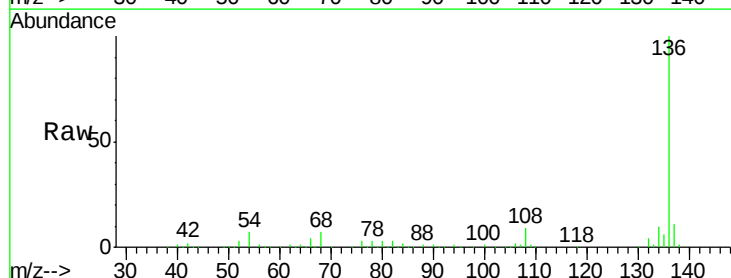

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

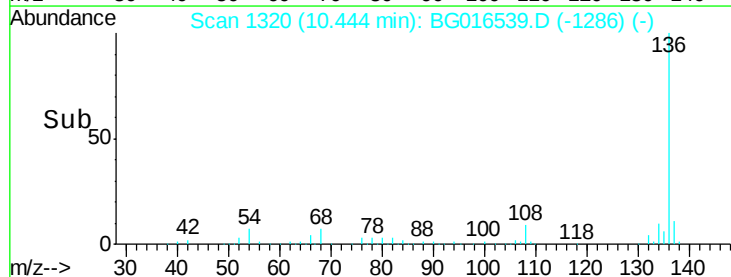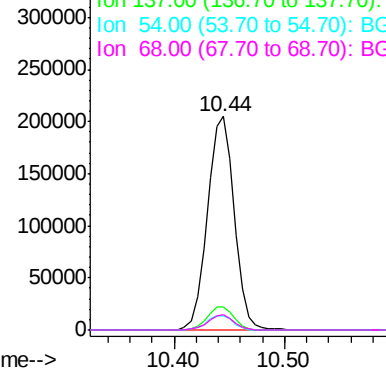






#23
 Nitrobenzene-d5
 Concen: 56.45 ng
 RT: 8.81 min Scan# 1042
 Delta R.T. -0.01 min
 Lab File: BG016539.D
 Acq: 19 Apr 2015 2:02

Instrument :
 BNA_G
 ClientSampled :
 P5-28(15-20)

Tgt Ion: 82 Resp: 339143
 Ion Ratio Lower Upper
 82 100
 128 51.1 37.8 56.8
 54 40.5 32.6 49.0

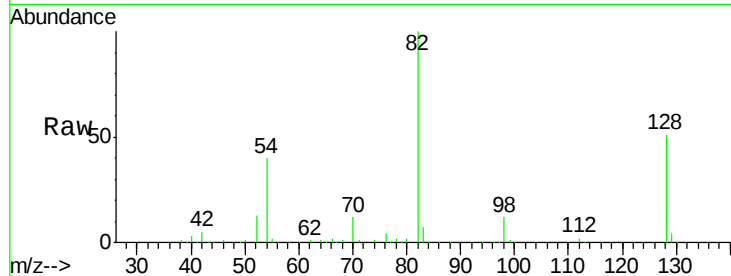


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

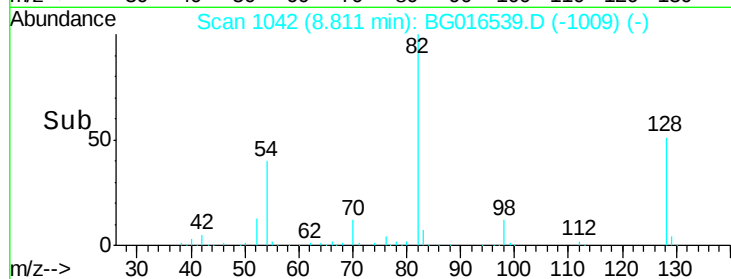
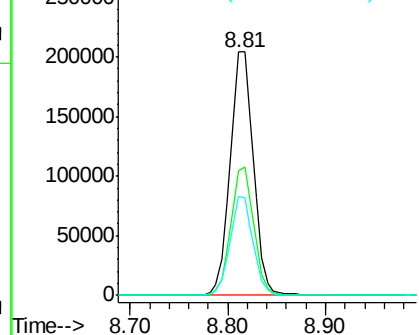


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.30 min Scan# 1976
 Delta R.T. -0.01 min
 Lab File: BG016539.D
 Acq: 19 Apr 2015 2:02

Tgt Ion: 164 Resp: 195115
 Ion Ratio Lower Upper
 164 100
 162 93.8 77.3 115.9
 160 41.5 36.7 55.1

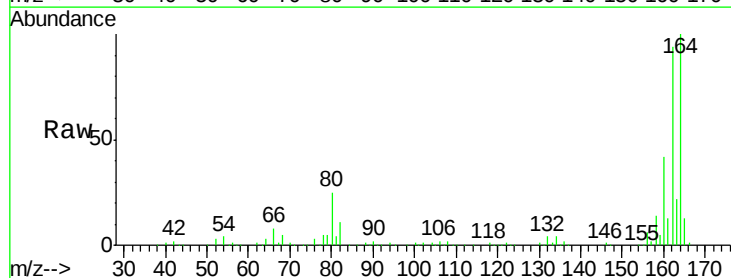

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

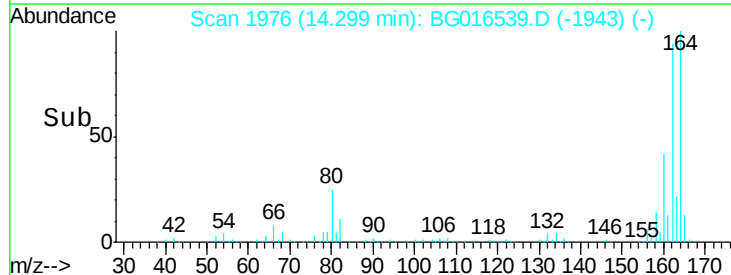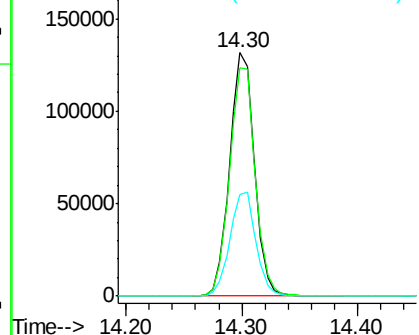







#41
 2,4,6-Tribromophenol
 Concen: 92.45 ng
 RT: 15.79 min Scan# 2230
 Delta R.T. -0.01 min
 Lab File: BG016539.D
 Acq: 19 Apr 2015 2:02

Instrument :
 BNA_G
 ClientSampleId :
 P5-28(15-20)

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.1	75.8	113.6
141	57.7	46.6	69.8

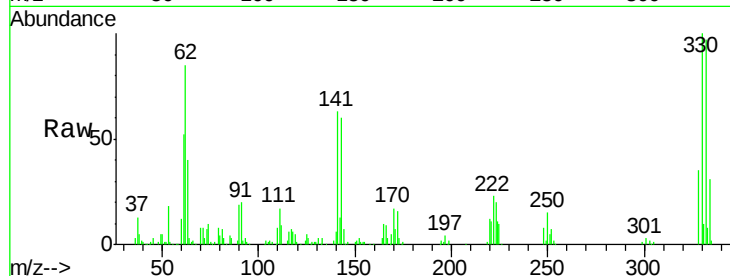


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

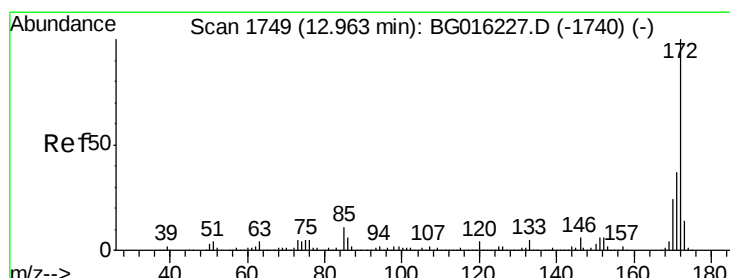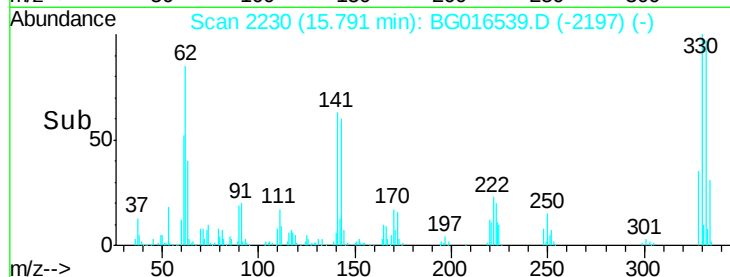
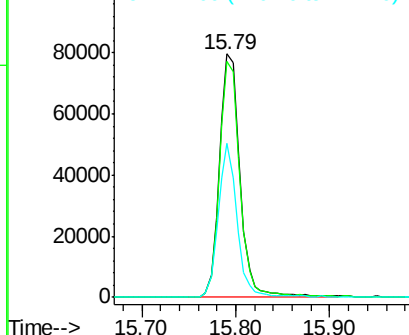



#44
 2-Fluorobiphenyl
 Concen: 62.72 ng
 RT: 12.92 min Scan# 1741
 Delta R.T. -0.01 min
 Lab File: BG016539.D
 Acq: 19 Apr 2015 2:02

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	29.6	44.4
170	23.9	19.4	29.2

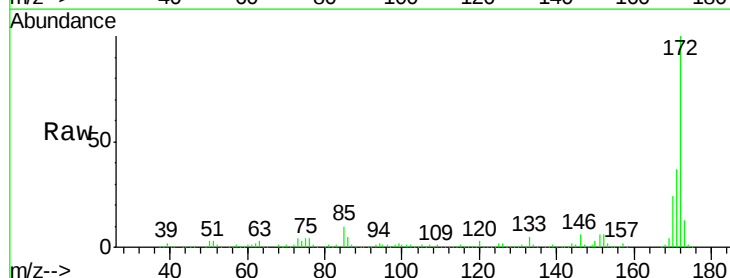

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

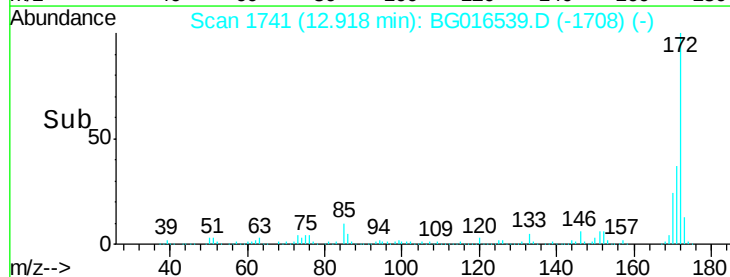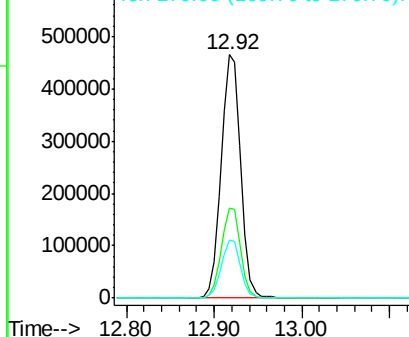

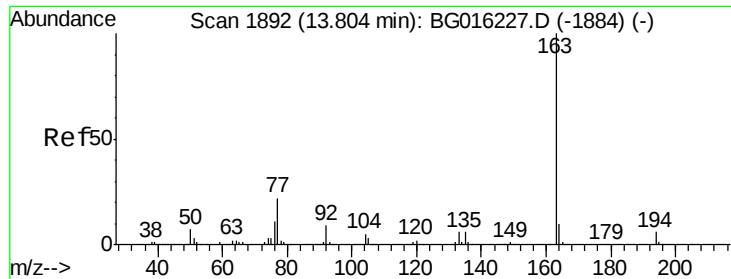

#49

Dimethylphthalate

Concen: 2.17 ng

RT: 13.76 min Scan# 1885

Delta R.T. -0.01 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02

Instrument :

BNA_G

ClientSampleId :

P5-28(15-20)


Tgt Ion:163 Resp: 30967

Ion Ratio Lower Upper

163 100

194 5.5 5.0 7.4




164 9.4 8.2 12.4

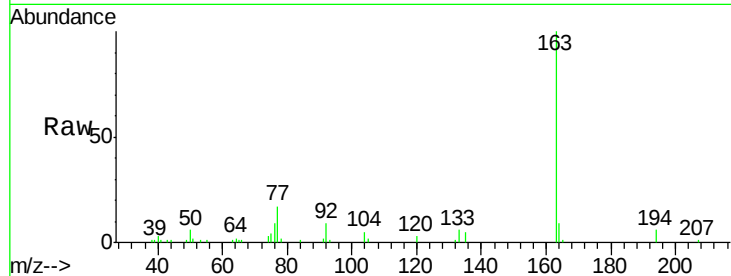

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

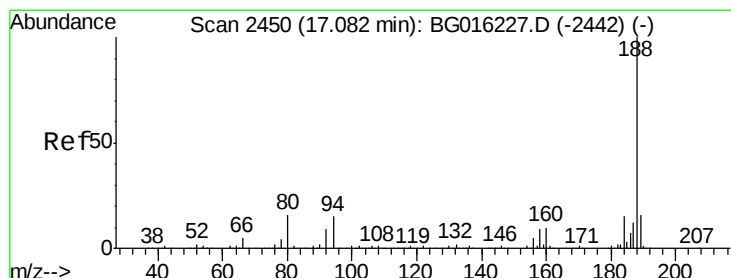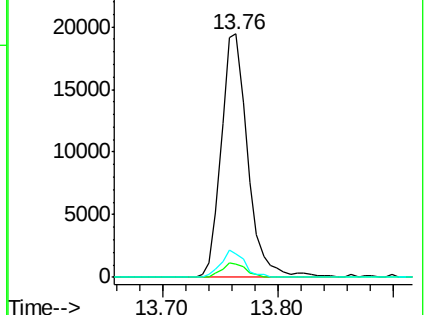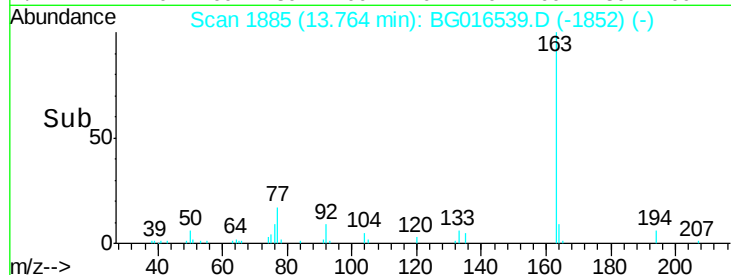

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.04 min Scan# 2443

Delta R.T. -0.01 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02


Tgt Ion:188 Resp: 391004

Ion Ratio Lower Upper

188 100

94 13.8 12.2 18.4



80 14.4 12.8 19.2

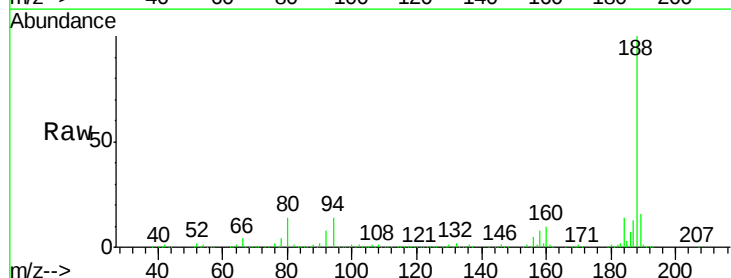


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

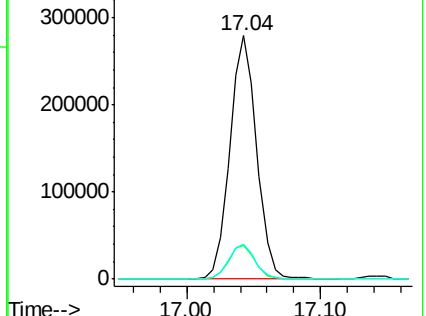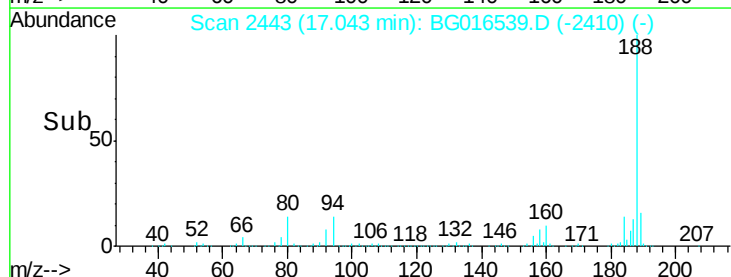

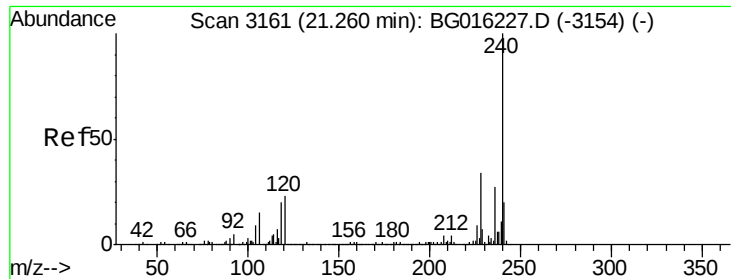

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.23 min Scan# 3155

Delta R.T. -0.01 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02

Instrument :

BNA_G

ClientSampleId :

P5-28(15-20)


Tgt Ion:240 Resp: 338617

Ion Ratio Lower Upper

240 100

120 20.3 18.6 28.0




236 27.2 21.7 32.5

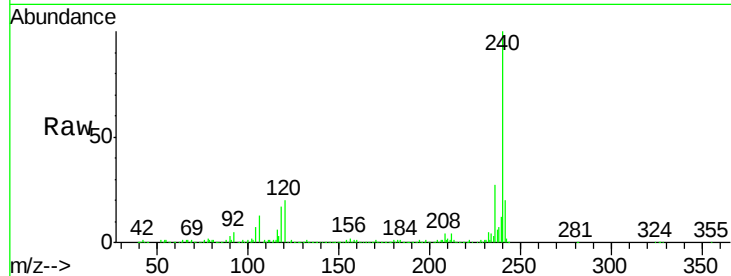

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

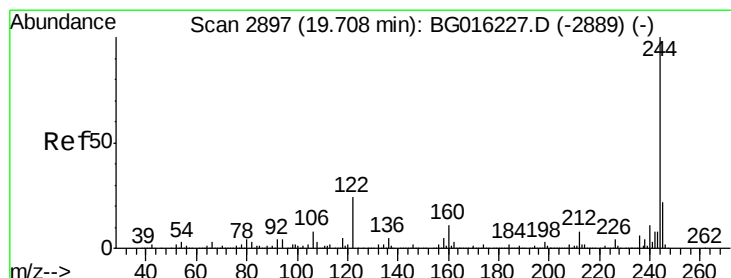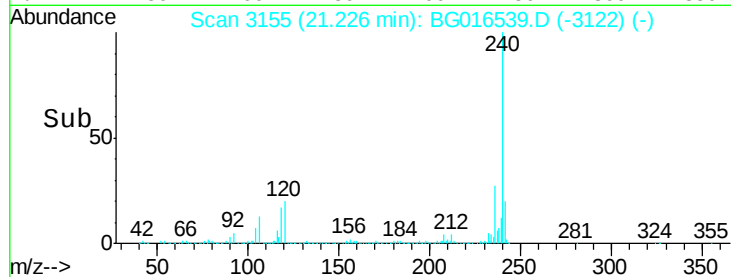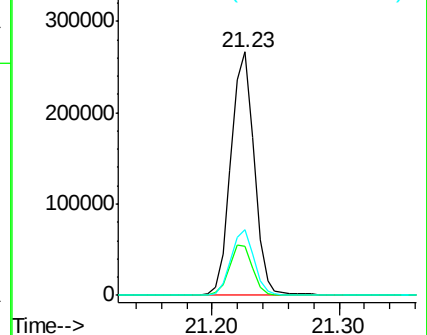

#78

Terphenyl-d14

Concen: 55.33 ng

RT: 19.67 min Scan# 2891

Delta R.T. 0.00 min

Lab File: BG016539.D

Acq: 19 Apr 2015 2:02


Tgt Ion:244 Resp: 800519

Ion Ratio Lower Upper

244 100

212 8.0 6.6 9.8



122 21.7 19.1 28.7

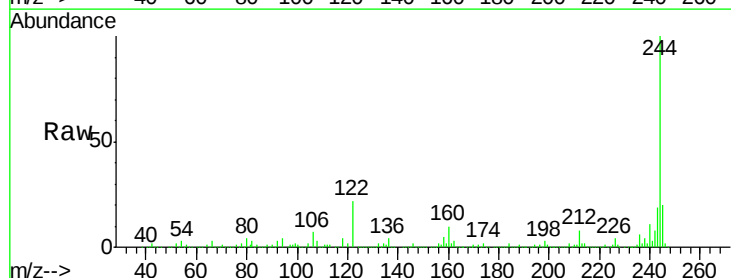


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

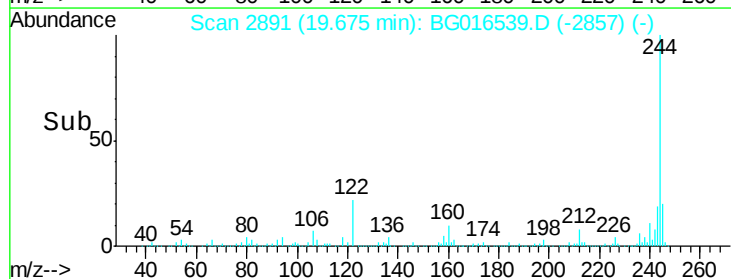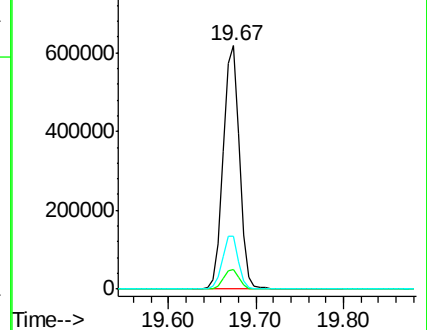

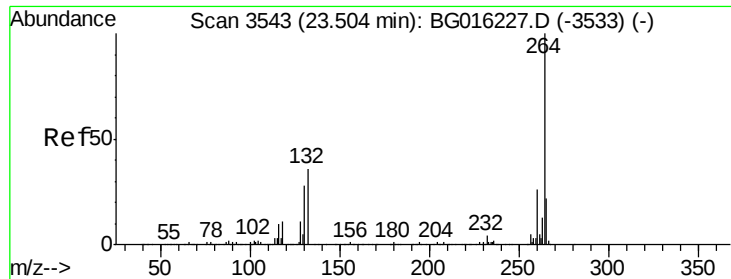

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.45 min Scan# 3534
Delta R.T. -0.01 min
Lab File: BG016539.D
Acq: 19 Apr 2015 2:02

Instrument :
BNA_G
ClientSampleId :
P5-28(15-20)

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.3	20.4	30.6
265	21.2	17.2	25.8

