

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
 Data File : BG016542.D
 Acq On : 19 Apr 2015 3:46
 Operator : TP/IZ
 Sample : G1890-13
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-03(SB-04-14)

Quant Time: Apr 20 04:14:13 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 20 03:57:28 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	82771	20.00	ng	0.00
21) Naphthalene-d8	10.44	136	345965	20.00	ng	0.00
38) Acenaphthene-d10	14.30	164	192500	20.00	ng	0.00
63) Phenanthrene-d10	17.04	188	383247	20.00	ng	0.00
75) Chrysene-d12	21.22	240	331723	20.00	ng	0.00
86) Perylene-d12	23.45	264	318644	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	637636	121.58	ng	0.00
7) Phenol-d6	6.85	99	810686	102.97	ng	0.00
23) Nitrobenzene-d5	8.82	82	497753	83.35	ng	0.00
41) 2,4,6-Tribromophenol	15.79	330	153818	118.15	ng	0.00
44) 2-Fluorobiphenyl	12.92	172	989690	87.53	ng	0.00
78) Terphenyl-d14	19.68	244	1077869	76.05	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016542.D
Acq On : 19 Apr 2015 3:46
Operator : TP/IZ
Sample : G1890-13
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-03(SB-04-14)

Quant Time: Apr 20 04:14:13 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

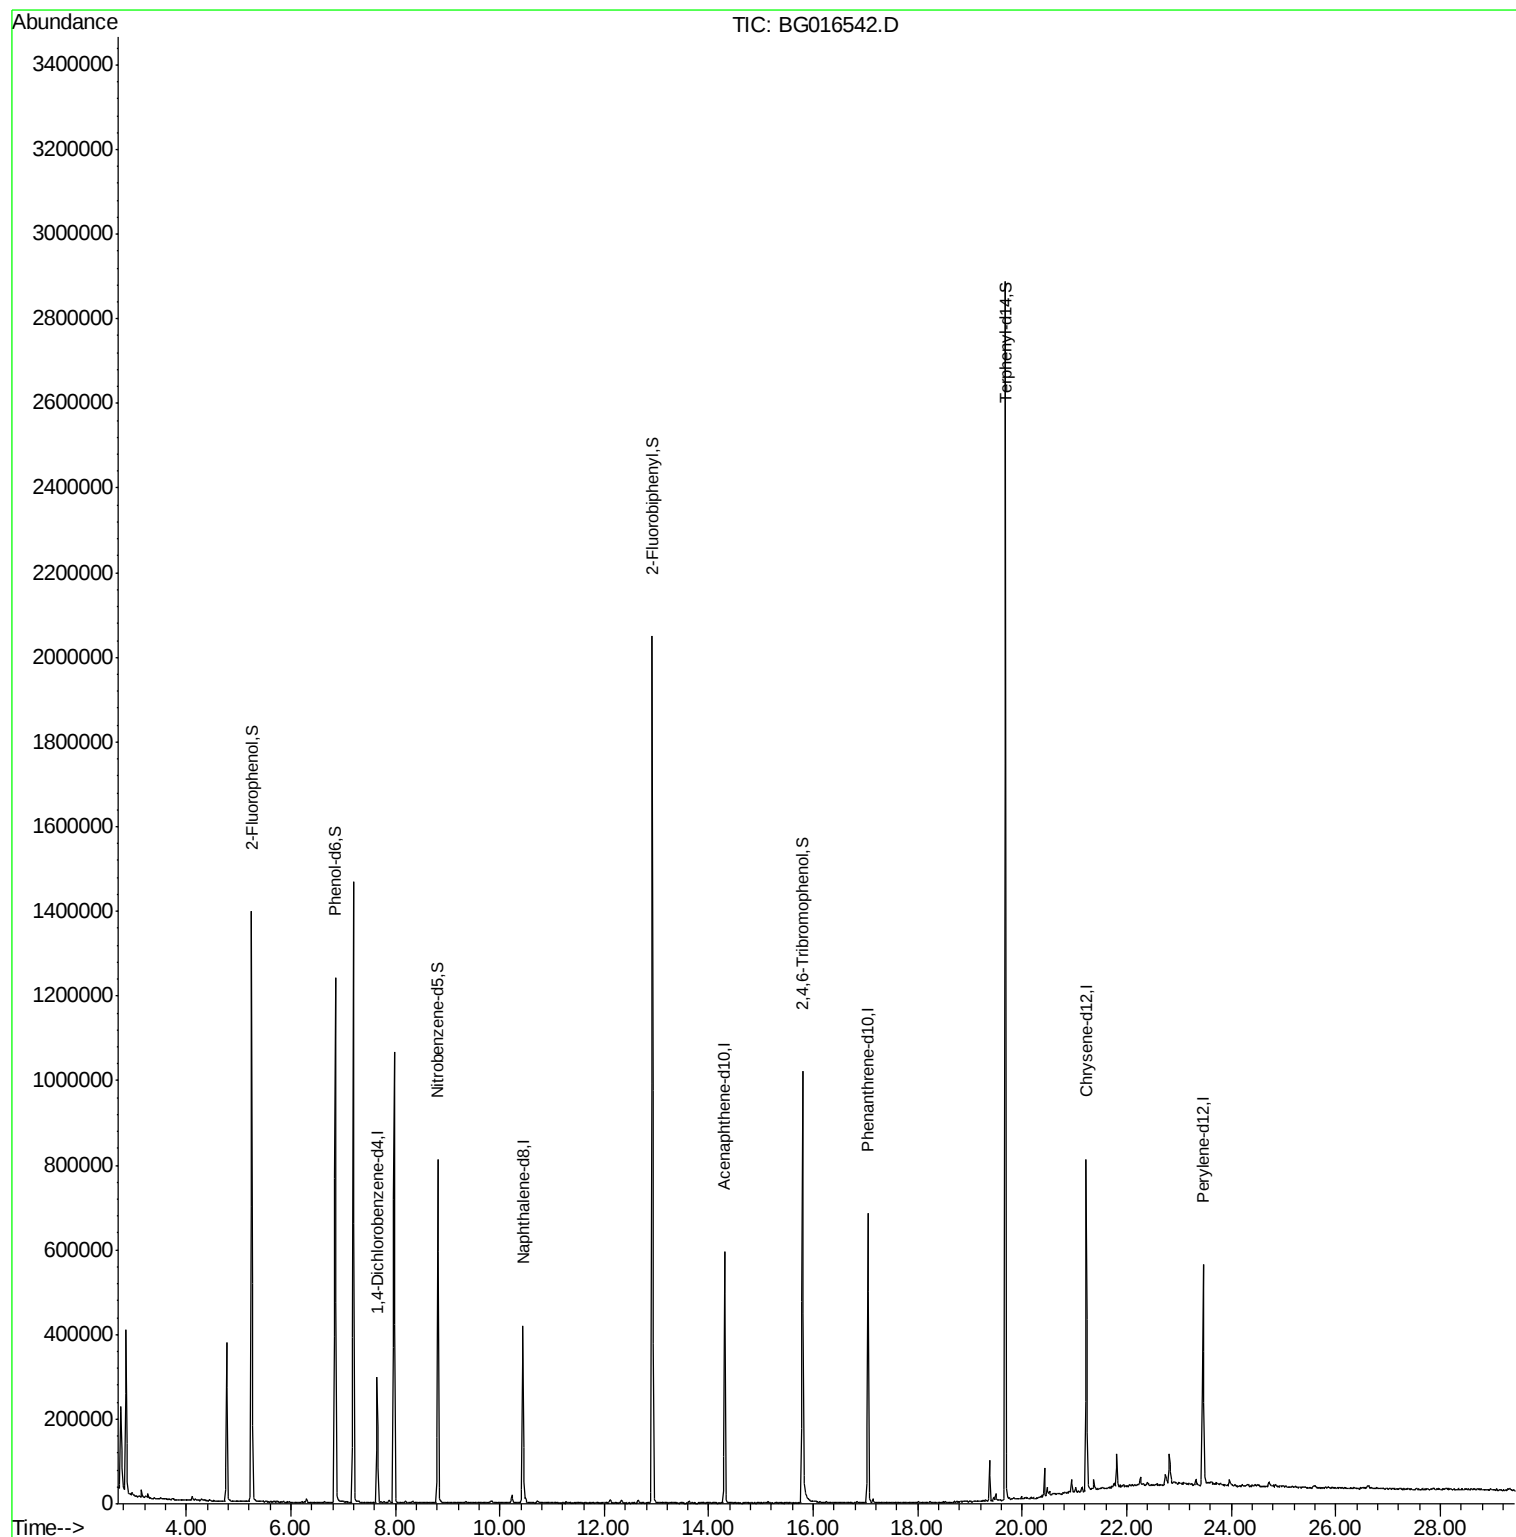

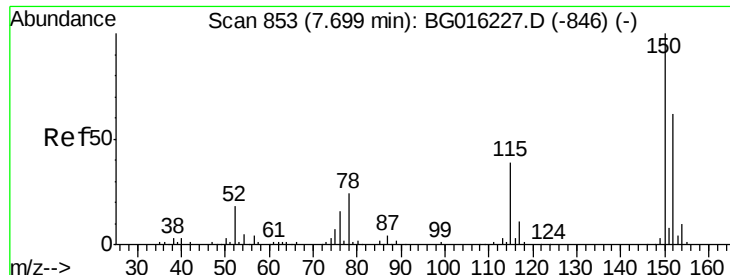

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.66 min Scan# 845

Delta R.T. -0.00 min

Lab File: BG016542.D

Acq: 19 Apr 2015 3:46

Instrument :

BNA_G

ClientSampleId :

WC-03(SB-04-14)


Tgt Ion:152 Resp: 82771

Ion Ratio Lower Upper

152 100

150 151.4 130.1 195.1




115 57.3 50.5 75.7

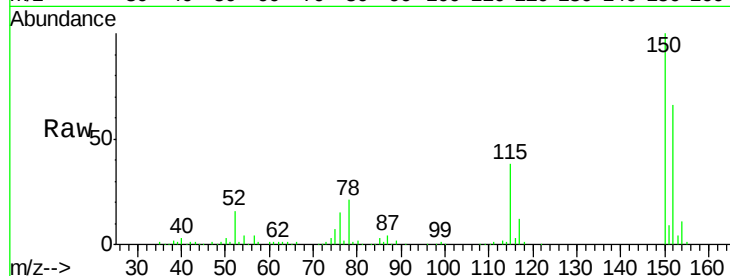

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

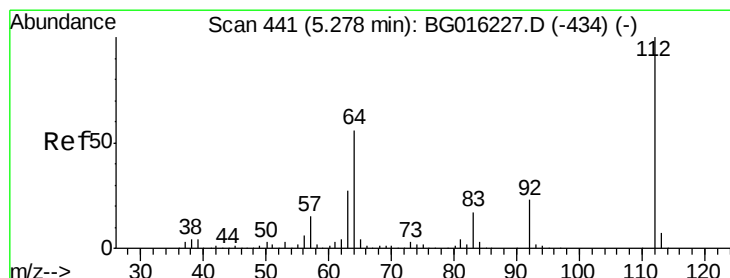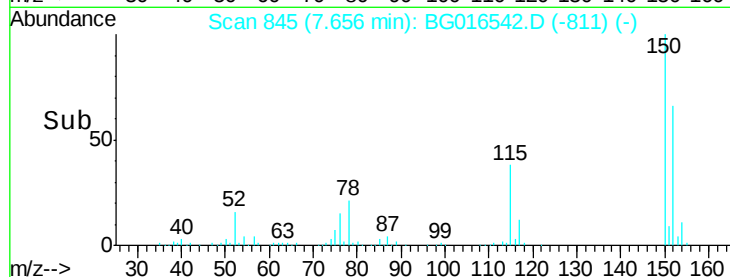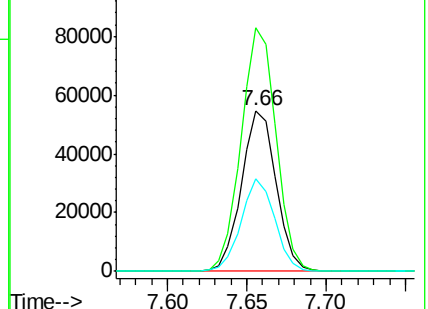

#5

2-Fluorophenol

Concen: 121.58 ng

RT: 5.25 min Scan# 436

Delta R.T. 0.00 min

Lab File: BG016542.D

Acq: 19 Apr 2015 3:46


Tgt Ion:112 Resp: 637636

Ion Ratio Lower Upper

112 100

64 52.5 44.5 66.7



63 25.1 21.4 32.0

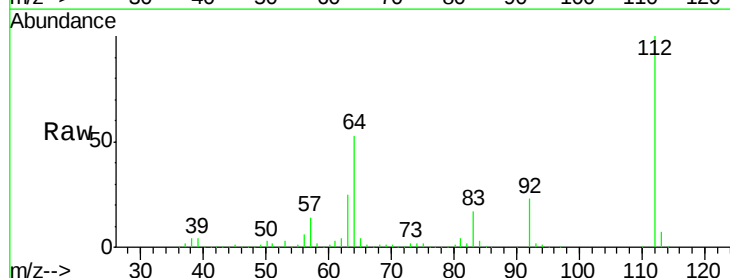

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

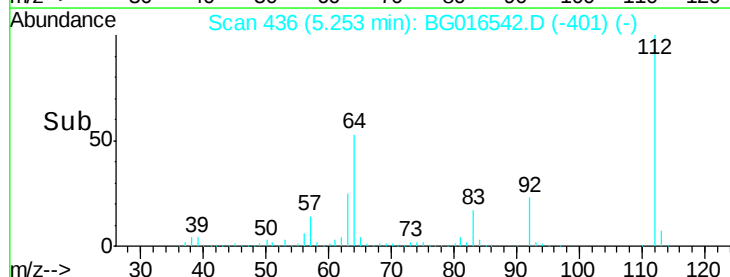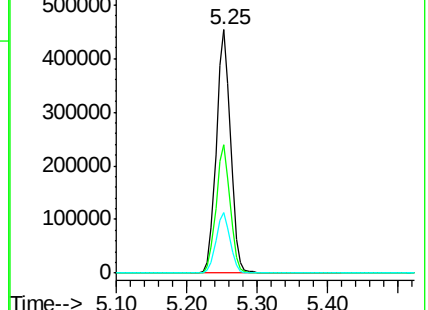



#7

Phenol-d6

Concen: 102.97 ng

RT: 6.85 min Scan# 708

Delta R.T. 0.00 min

Lab File: BG016542.D

Acq: 19 Apr 2015 3:46

Instrument :

BNA_G

ClientSampleId :

WC-03(SB-04-14)


Tgt Ion: 99 Resp: 810686

Ion Ratio Lower Upper



99 100

42 12.1 10.0 15.0

71 26.0 21.5 32.3

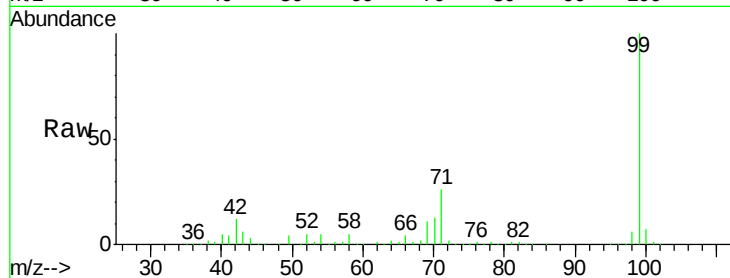

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

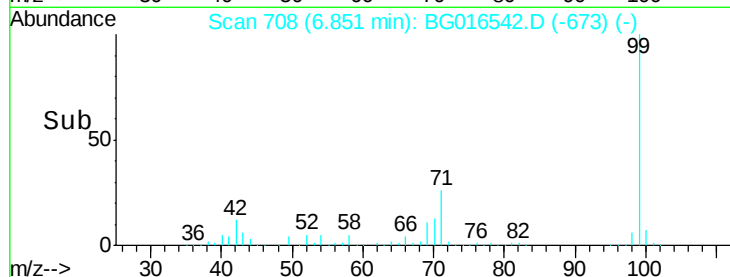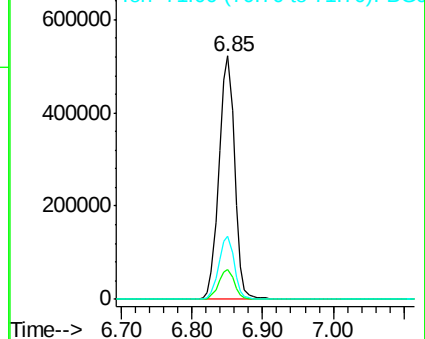

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.44 min Scan# 1319

Delta R.T. -0.00 min

Lab File: BG016542.D

Acq: 19 Apr 2015 3:46

Tgt Ion: 136 Resp: 345965


Ion Ratio Lower Upper

136 100



137 10.9 8.7 13.1

54 6.5 6.3 9.5

68 7.1 6.5 9.7

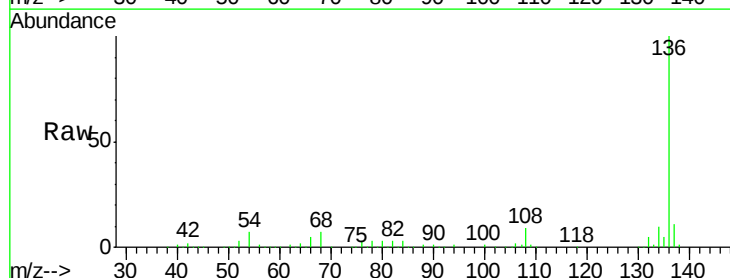

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



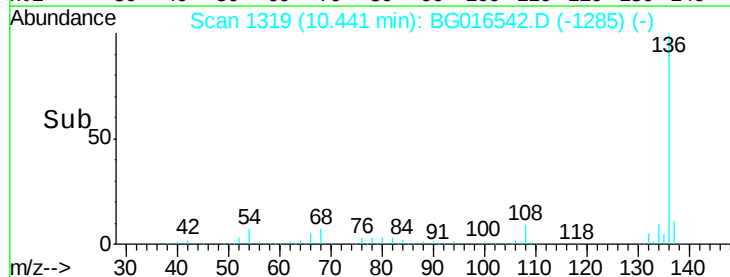
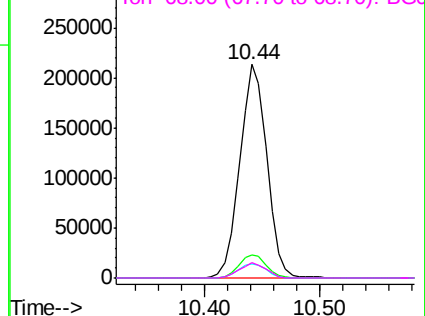




#23
 Nitrobenzene-d5
 Concen: 83.35 ng
 RT: 8.82 min Scan# 1043
 Delta R.T. 0.00 min
 Lab File: BG016542.D
 Acq: 19 Apr 2015 3:46




Instrument :
 BNA_G
 ClientSampleId :
 WC-03(SB-04-14)

Tgt Ion	Ratio	Lower	Upper
82	100		
128	53.6	37.8	56.8
54	40.0	32.6	49.0

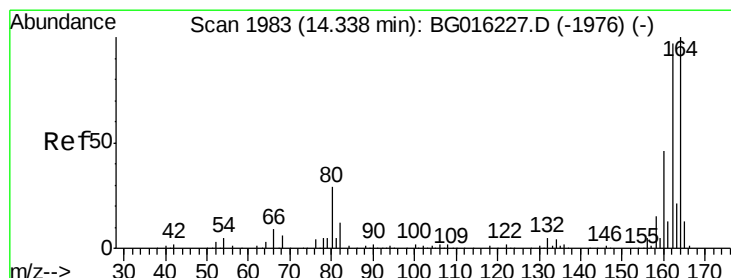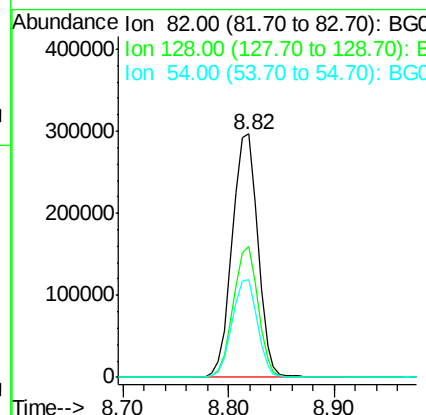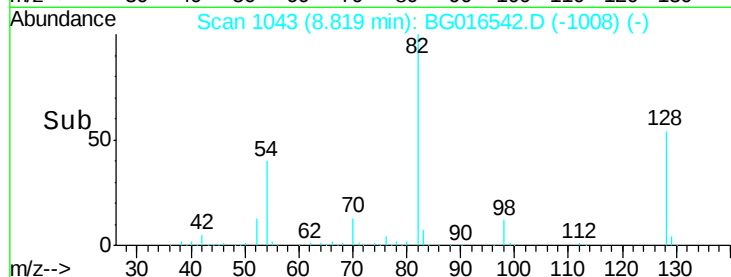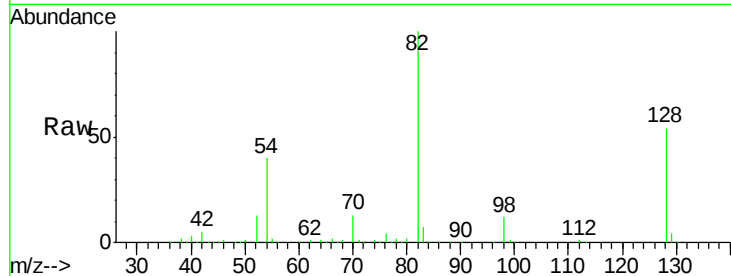

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.30 min Scan# 1976
 Delta R.T. -0.00 min
 Lab File: BG016542.D
 Acq: 19 Apr 2015 3:46

Tgt Ion	Ratio	Lower	Upper
164	100		
162	96.5	77.3	115.9
160	44.9	36.7	55.1

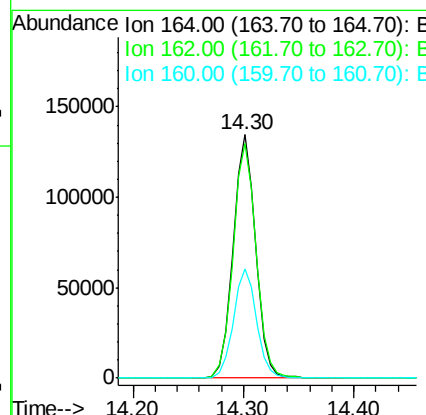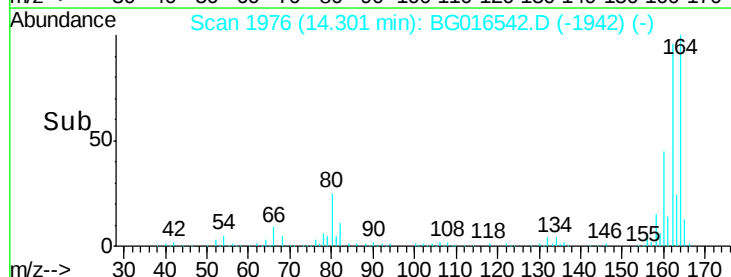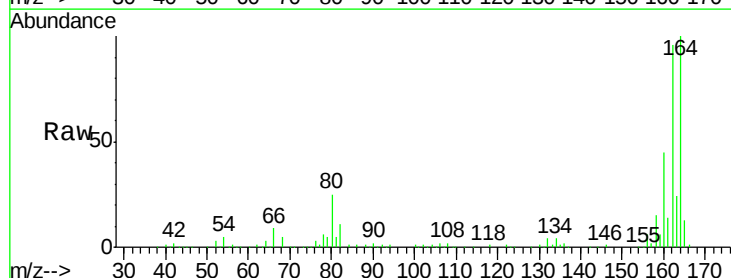







#41
 2,4,6-Tribromophenol
 Concen: 118.15 ng
 RT: 15.79 min Scan# 2230
 Delta R.T. -0.00 min
 Lab File: BG016542.D
 Acq: 19 Apr 2015 3:46

Instrument :
 BNA_G
 ClientSampleId :
 WC-03(SB-04-14)

Tgt Ion:330 Resp: 153818
 Ion Ratio Lower Upper
 330 100
 332 93.0 75.8 113.6
 141 57.4 46.6 69.8

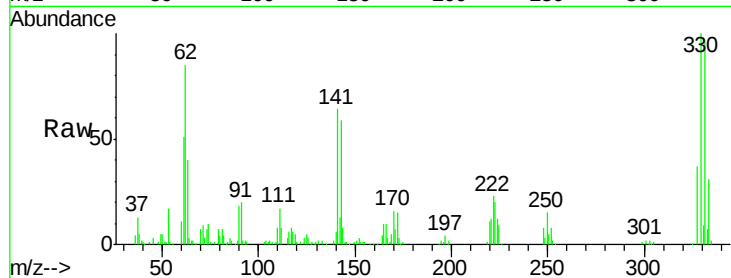


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

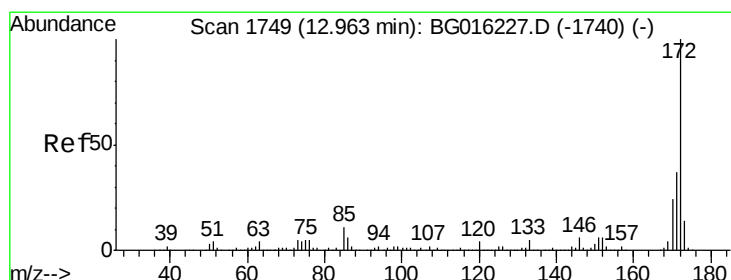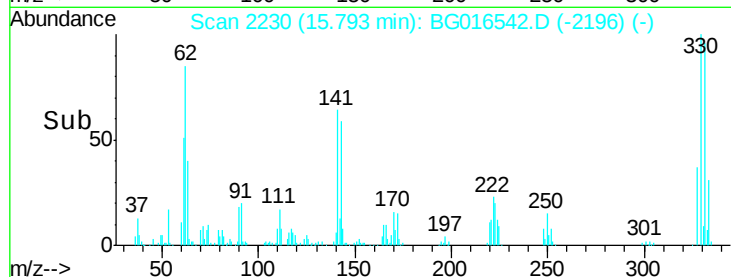
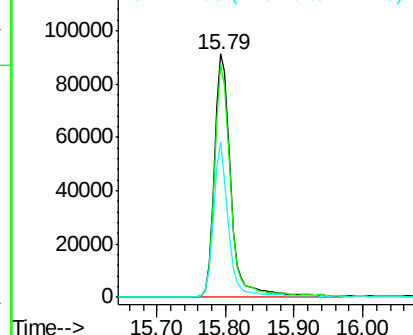


#44
 2-Fluorobiphenyl
 Concen: 87.53 ng
 RT: 12.92 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: BG016542.D
 Acq: 19 Apr 2015 3:46

Tgt Ion:172 Resp: 989690
 Ion Ratio Lower Upper
 172 100
 171 37.4 29.6 44.4
 170 25.0 19.4 29.2

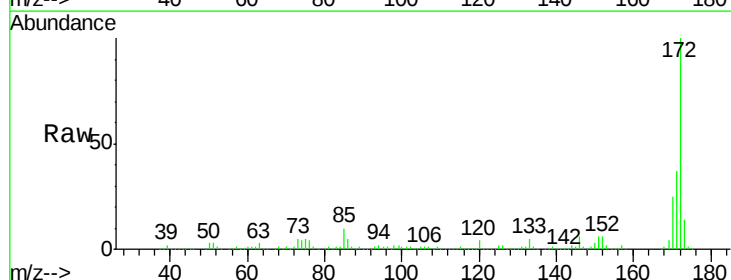

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

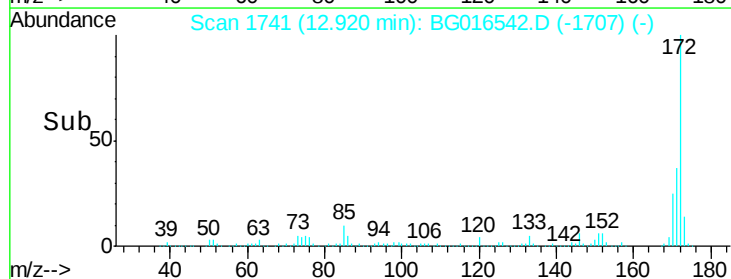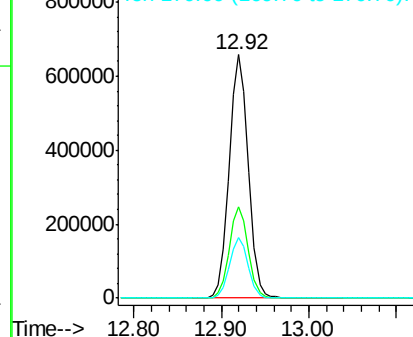







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.04 min Scan# 2443
Delta R.T. -0.00 min
Lab File: BG016542.D
Acq: 19 Apr 2015 3:46

Instrument :
BNA_G
ClientSampleId :
WC-03(SB-04-14)

Tgt Ion:188 Resp: 383247
Ion Ratio Lower Upper
188 100
94 14.0 12.2 18.4
80 14.0 12.8 19.2

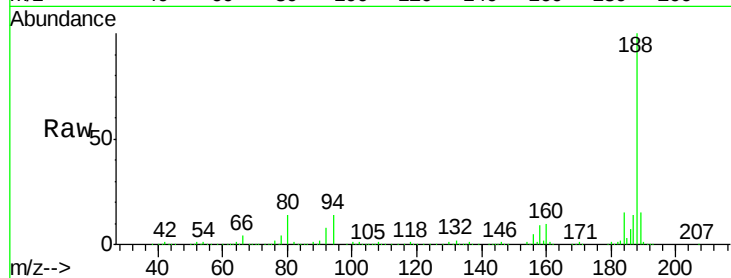


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

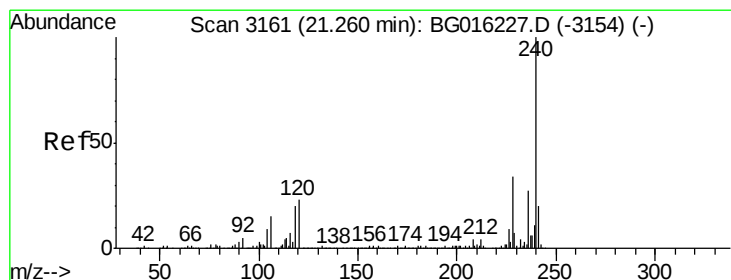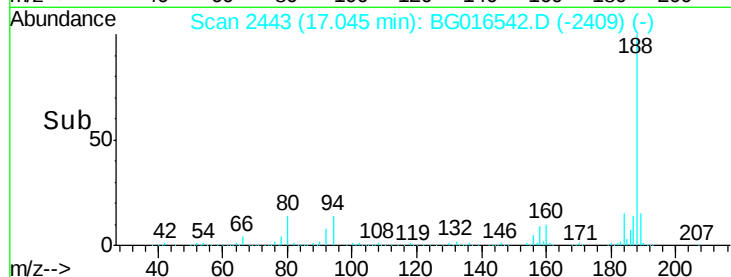
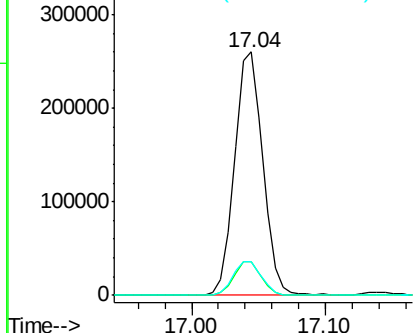



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.22 min Scan# 3154
Delta R.T. -0.01 min
Lab File: BG016542.D
Acq: 19 Apr 2015 3:46

Tgt Ion:240 Resp: 331723
Ion Ratio Lower Upper
240 100
120 22.6 18.6 28.0
236 26.0 21.7 32.5

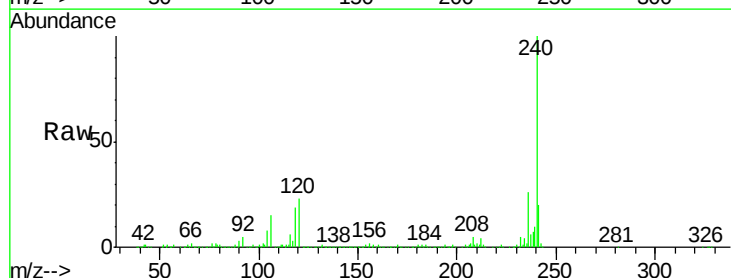

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

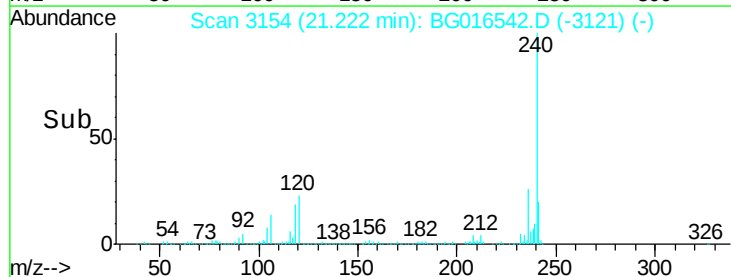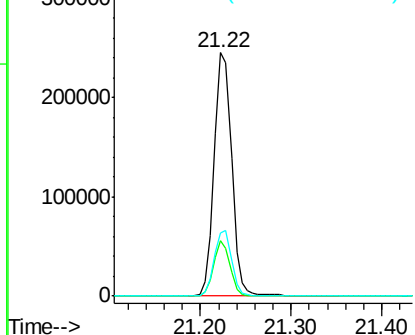

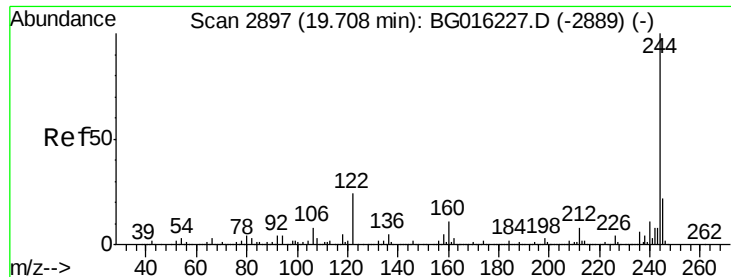

#78

Terphenyl-d14

Concen: 76.05 ng

RT: 19.68 min Scan# 2891

Delta R.T. 0.00 min

Lab File: BG016542.D

Acq: 19 Apr 2015 3:46

Instrument :

BNA_G

ClientSampleId :

WC-03(SB-04-14)


Tgt Ion:244 Resp: 1077869

Ion Ratio Lower Upper

244 100

212 8.9 6.6 9.8




122 23.0 19.1 28.7

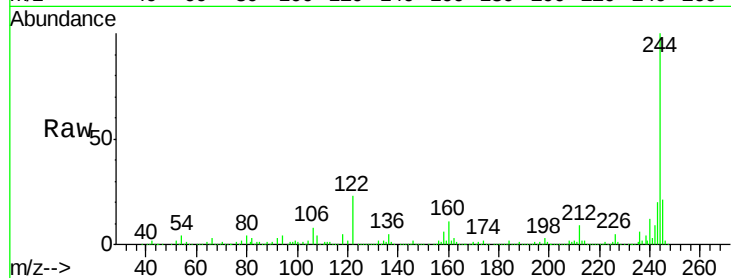

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

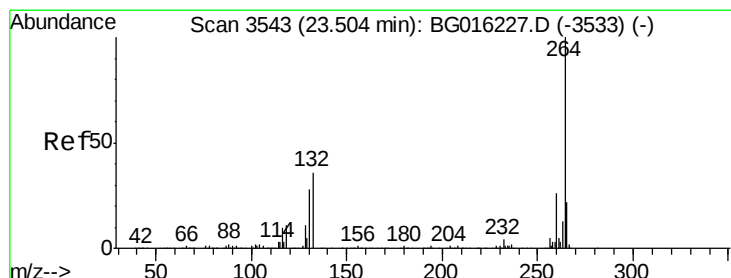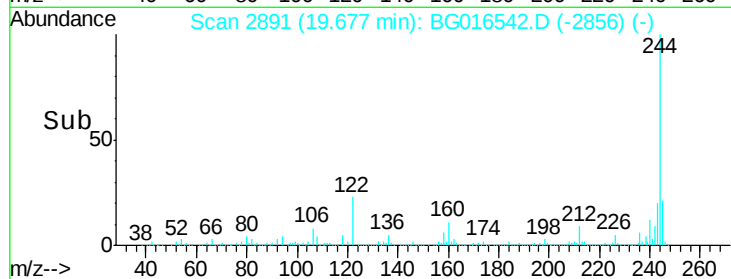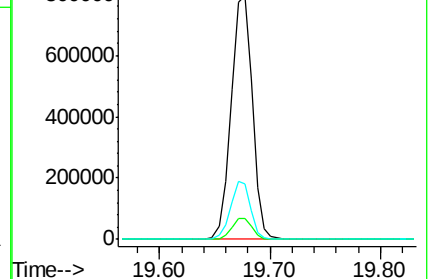

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.45 min Scan# 3534

Delta R.T. -0.00 min

Lab File: BG016542.D

Acq: 19 Apr 2015 3:46


Tgt Ion:264 Resp: 318644

Ion Ratio Lower Upper

264 100

260 25.1 20.4 30.6

265 21.9 17.2 25.8

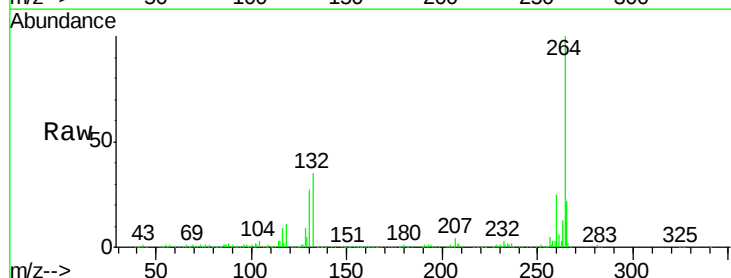

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

