


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016505.D
Acq On : 18 Apr 2015 3:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Apr 18 00:32:09 2015

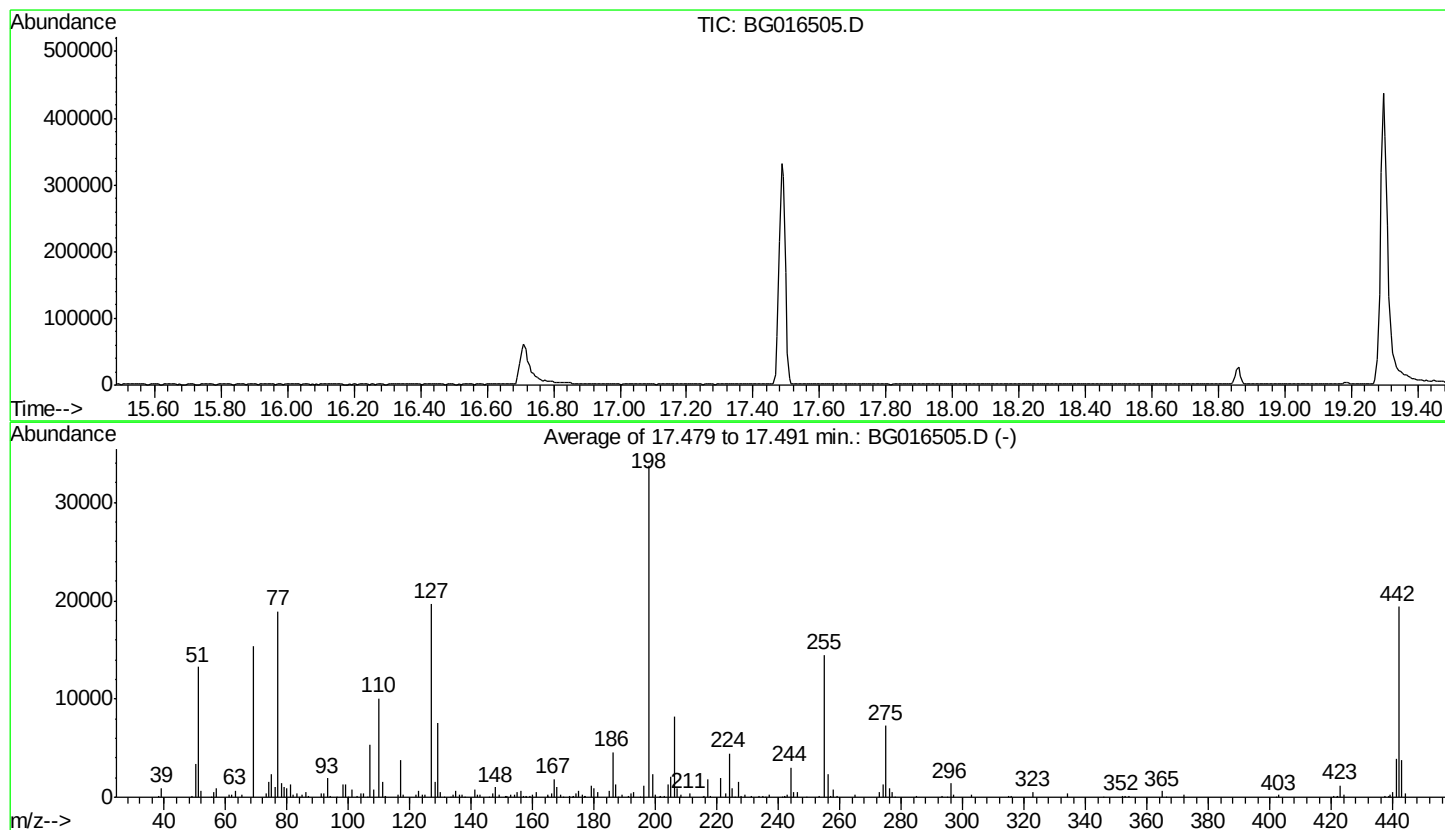

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	13282	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.5	15346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.3	19678	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33749	PASS
199	198	5	9	7.1	2404	PASS
275	198	10	60	21.4	7238	PASS
365	198	1	100	1.8	592	PASS
441	442	0.01	24	20.0	3873	PASS
442	198	50	100	57.5	19394	PASS
443	442	15	24	19.6	3802	PASS