


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
 Data File : BG016526.D
 Acq On : 18 Apr 2015 17:54
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 14 14:00:56 2015

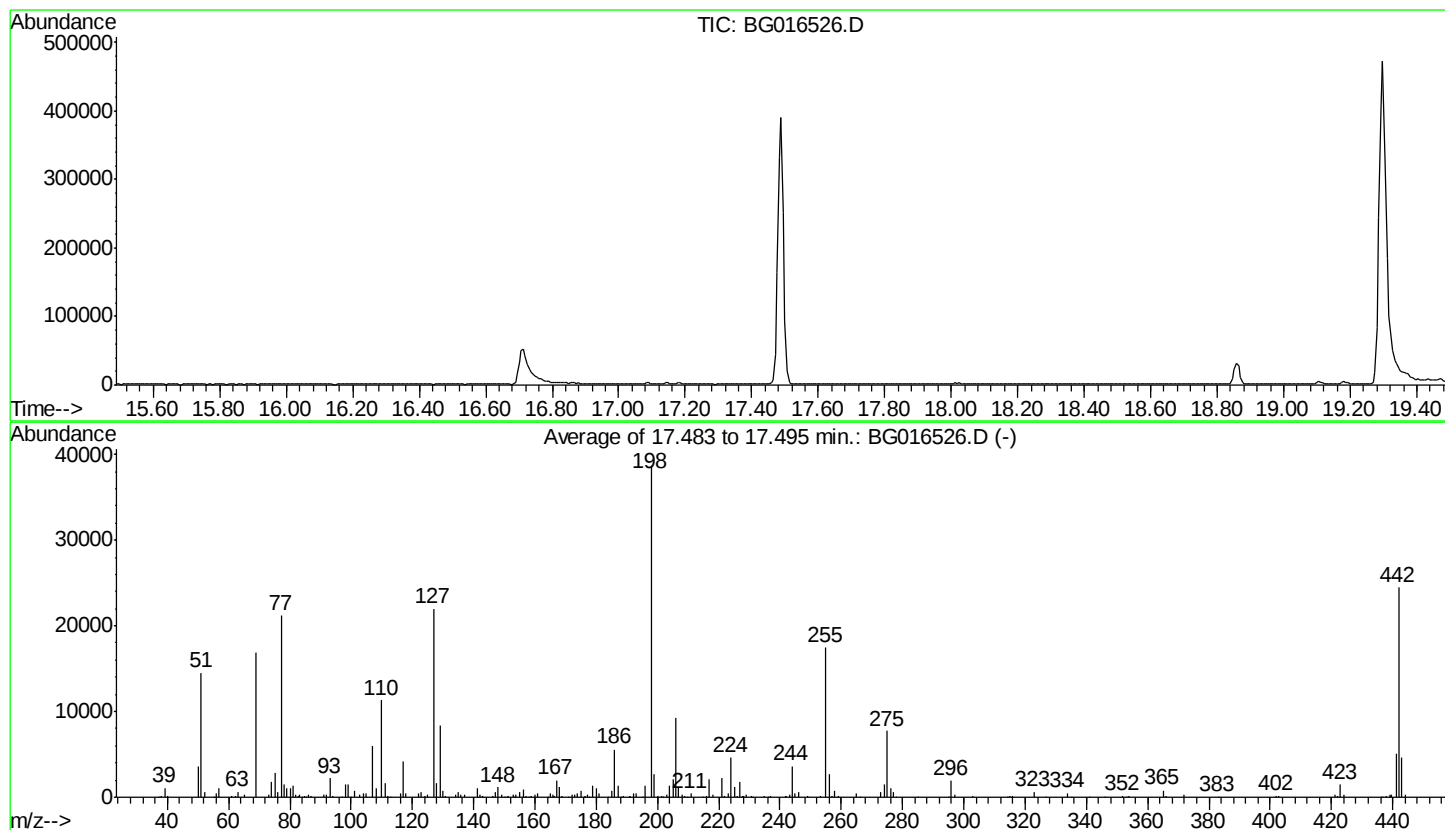

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	14522	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.7	16892	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.9	21992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38682	PASS
199	198	5	9	7.0	2692	PASS
275	198	10	60	19.9	7709	PASS
365	198	1	100	2.1	815	PASS
441	442	0.01	24	21.0	5140	PASS
442	198	50	100	63.3	24474	PASS
443	442	15	24	18.9	4628	PASS