
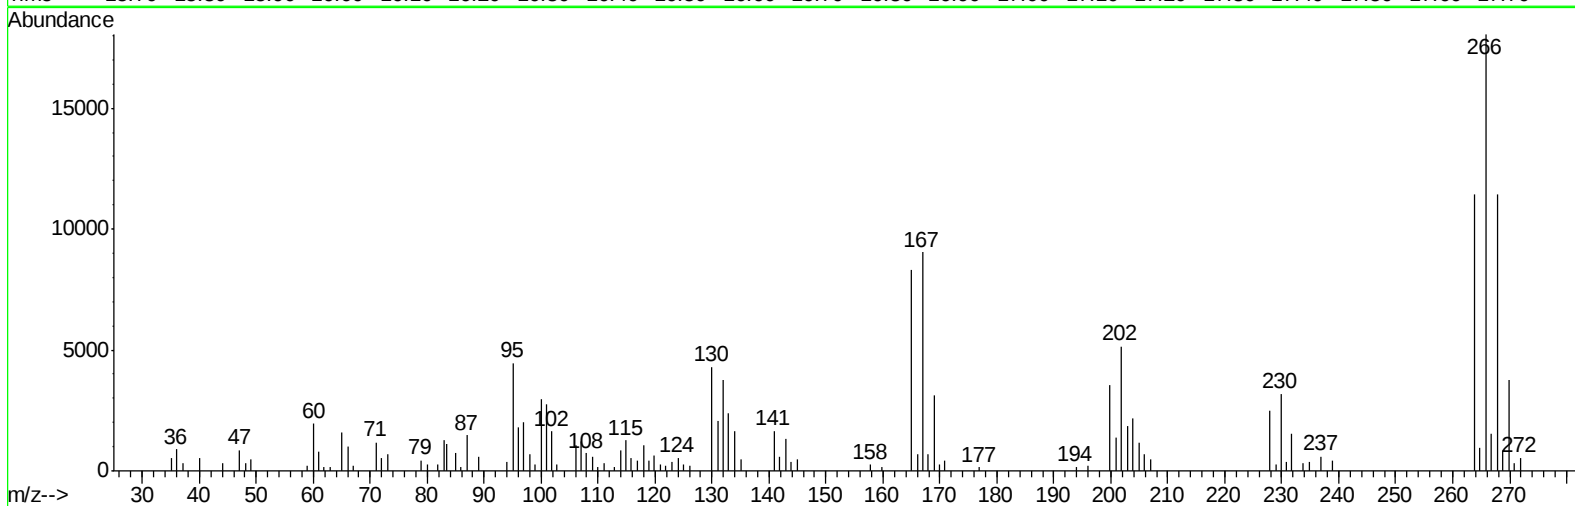


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016486.D
Acq On : 17 Apr 2015 11:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:23:50 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

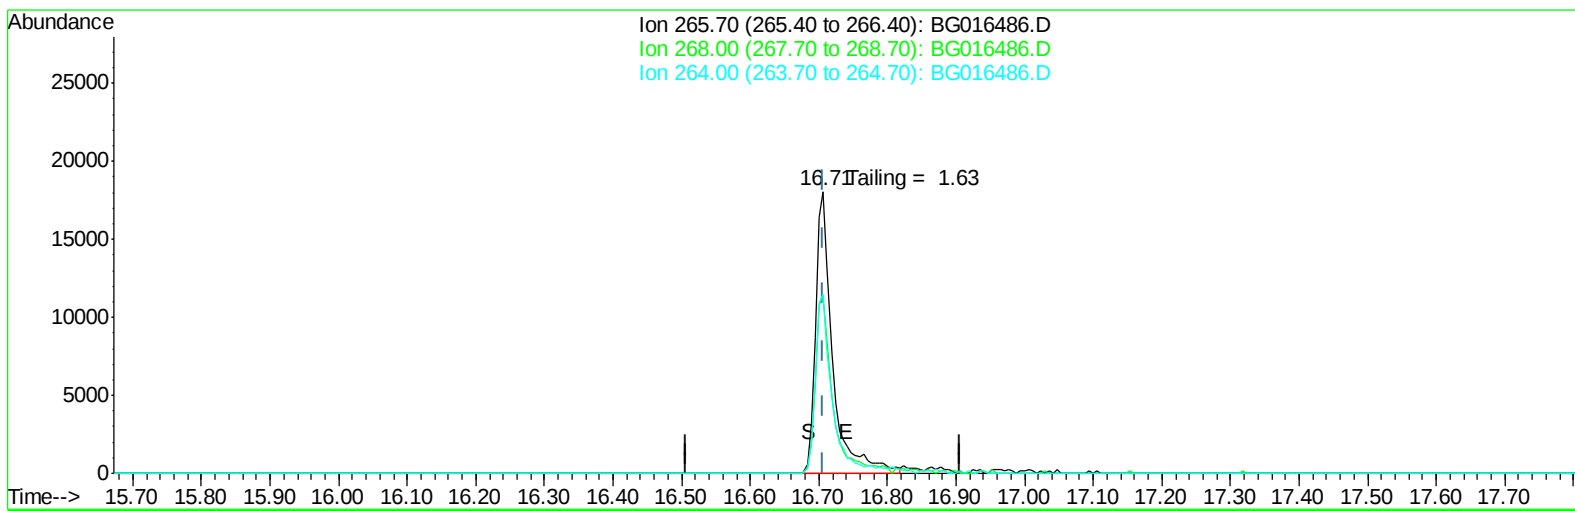

TIC: BG016486.D

(69) Pentachlorophenol (C)



16.706min (-0.001) 94283.69ng

response 31054

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.23
264.00	66.00	63.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016486.D
Acq On : 17 Apr 2015 11:53
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:23:50 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

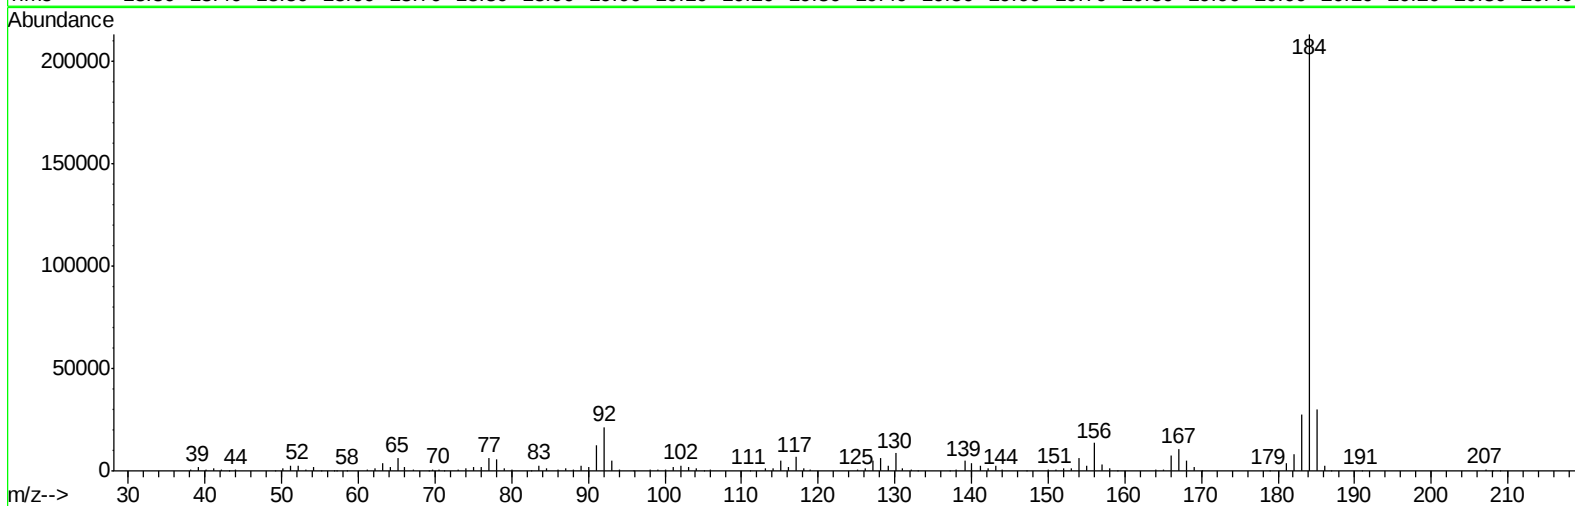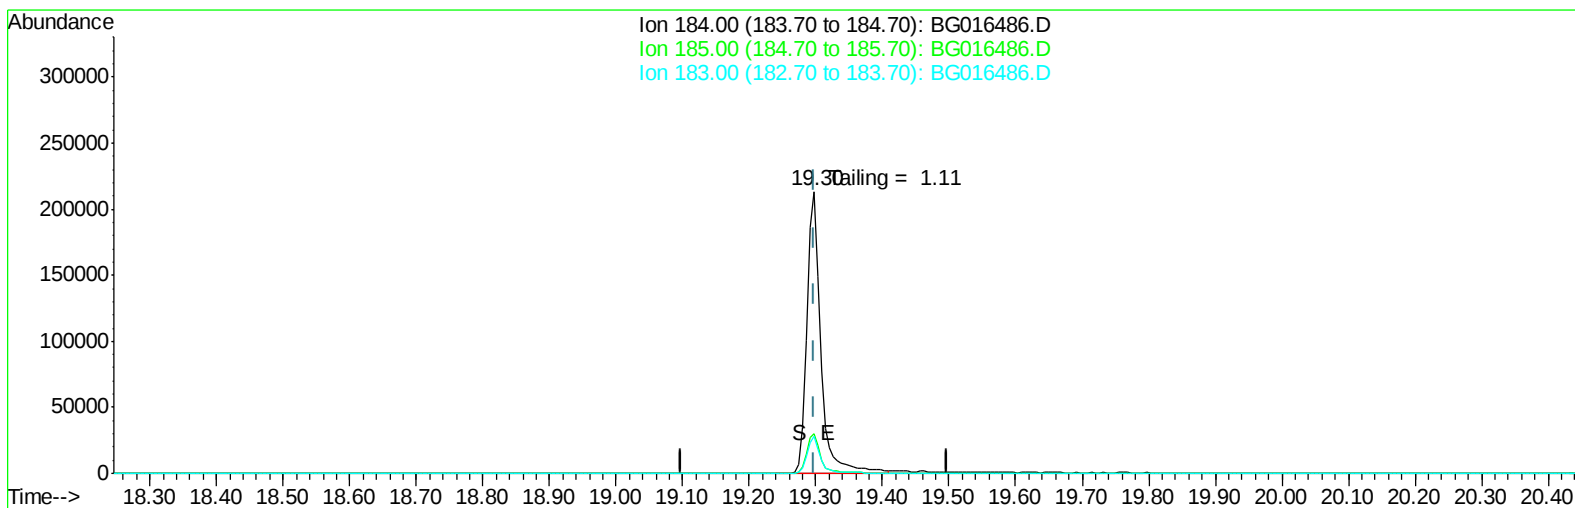

TIC: BG016486.D

(76) Benzidine

19.297min (-0.001) 17114.09ng

response 319336

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.07
183.00	13.00	12.98
0.00	0.00	0.00