
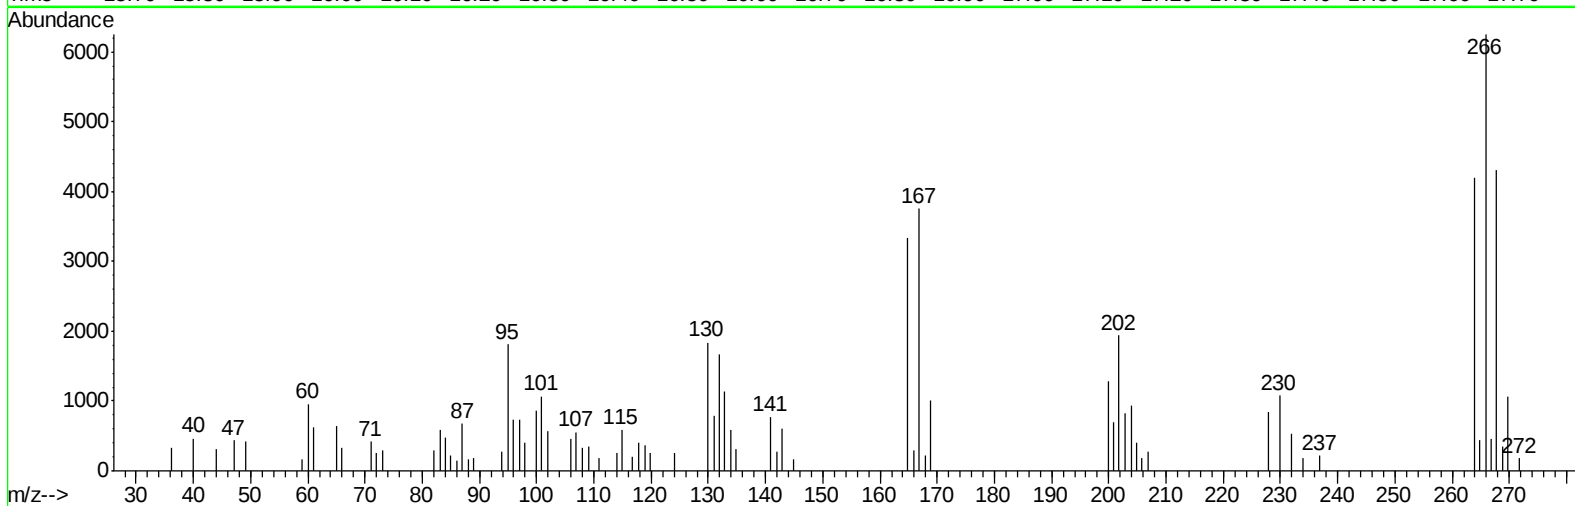


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016505.D
Acq On : 18 Apr 2015 3:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:34:37 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

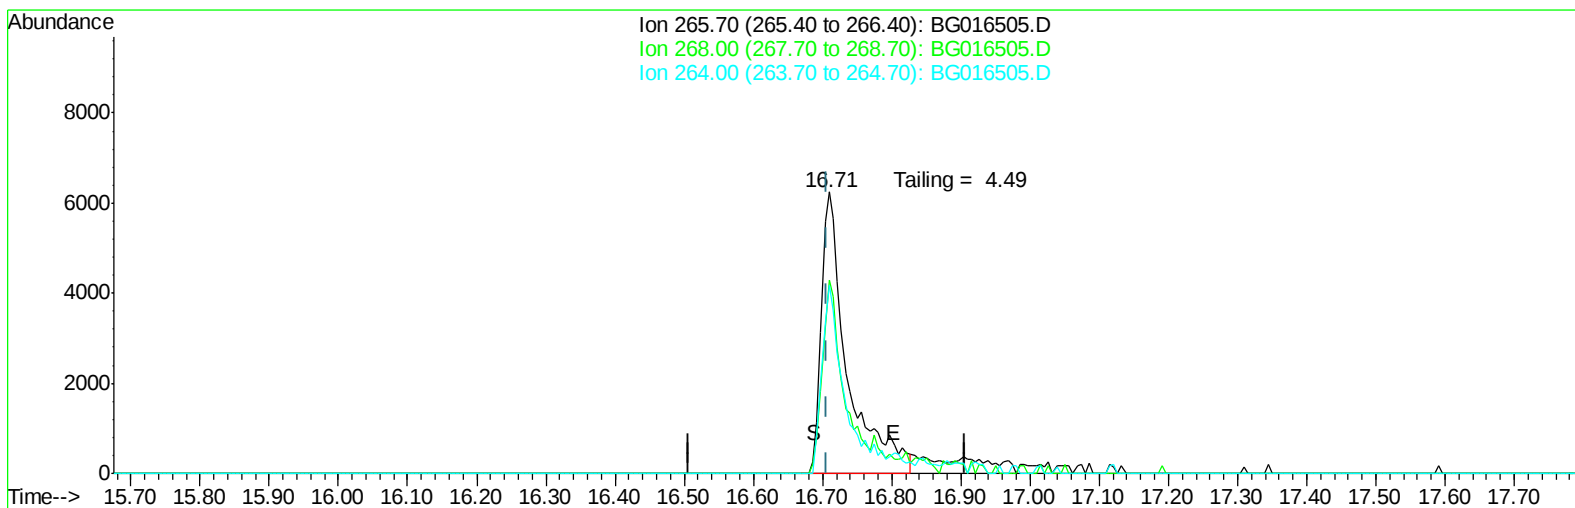

TIC: BG016505.D

(69) Pentachlorophenol (C)



16.709min (+0.003) 0.00ng m

response 16234

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	68.86
264.00	66.00	67.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016505.D
Acq On : 18 Apr 2015 3:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:34:37 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

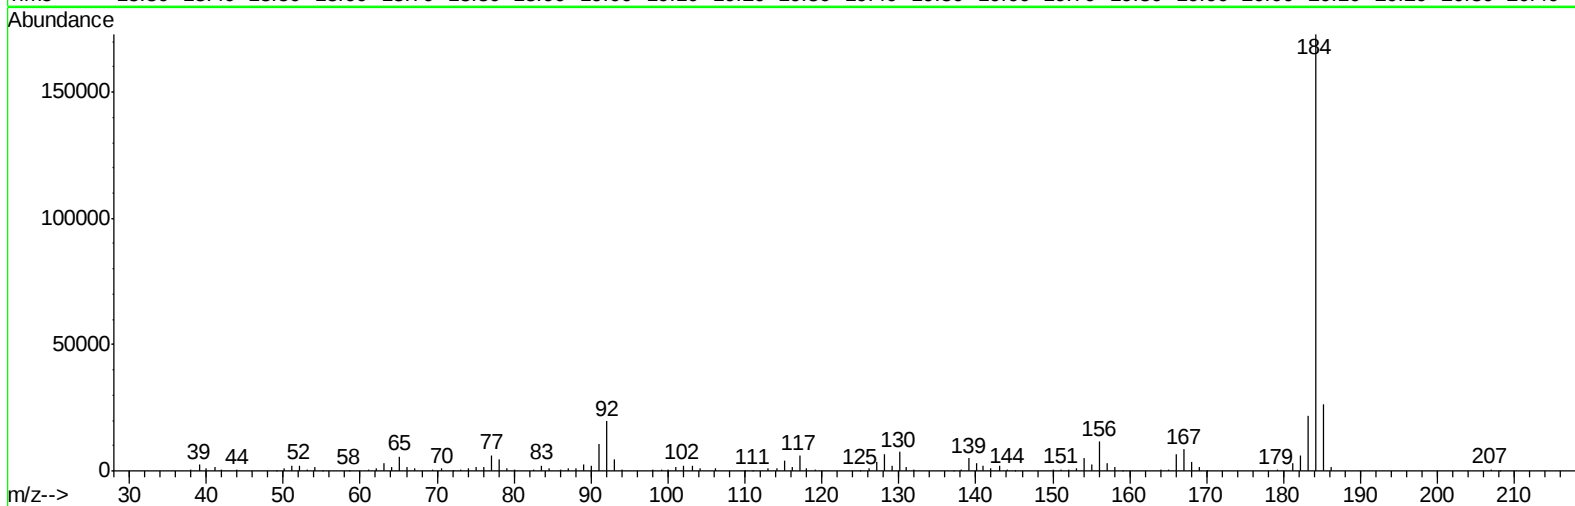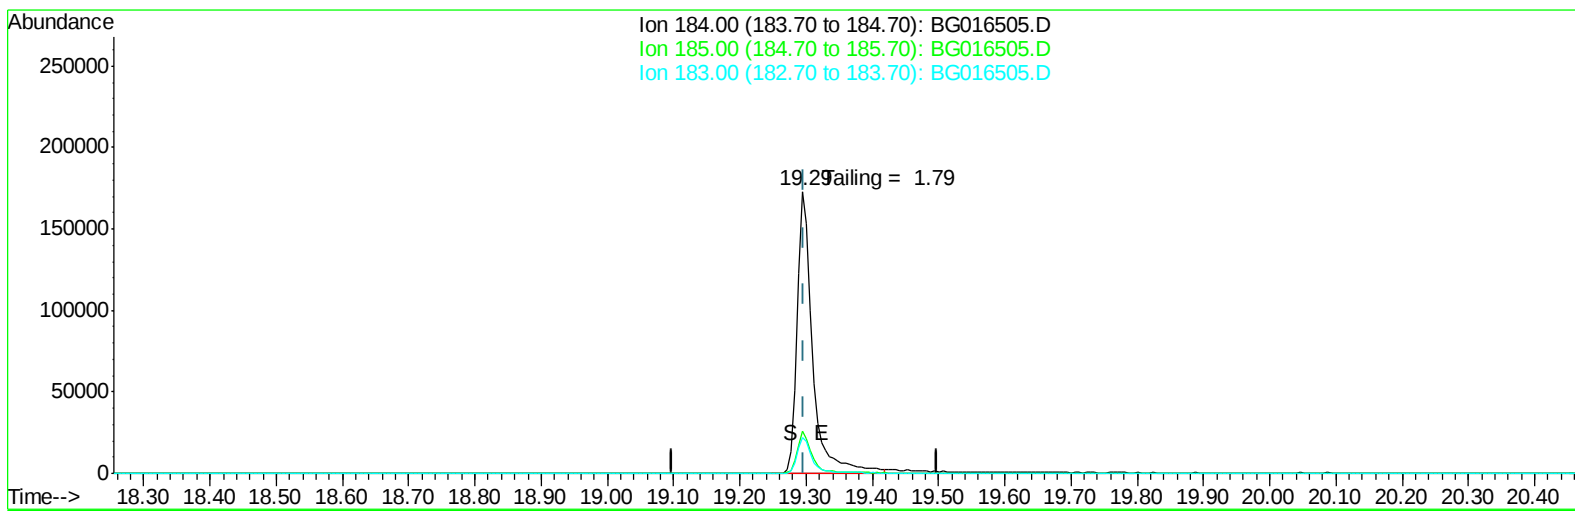

TIC: BG016505.D

(76) Benzidine

19.295min (-0.003) 19481.97ng m

response 285858

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.19
183.00	13.00	12.75
0.00	0.00	0.00