
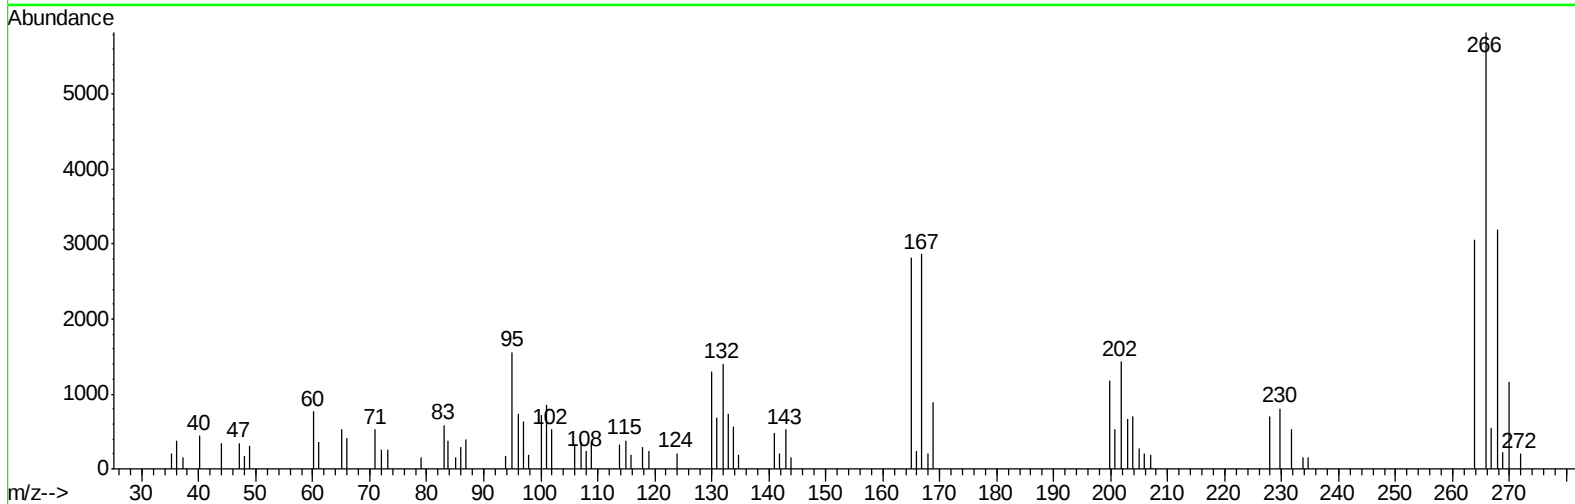


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016526.D
Acq On : 18 Apr 2015 17:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:35:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

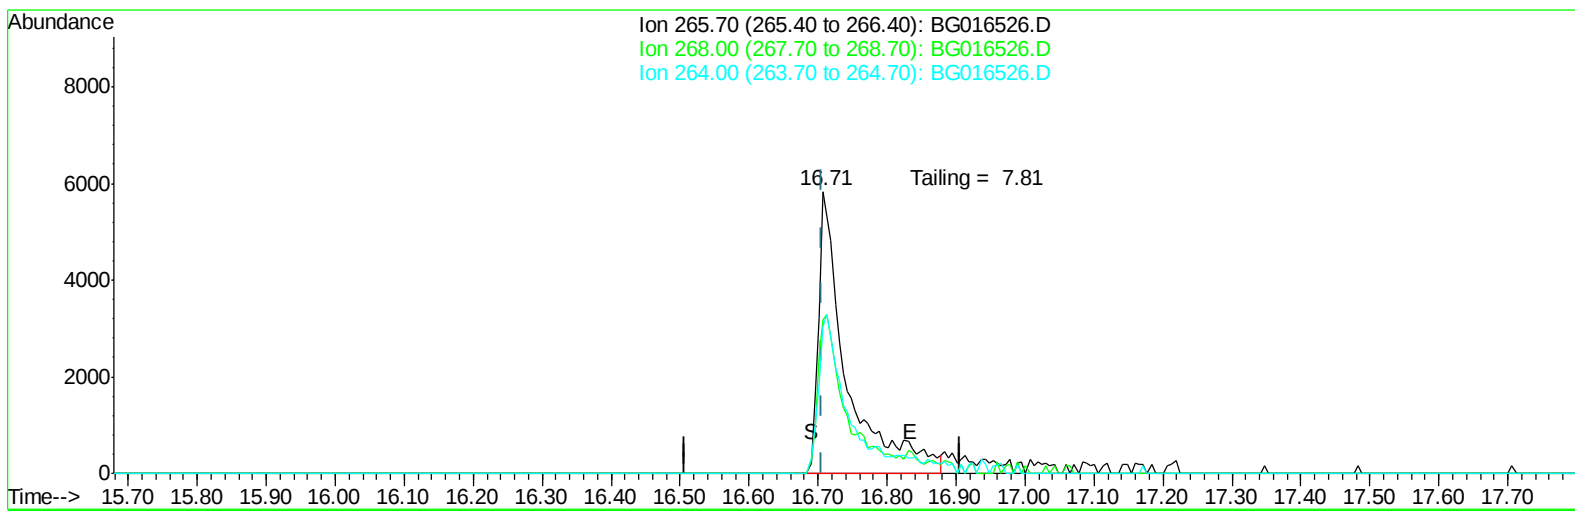

TIC: BG016526.D

(69) Pentachlorophenol (C)



16.707min (+0.000) 8616.12ng

response 14364

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	58.65
264.00	66.00	52.39#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016526.D
Acq On : 18 Apr 2015 17:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 20 07:35:52 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 20 03:57:28 2015
Response via : Initial Calibration

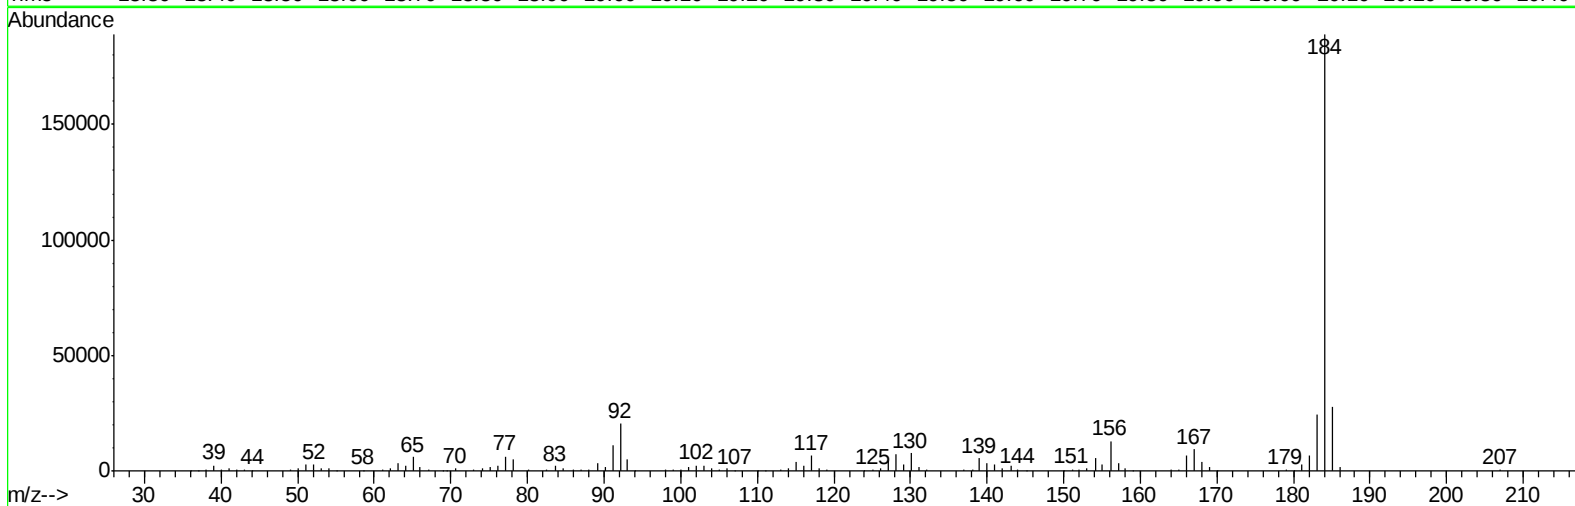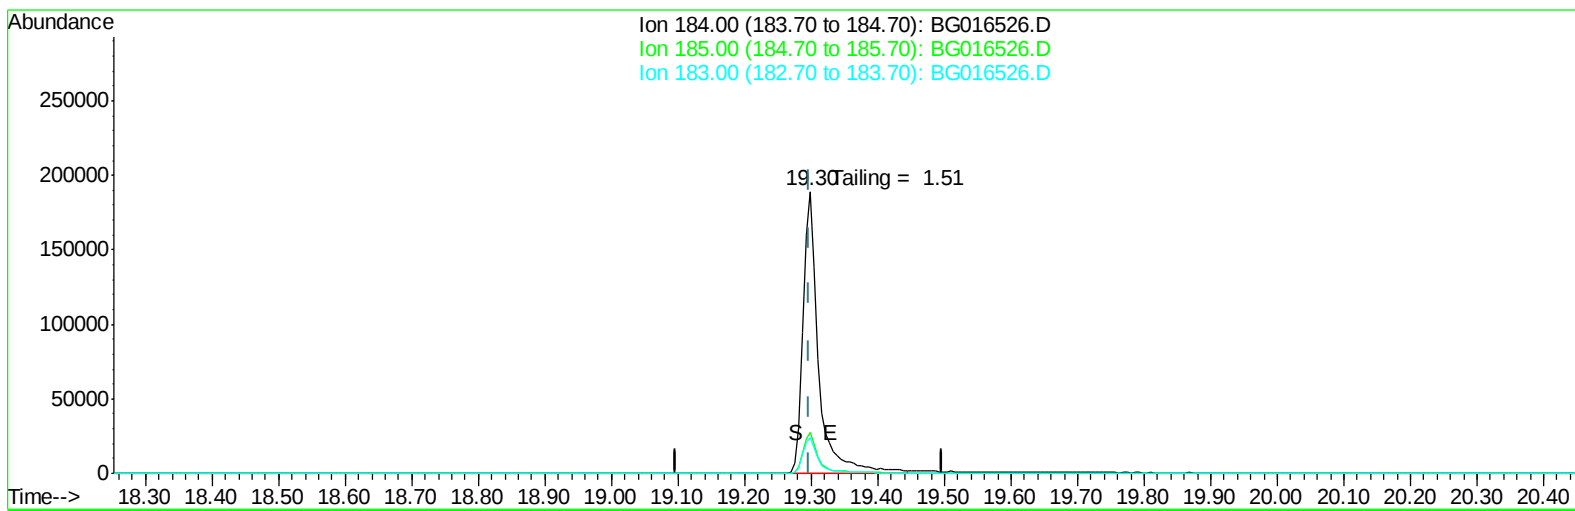

TIC: BG016526.D

(76) Benzidine

19.298min (+0.000) 15630.10ng

response 314182

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.53
183.00	13.00	12.80
0.00	0.00	0.00