

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
 Data File : BG016488.D
 Acq On : 17 Apr 2015 14:15
 Operator : TP/IZ
 Sample : PB82828BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB82828BL

Quant Time: Apr 18 00:48:35 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 18 00:32:09 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	67137	20.00	ng	0.00
21) Naphthalene-d8	10.44	136	285790	20.00	ng	0.00
38) Acenaphthene-d10	14.30	164	166177	20.00	ng	0.00
63) Phenanthrene-d10	17.04	188	359197	20.00	ng	0.00
75) Chrysene-d12	21.23	240	310399	20.00	ng	0.00
86) Perylene-d12	23.45	264	291643	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	470925	110.70	ng	0.00
7) Phenol-d6	6.84	99	629524	98.58	ng	0.00
23) Nitrobenzene-d5	8.81	82	317207	64.30	ng	0.00
41) 2,4,6-Tribromophenol	15.80	330	126713	112.75	ng	0.00
44) 2-Fluorobiphenyl	12.92	172	705874	72.32	ng	0.00
78) Terphenyl-d14	19.68	244	874364	65.93	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG041715\
Data File : BG016488.D
Acq On : 17 Apr 2015 14:15
Operator : TP/IZ
Sample : PB82828BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82828BL

Quant Time: Apr 18 00:48:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 18 00:32:09 2015
Response via : Initial Calibration

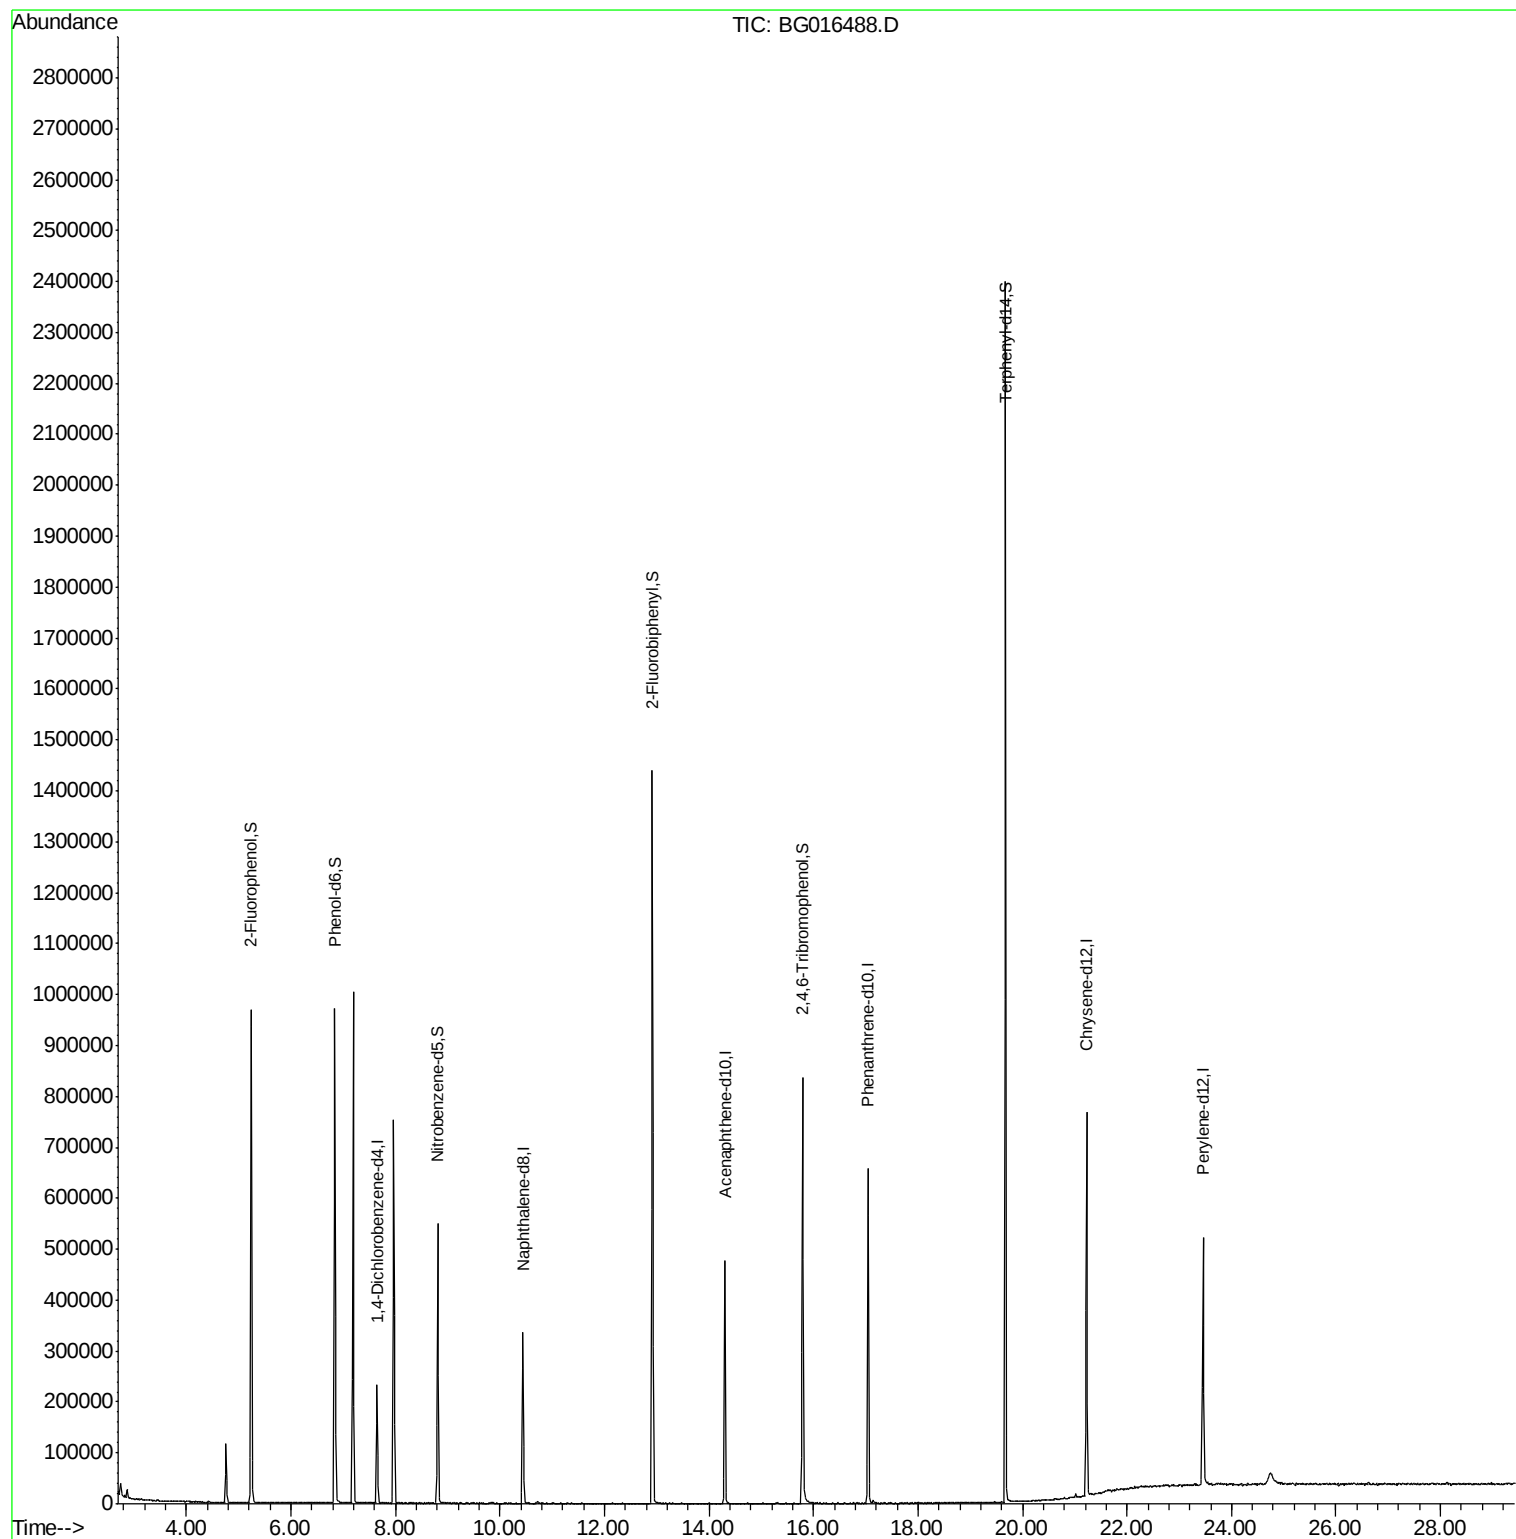

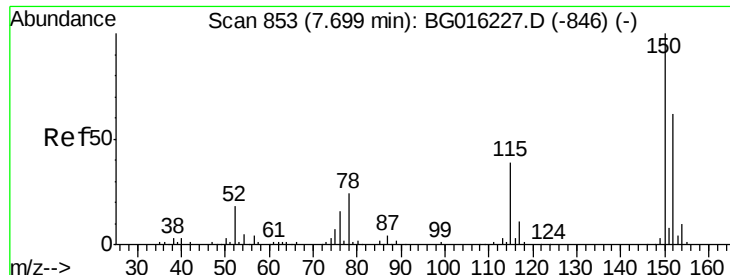


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.65 min Scan# 845
 Delta R.T. 0.00 min
 Lab File: BG016488.D
 Acq: 17 Apr 2015 14:15

Instrument :
 BNA_G
 ClientSampleId :
 PB82828BL

Tgt Ion:152 Resp: 67137
 Ion Ratio Lower Upper
 152 100
 150 151.2 130.1 195.1
 115 54.1 50.5 75.7

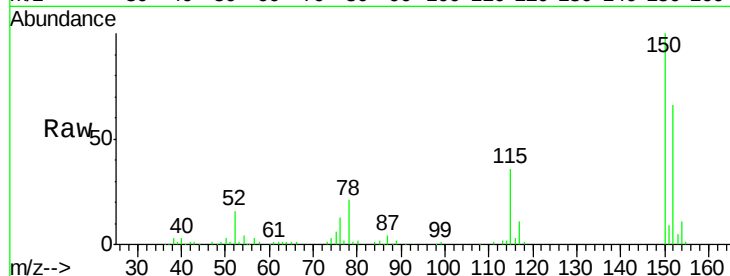


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

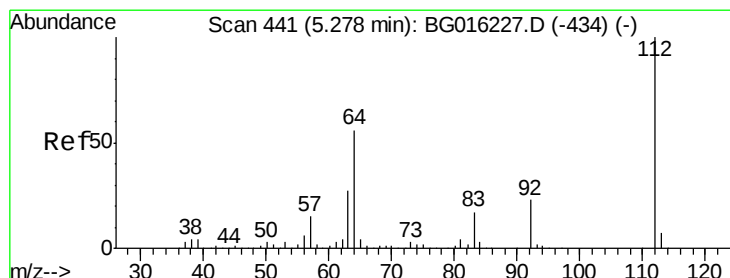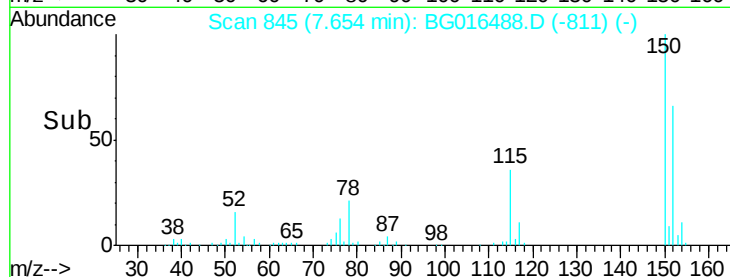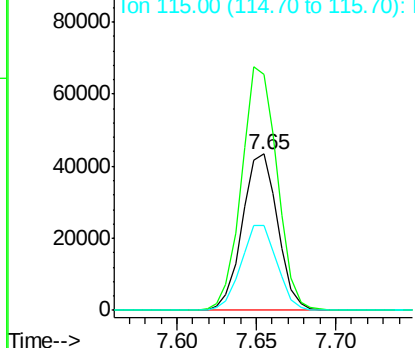



#5


2-Fluorophenol
 Concen: 110.70 ng
 RT: 5.24 min Scan# 434
 Delta R.T. -0.00 min
 Lab File: BG016488.D
 Acq: 17 Apr 2015 14:15

Tgt Ion:112 Resp: 470925
 Ion Ratio Lower Upper
 112 100
 64 51.7 44.5 66.7
 63 24.4 21.4 32.0

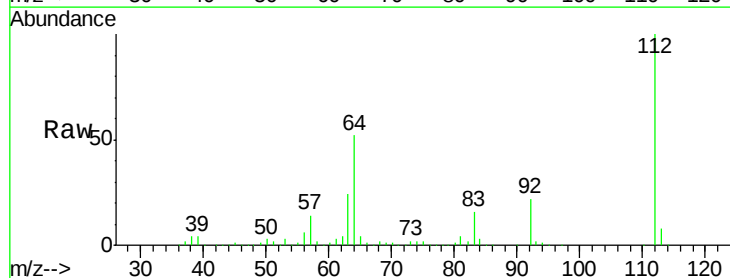

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

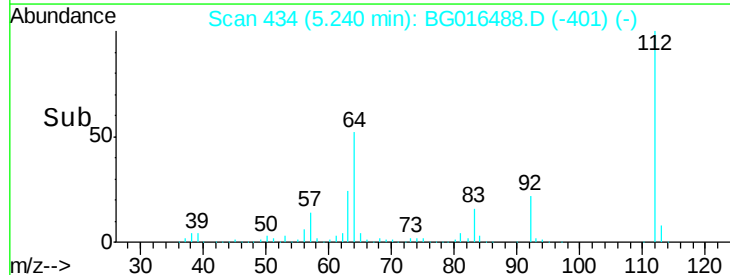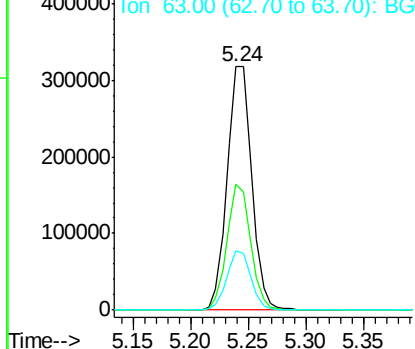

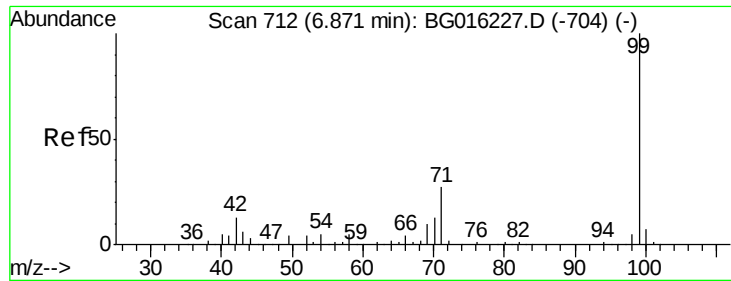

#7

Phenol-d6

Concen: 98.58 ng

RT: 6.84 min Scan# 707

Delta R.T. 0.00 min

Lab File: BG016488.D

Acq: 17 Apr 2015 14:15

Instrument :

BNA_G

ClientSampled :

PB82828BL


Tgt Ion: 99 Resp: 629524

Ion Ratio Lower Upper




99 100

42 11.6 10.0 15.0

71 26.1 21.5 32.3

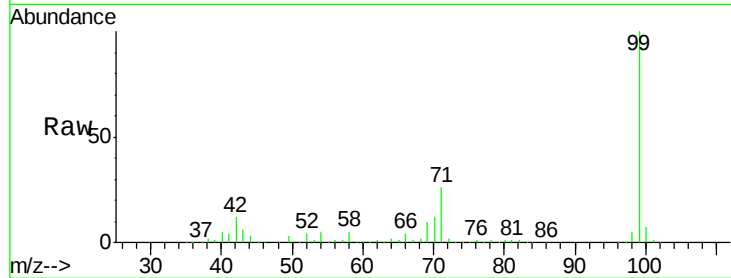

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

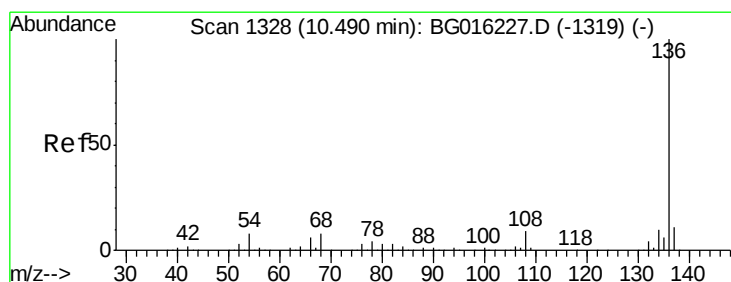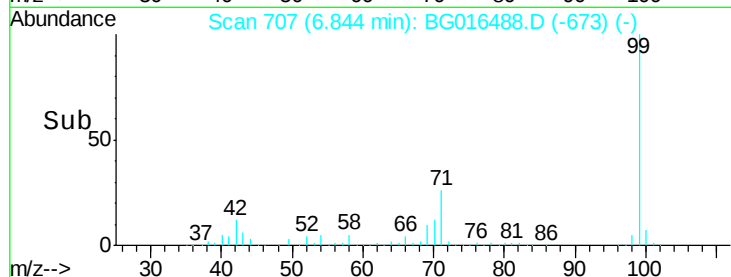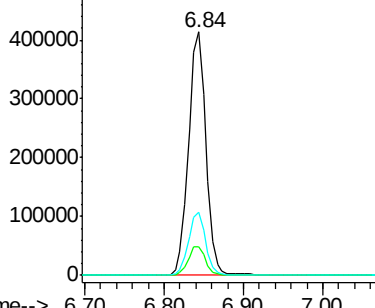

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.44 min Scan# 1319

Delta R.T. -0.00 min

Lab File: BG016488.D

Acq: 17 Apr 2015 14:15

Tgt Ion: 136 Resp: 285790


Ion Ratio Lower Upper

136 100



137 11.2 8.7 13.1

54 7.0 6.3 9.5

68 7.0 6.5 9.7

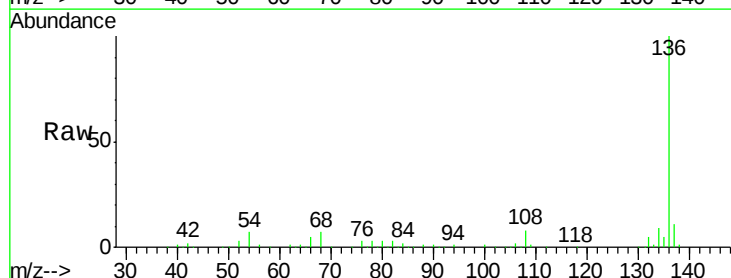

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

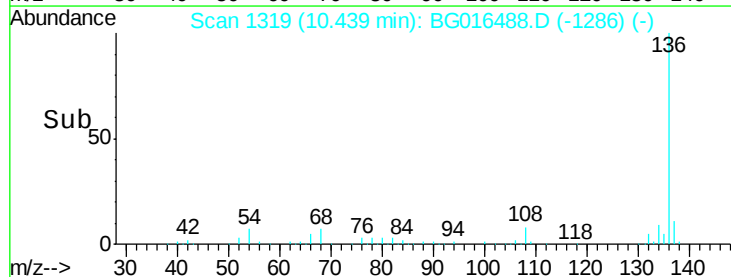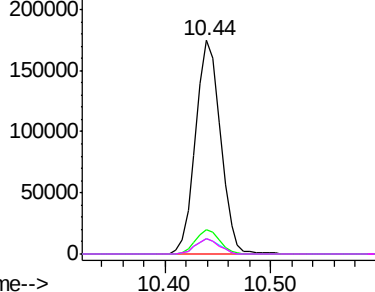






#23
 Nitrobenzene-d5
 Concen: 64.30 ng
 RT: 8.81 min Scan# 1042
 Delta R.T. -0.00 min
 Lab File: BG016488.D
 Acq: 17 Apr 2015 14:15

Instrument :
 BNA_G
 ClientSampled :
 PB82828BL

Tgt Ion: 82 Resp: 317207
 Ion Ratio Lower Upper
 82 100
 128 52.3 37.8 56.8
 54 37.6 32.6 49.0

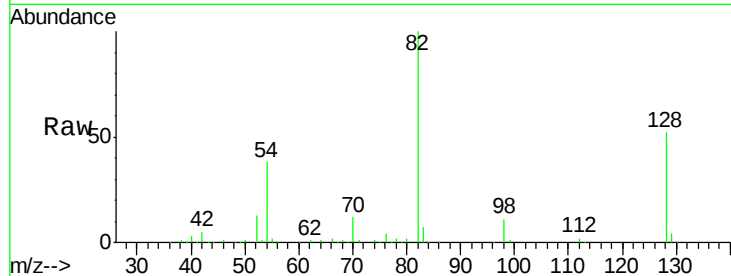


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

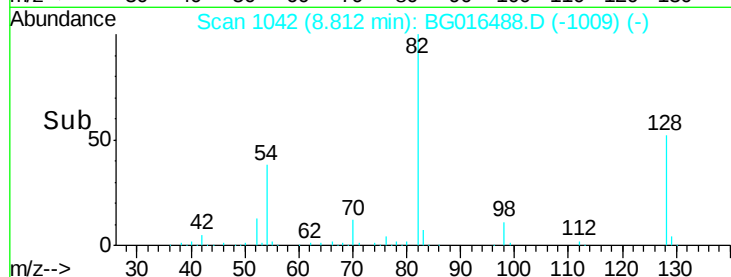
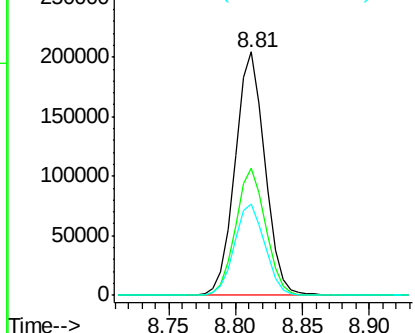


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.30 min Scan# 1976
 Delta R.T. -0.00 min
 Lab File: BG016488.D
 Acq: 17 Apr 2015 14:15

Tgt Ion: 164 Resp: 166177
 Ion Ratio Lower Upper
 164 100
 162 95.5 77.3 115.9
 160 42.8 36.7 55.1

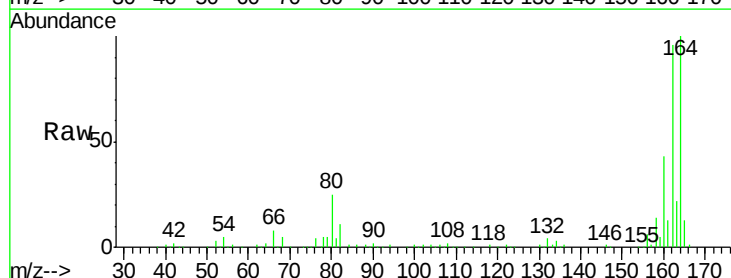

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

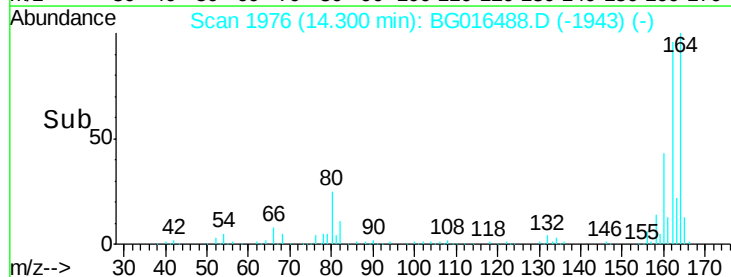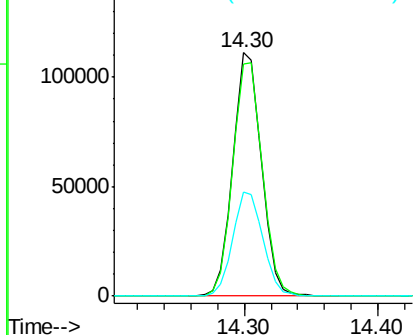






#41
 2,4,6-Tribromophenol
 Concen: 112.75 ng
 RT: 15.80 min Scan# 2231
 Delta R.T. 0.00 min
 Lab File: BG016488.D
 Acq: 17 Apr 2015 14:15

Instrument :
 BNA_G
 ClientSampled :
 PB82828BL

Tgt Ion:330 Resp: 126713
 Ion Ratio Lower Upper
 330 100
 332 94.3 75.8 113.6
 141 54.0 46.6 69.8

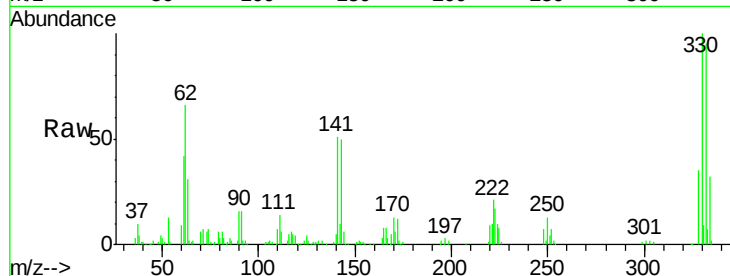


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

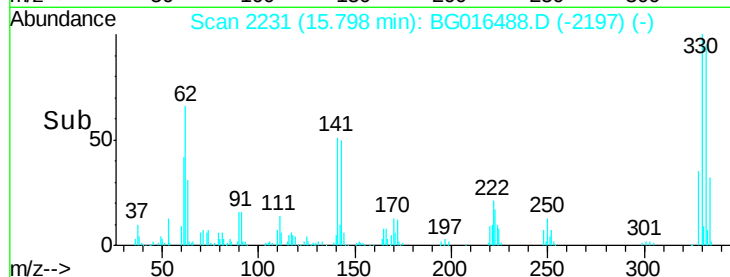
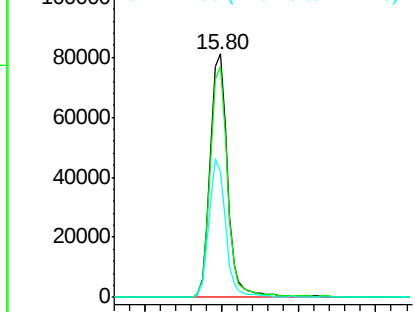


#44
 2-Fluorobiphenyl
 Concen: 72.32 ng
 RT: 12.92 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: BG016488.D
 Acq: 17 Apr 2015 14:15

Tgt Ion:172 Resp: 705874
 Ion Ratio Lower Upper
 172 100
 171 37.0 29.6 44.4
 170 23.9 19.4 29.2

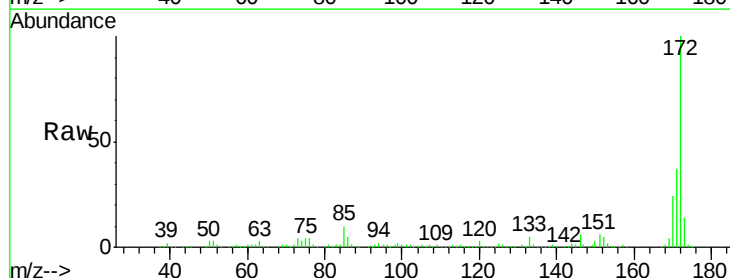

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

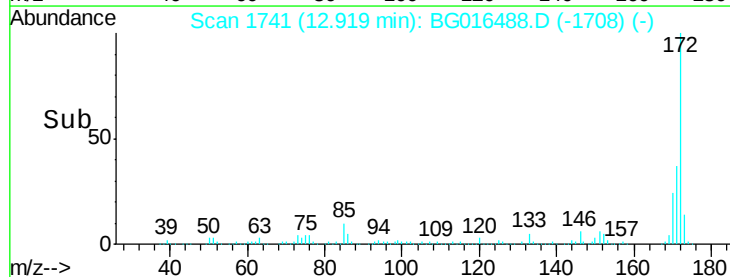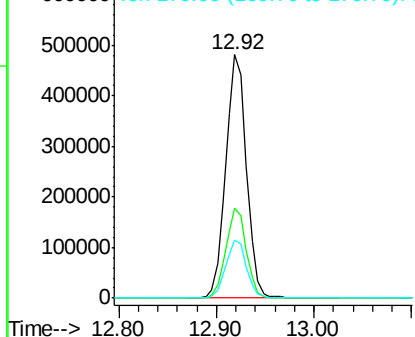







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.04 min Scan# 2443
Delta R.T. 0.00 min
Lab File: BG016488.D
Acq: 17 Apr 2015 14:15

Instrument :
BNA_G
ClientSampleId :
PB82828BL

Tgt Ion:188 Resp: 359197
Ion Ratio Lower Upper
188 100
94 13.8 12.2 18.4
80 13.8 12.8 19.2

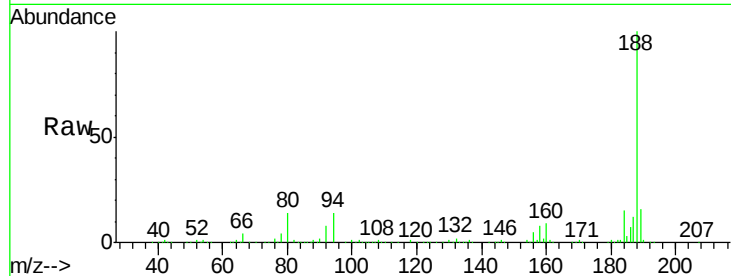


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

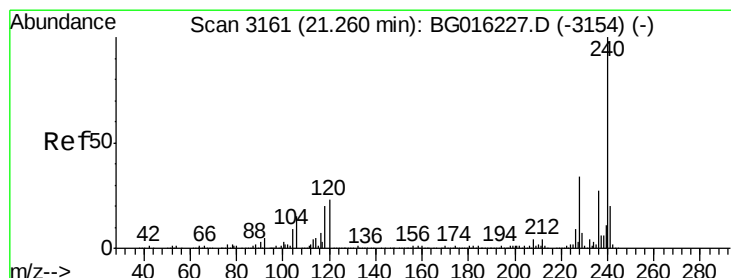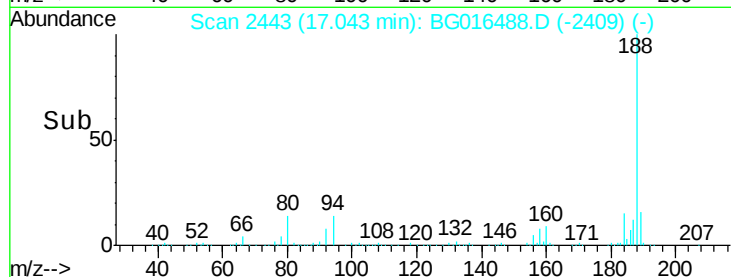
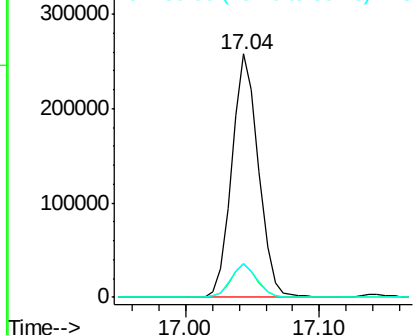


#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.23 min Scan# 3155
Delta R.T. -0.00 min
Lab File: BG016488.D
Acq: 17 Apr 2015 14:15

Tgt Ion:240 Resp: 310399
Ion Ratio Lower Upper
240 100
120 19.6 18.6 28.0
236 26.2 21.7 32.5

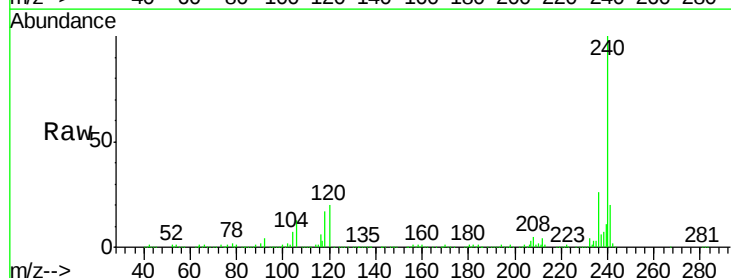

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

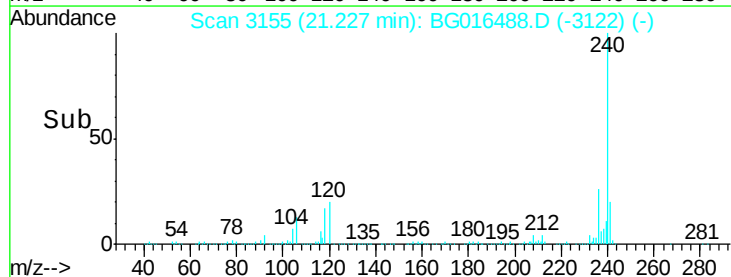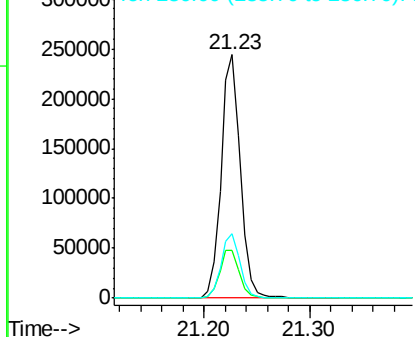



#78

Terphenyl-d14

Concen: 65.93 ng

RT: 19.68 min Scan# 2891

Delta R.T. 0.00 min

Lab File: BG016488.D

Acq: 17 Apr 2015 14:15

Instrument :

BNA_G

ClientSampleId :

PB82828BL


Tgt Ion:244 Resp: 874364

Ion Ratio Lower Upper

244 100

212 8.1 6.6 9.8




122 22.0 19.1 28.7

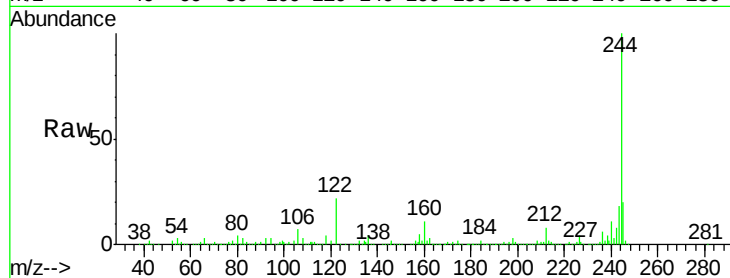

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

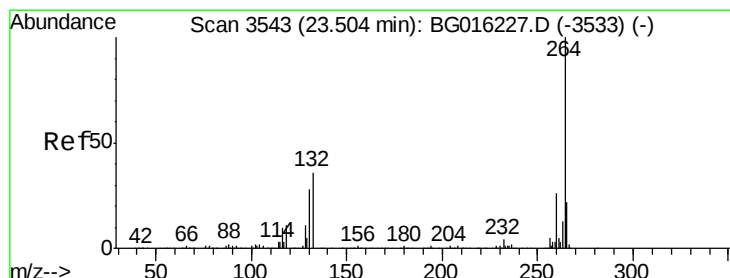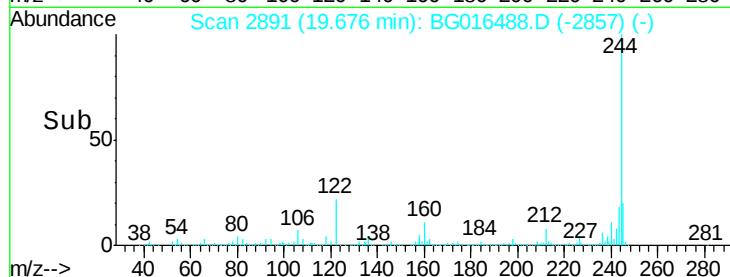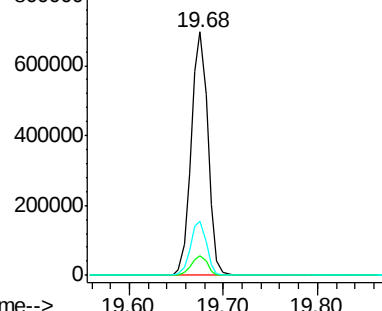

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.45 min Scan# 3534

Delta R.T. 0.00 min

Lab File: BG016488.D

Acq: 17 Apr 2015 14:15


Tgt Ion:264 Resp: 291643

Ion Ratio Lower Upper

264 100

260 25.0 20.4 30.6

265 22.2 17.2 25.8

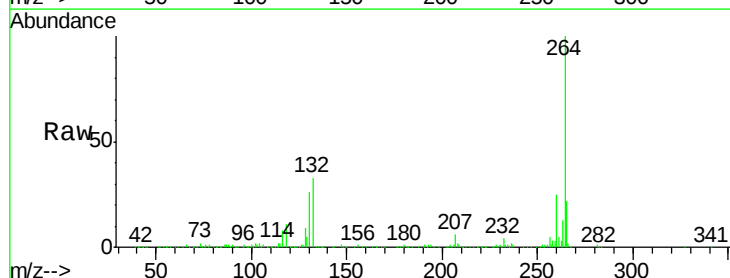

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

