


Data Path : Z:\HPCHEM1\BNA_G\Data\BG041715\
 Data File : BG016505.D
 Acq On : 18 Apr 2015 3:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG040615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 14 14:00:56 2015

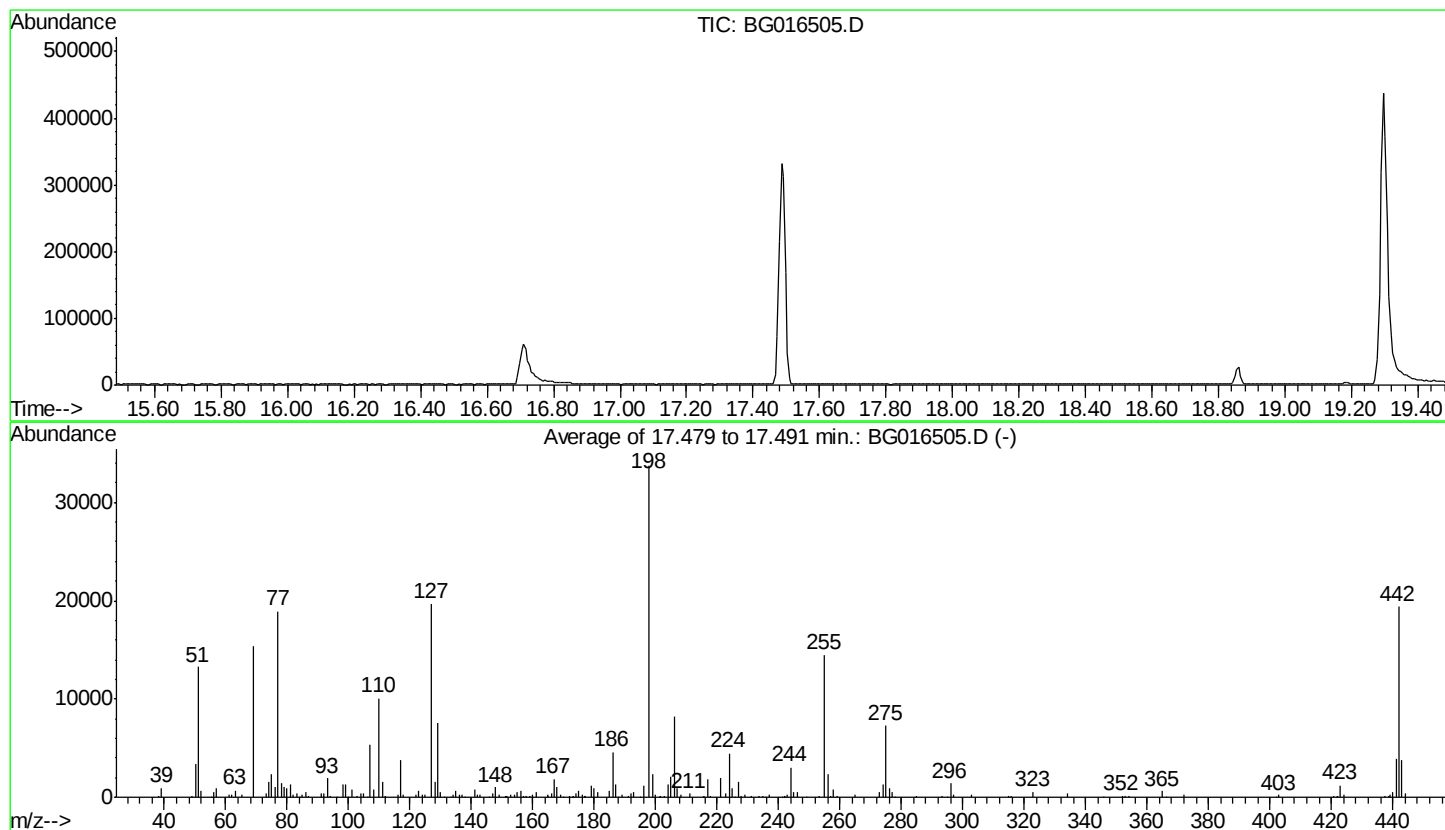

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	13282	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.5	15346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.3	19678	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33749	PASS
199	198	5	9	7.1	2404	PASS
275	198	10	60	21.4	7238	PASS
365	198	1	100	1.8	592	PASS
441	442	0.01	24	20.0	3873	PASS
442	198	50	100	57.5	19394	PASS
443	442	15	24	19.6	3802	PASS