
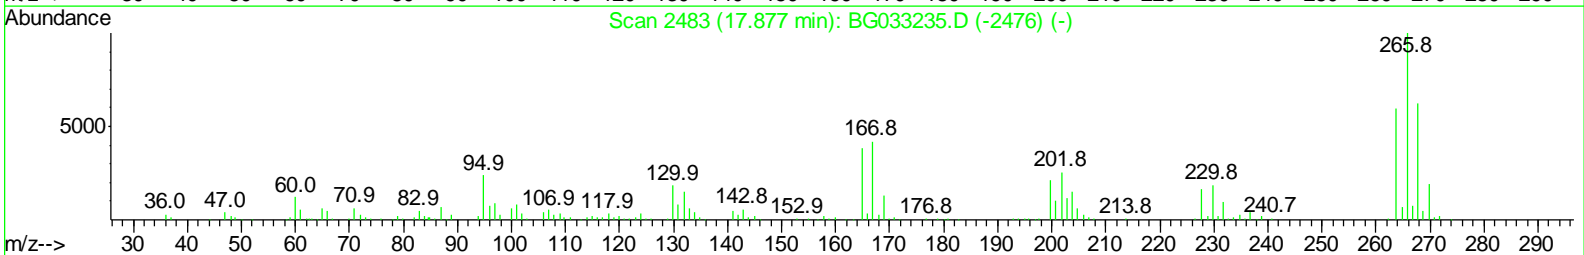
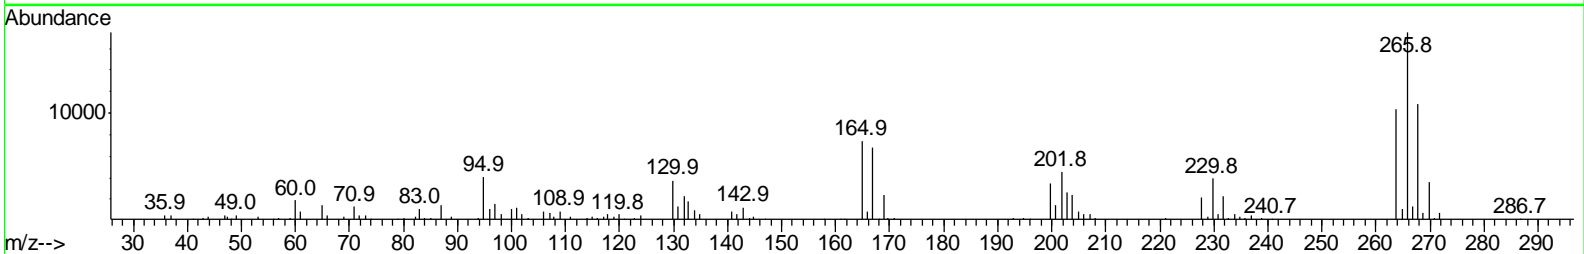


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041718\
 Data File : BG033845.D
 Acq On : 17 Apr 2018 14:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 05:30:27 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 17 18:35:38 2018
 Response via : Initial Calibration

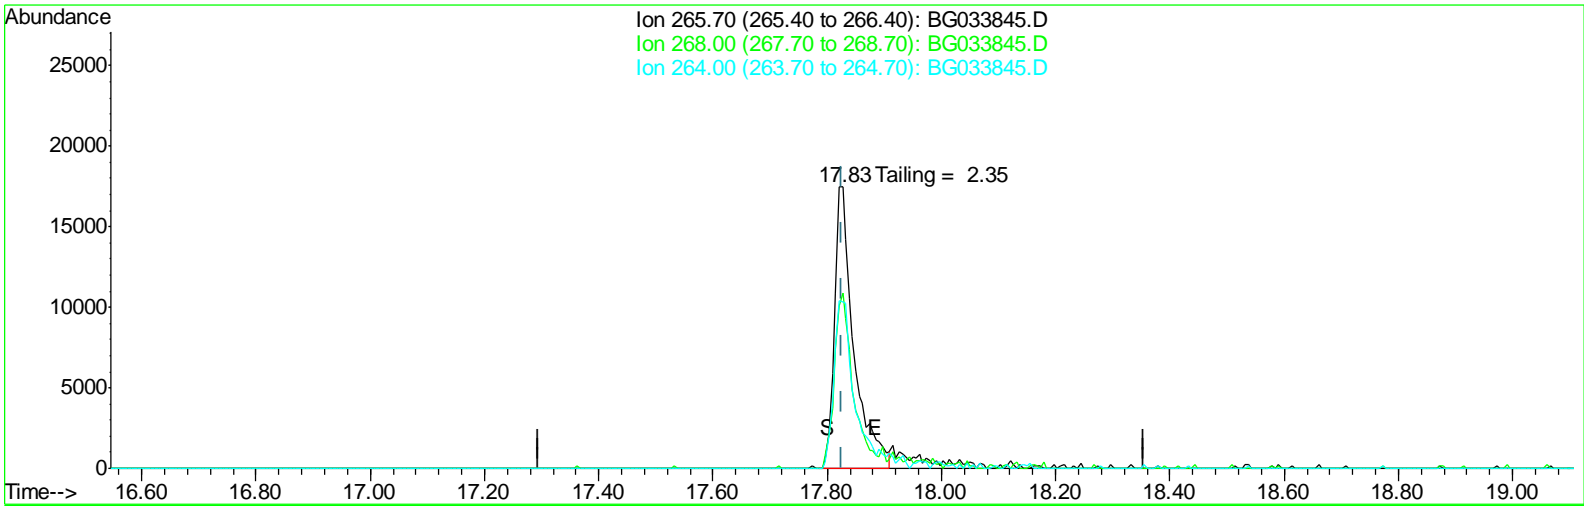

TIC: BG033845.D

(69) Pentachlorophenol (C)




17.826min (+0.000) 0.00ng

response 41022

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.10
264.00	62.00	59.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041718\
 Data File : BG033845.D
 Acq On : 17 Apr 2018 14:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 05:30:27 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 17 18:35:38 2018
 Response via : Initial Calibration

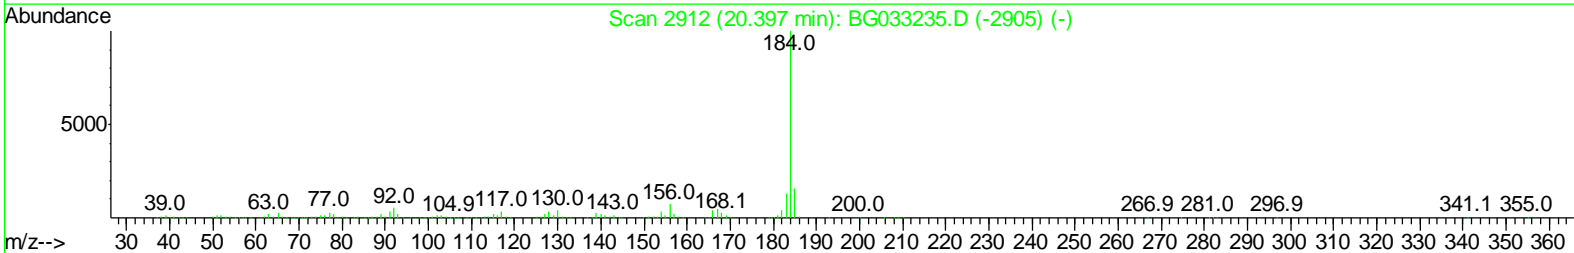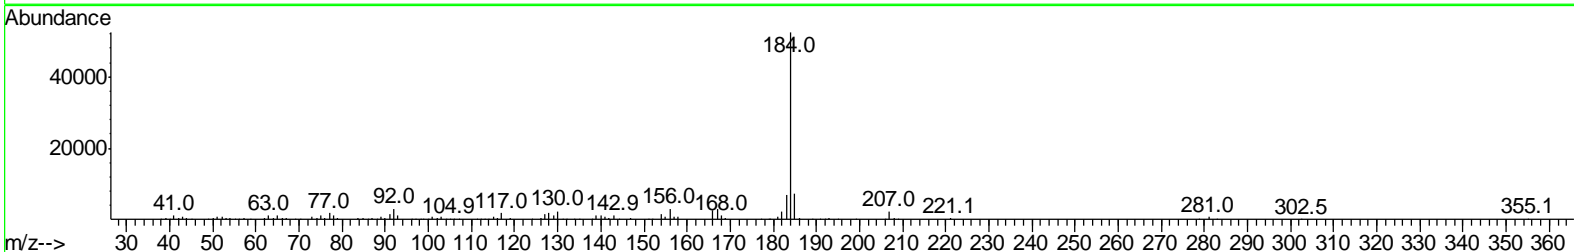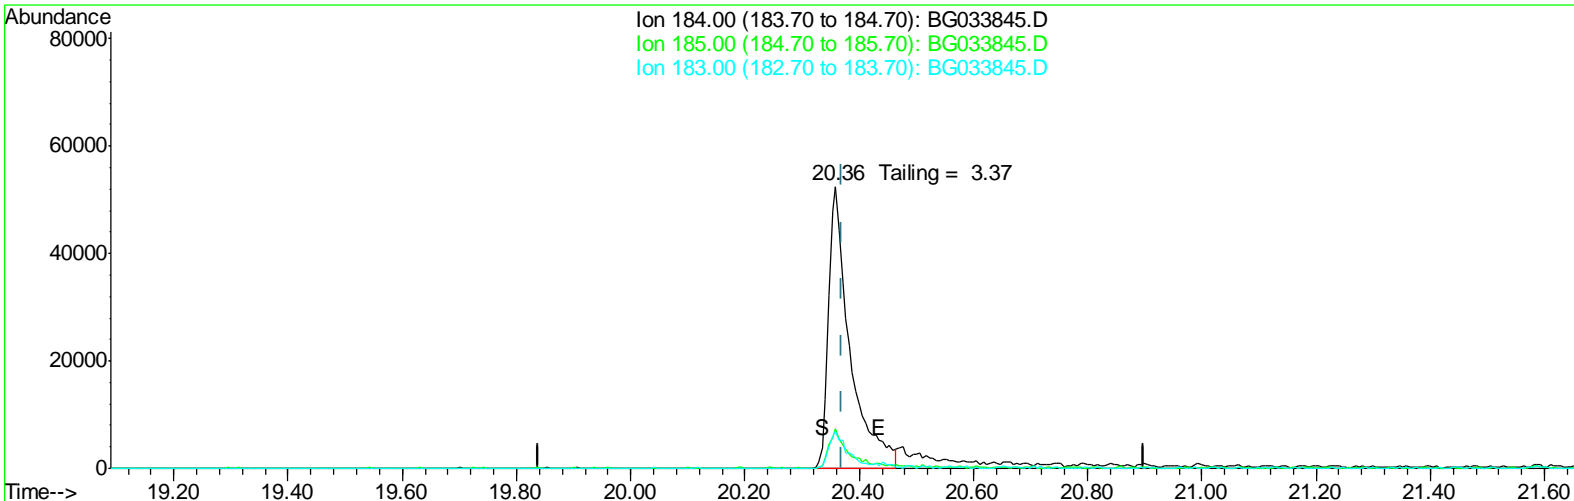

TIC: BG033845.D

(76) Benzidine

20.359min (-0.012) 79833.56ng

response 136393

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.30
183.00	13.30	12.98
0.00	0.00	0.00