


Data Path : Z:\HPCHEM1\BNA G\Data\BG041718\
 Data File : BG033845.D
 Acq On : 17 Apr 2018 14:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 17 18:35:38 2018

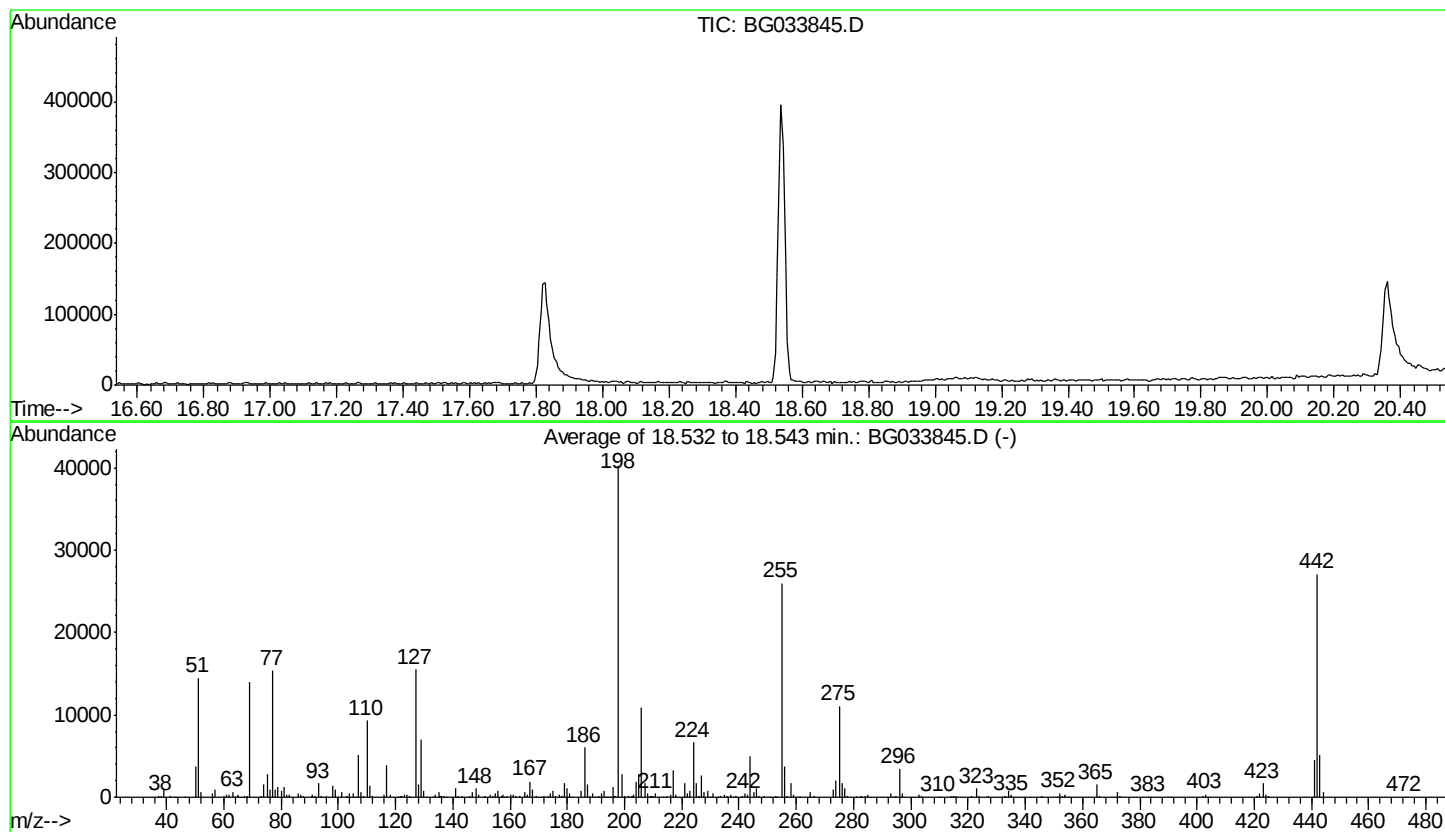

AutoFind: Scans 2594, 2595, 2596; Background Corrected with Scan 2585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	14471	PASS
68	69	0.00	2	1.1	159	PASS
69	198	0.00	100	34.7	13977	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.4	15480	PASS
197	198	0.00	2	0.5	197	PASS
198	198	100	100	100.0	40266	PASS
199	198	5	9	6.8	2750	PASS
275	198	10	60	27.5	11061	PASS
365	198	1	100	3.8	1522	PASS
441	443	0.01	100	88.3	4494	PASS
442	198	50	100	67.3	27104	PASS
443	442	15	24	18.8	5091	PASS