
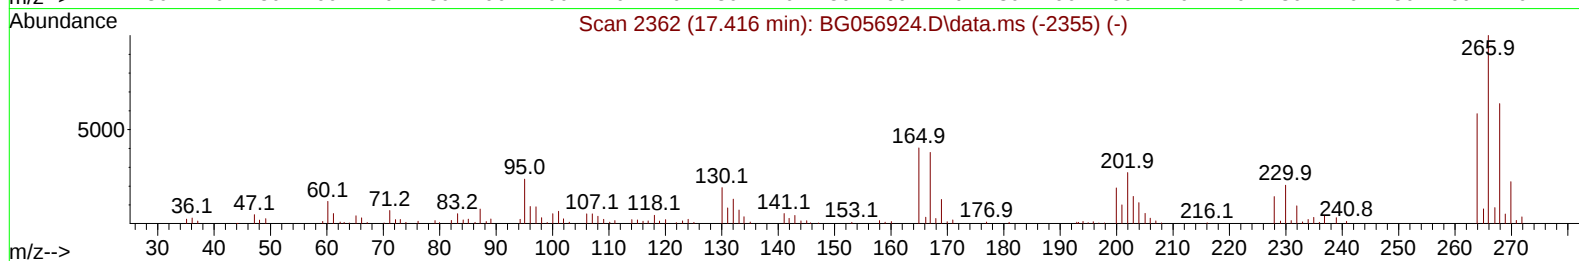
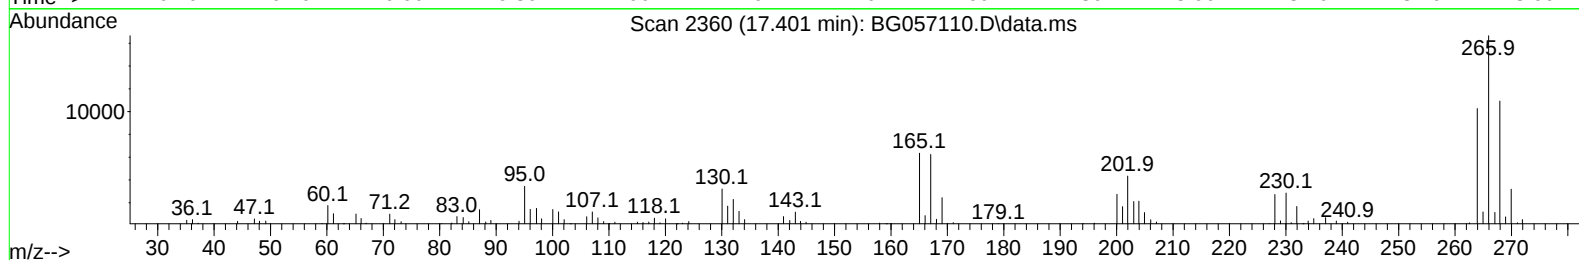


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041723\
Data File : BG057110.D
Acq On : 17 Apr 2023 12:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 04:03:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 19:00:08 2023
Response via : Initial Calibration

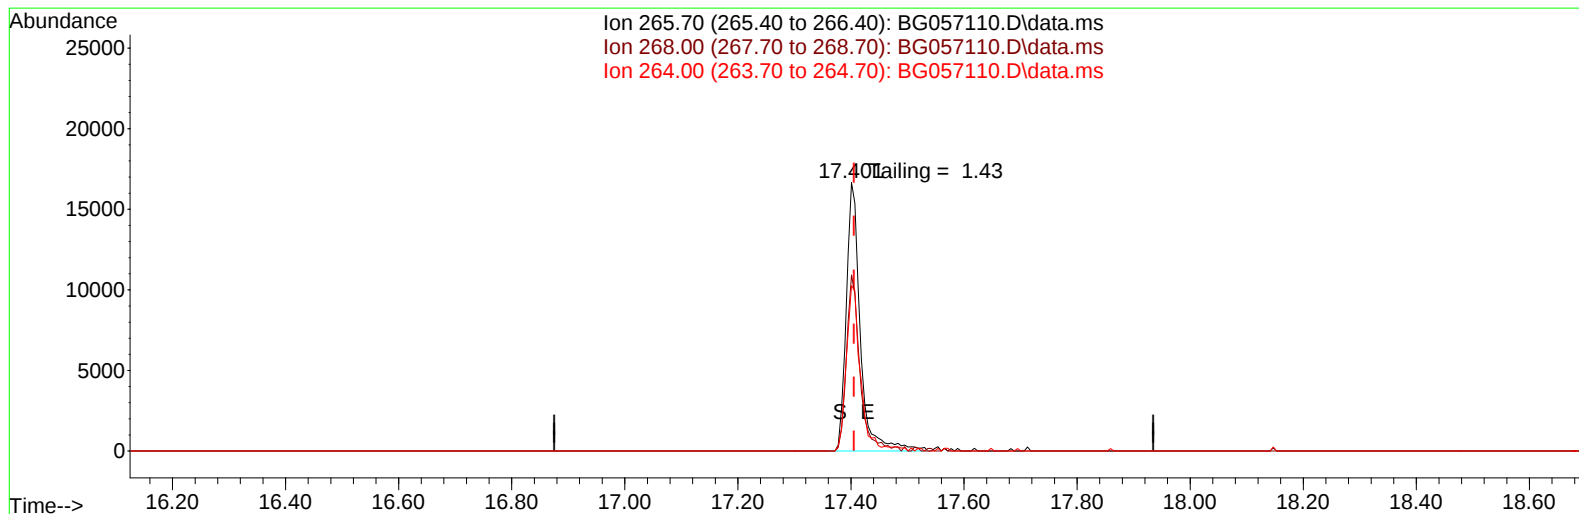

TIC: BG057110.D\data.ms

(70) Pentachlorophenol (C)




17.401min (-0.004) 20824.19 ng

response 28875

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.57
264.00	58.50	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041723\
Data File : BG057110.D
Acq On : 17 Apr 2023 12:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 04:03:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 19:00:08 2023
Response via : Initial Calibration

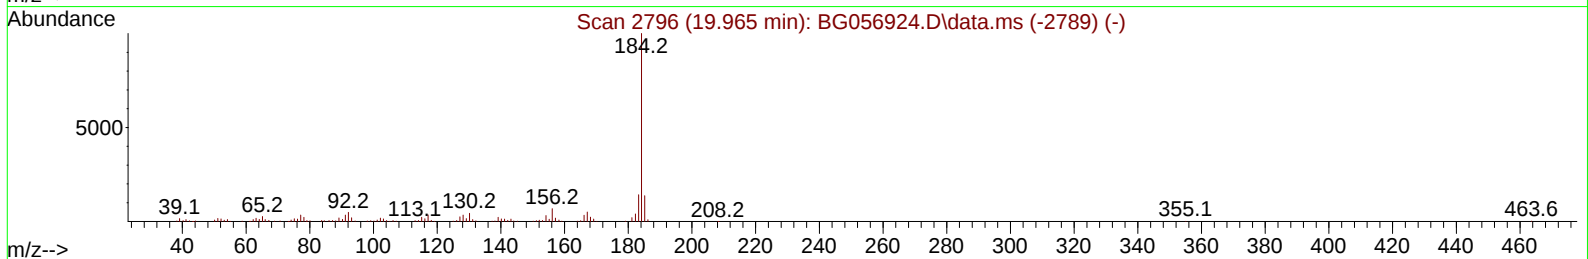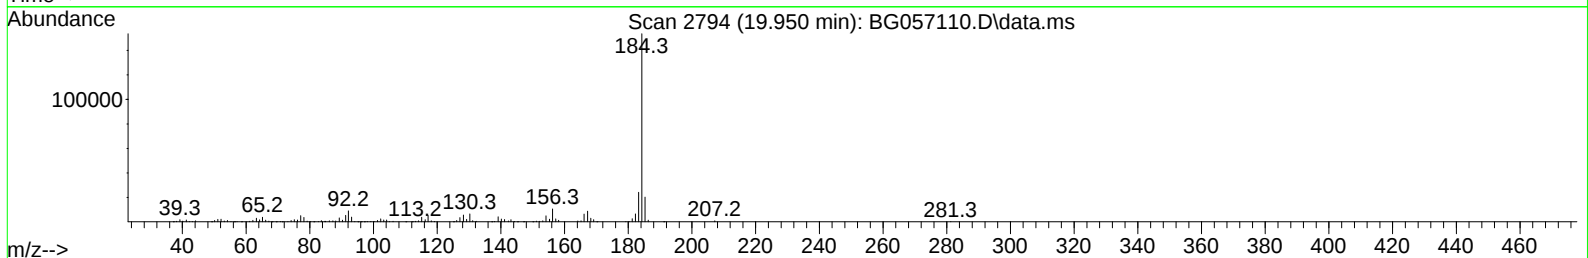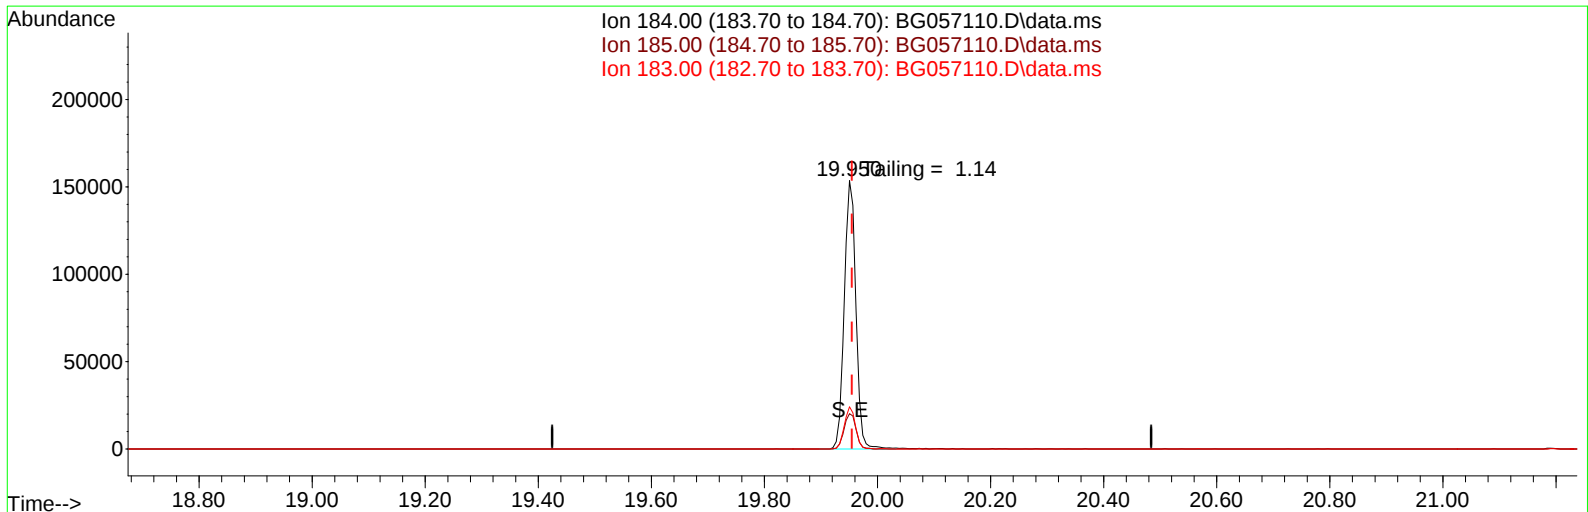

TIC: BG057110.D\data.ms

(77) Benzidine

19.950min (-0.004) 0.00 ng

response 219290

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.22
183.00	14.20	15.72
0.00	0.00	0.00