
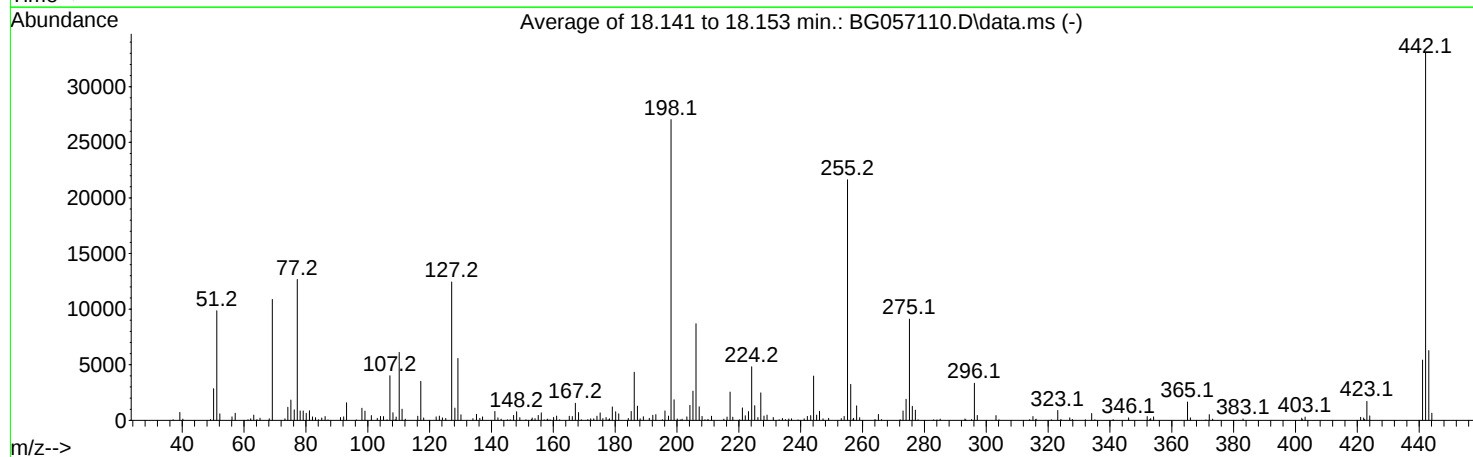


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041723\
 Data File : BG057110.D
 Acq On : 17 Apr 2023 12:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 19:00:08 2023

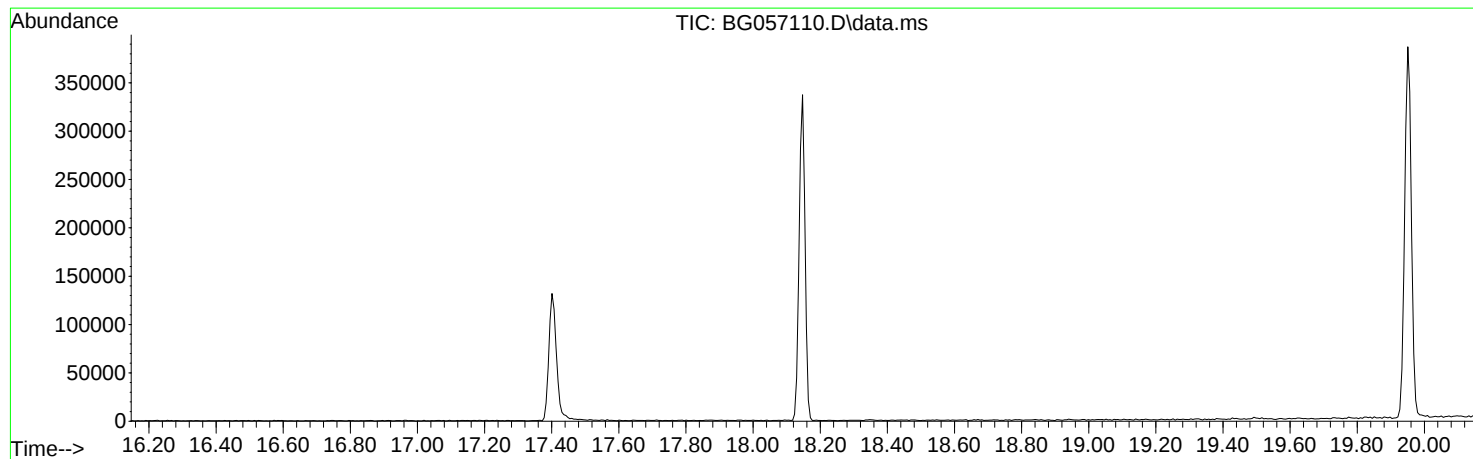




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	9851	PASS
68	69	0.00	2	1.4	148	PASS
69	198	0.00	100	40.2	10877	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	12448	PASS
197	198	0.00	2	1.4	386	PASS
198	198	100	100	100.0	27043	PASS
199	198	5	9	6.8	1851	PASS
275	198	10	60	33.7	9106	PASS
365	198	1	100	6.1	1649	PASS
441	198	0.01	100	20.1	5425	PASS
442	442	50	100	100.0	33072	PASS
443	442	15	24	18.9	6266	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041723\
Data File : BG057110.D
Acq On : 17 Apr 2023 12:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 18 04:03:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 19:00:08 2023
Response via : Initial Calibration

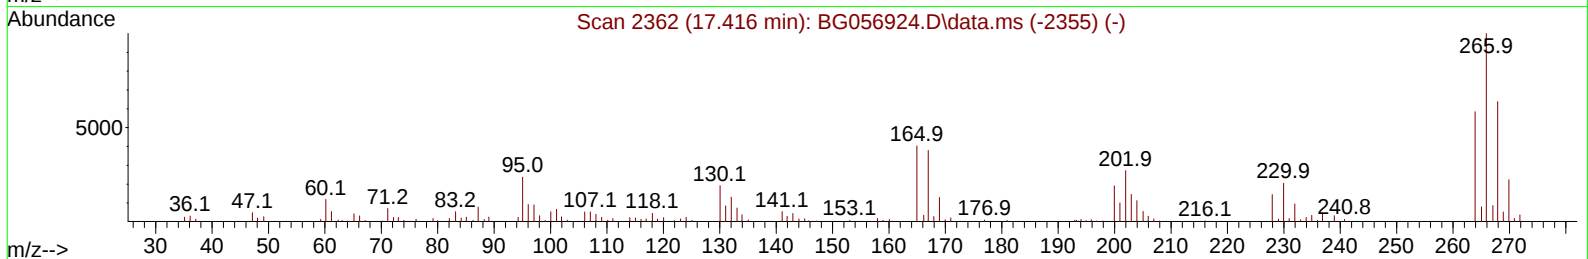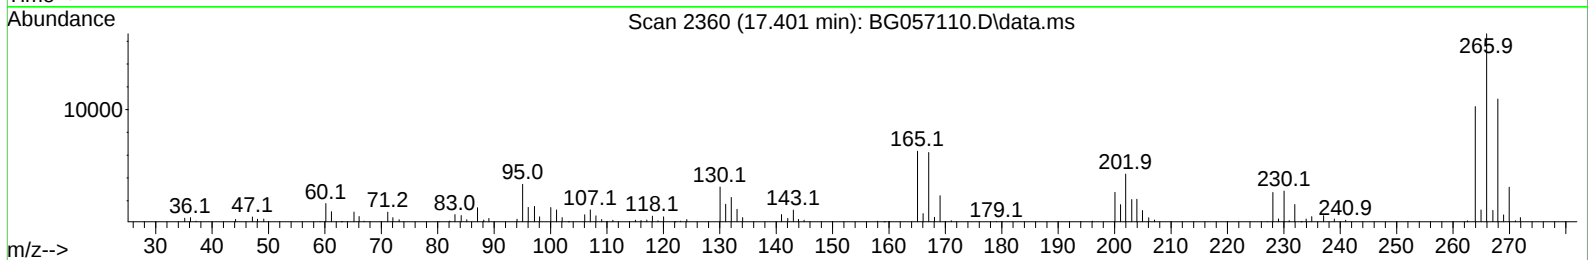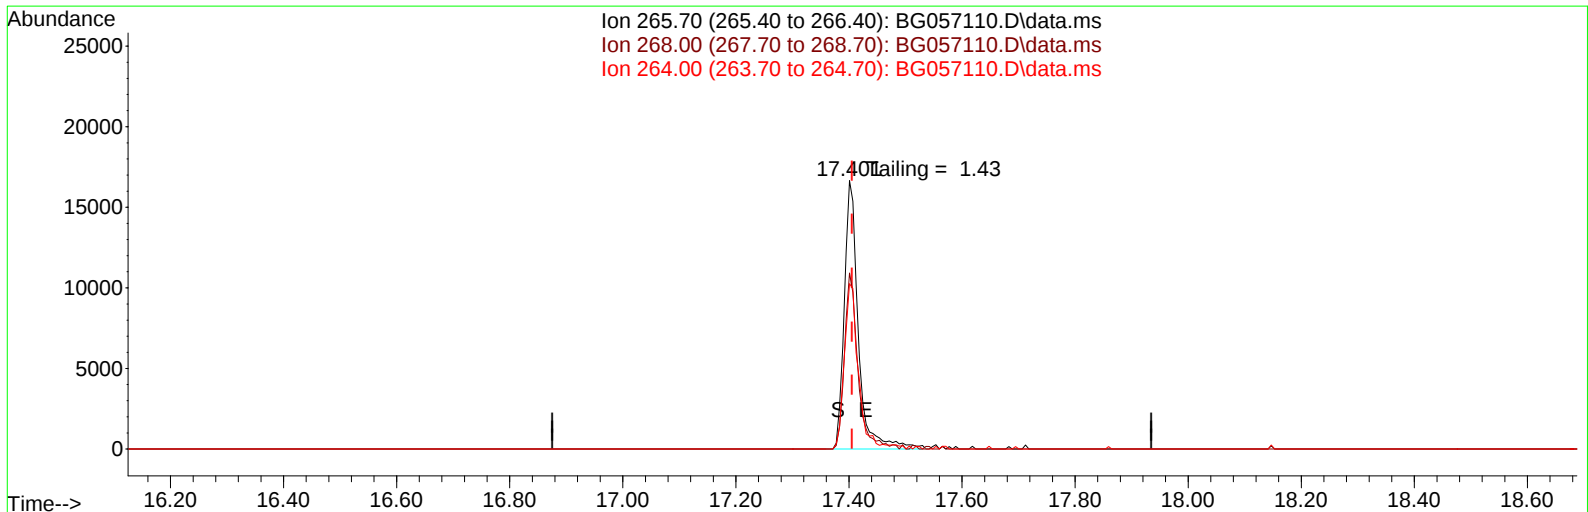

TIC: BG057110.D\data.ms

(70) Pentachlorophenol (C)

17.401min (-0.004) 20824.19 ng




response 28875

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.57
264.00	58.50	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041723\
 Data File : BG057110.D
 Acq On : 17 Apr 2023 12:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 18 04:03:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 19:00:08 2023
 Response via : Initial Calibration

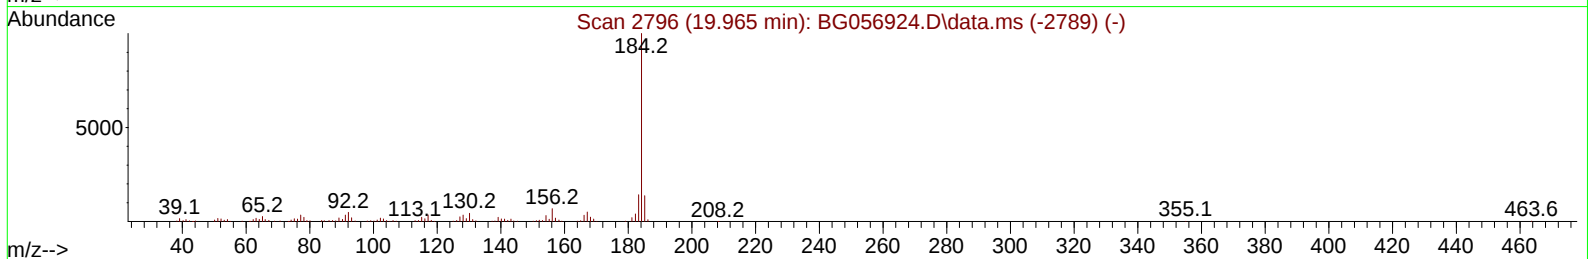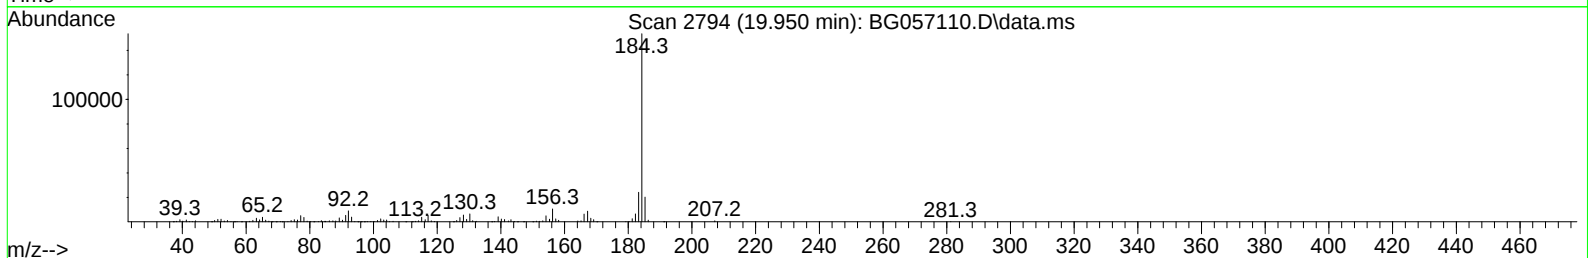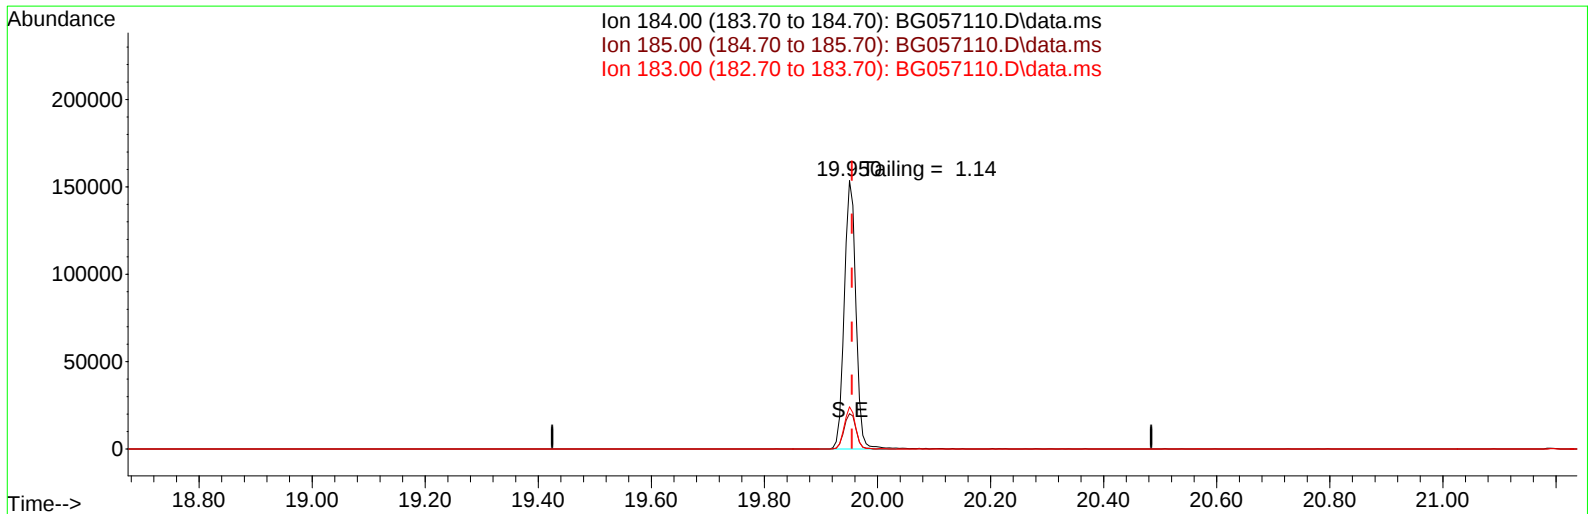

TIC: BG057110.D\data.ms

(77) Benzidine

19.950min (-0.004) 0.00 ng

response 219290

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.22
183.00	14.20	15.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/17/2023	BNA_G	BG057110.D
Compound Name	Response	Retention Time
DDT	97933	21.19
DDD	4168	20.732
DDE	0	20.217
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4168	102101	4.08

Instrument :
BNA_G
ClientSampleId :
DFTPP