
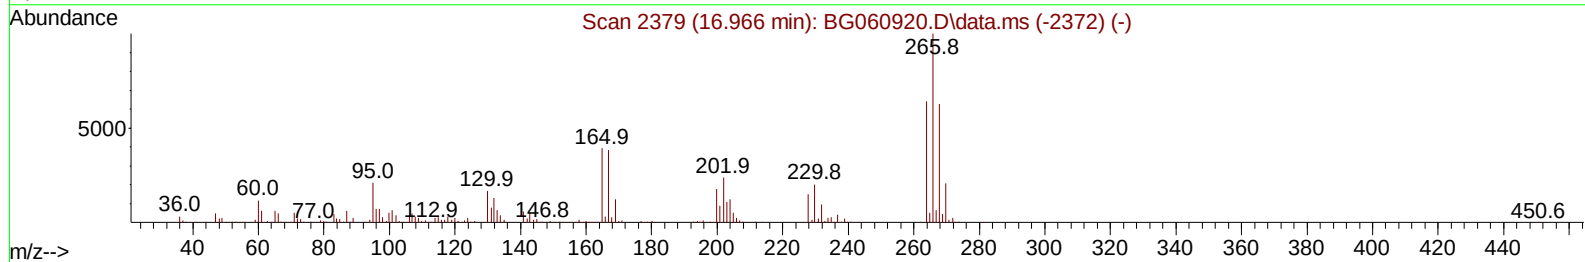
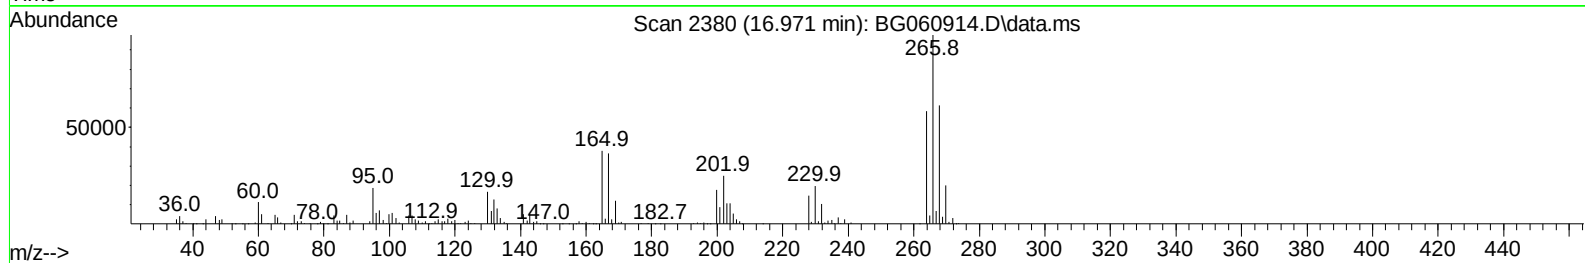


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041724\
Data File : BG060914.D
Acq On : 17 Apr 2024 10:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 02:10:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

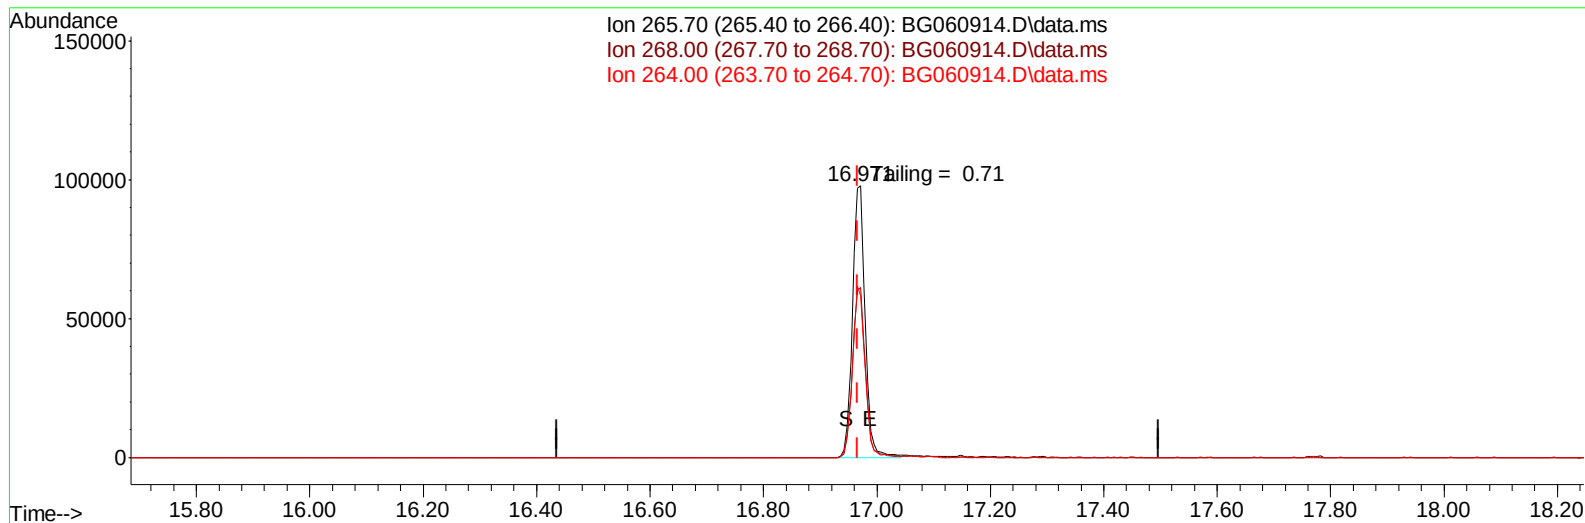




TIC: BG060914.D\data.ms

(70) Pentachlorophenol (C)**16.971min (+ 0.005) 103623.87 ng****response 152268**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.63
264.00	64.00	59.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041724\
Data File : BG060914.D
Acq On : 17 Apr 2024 10:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 02:10:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

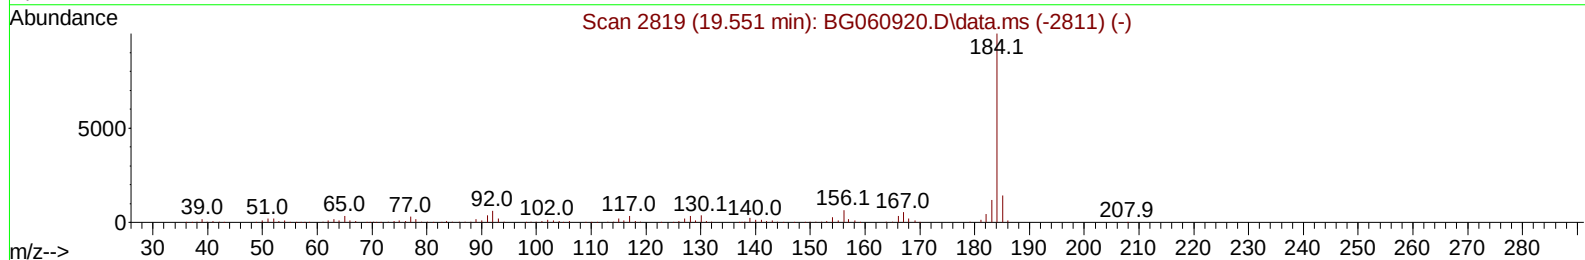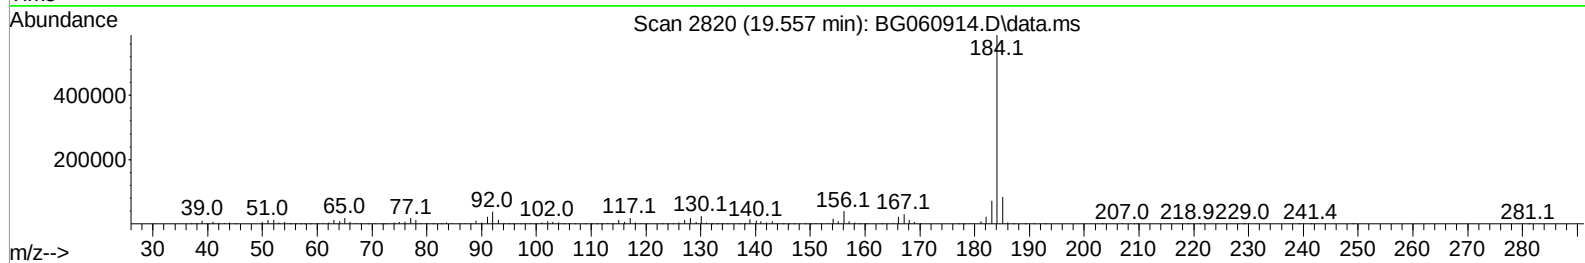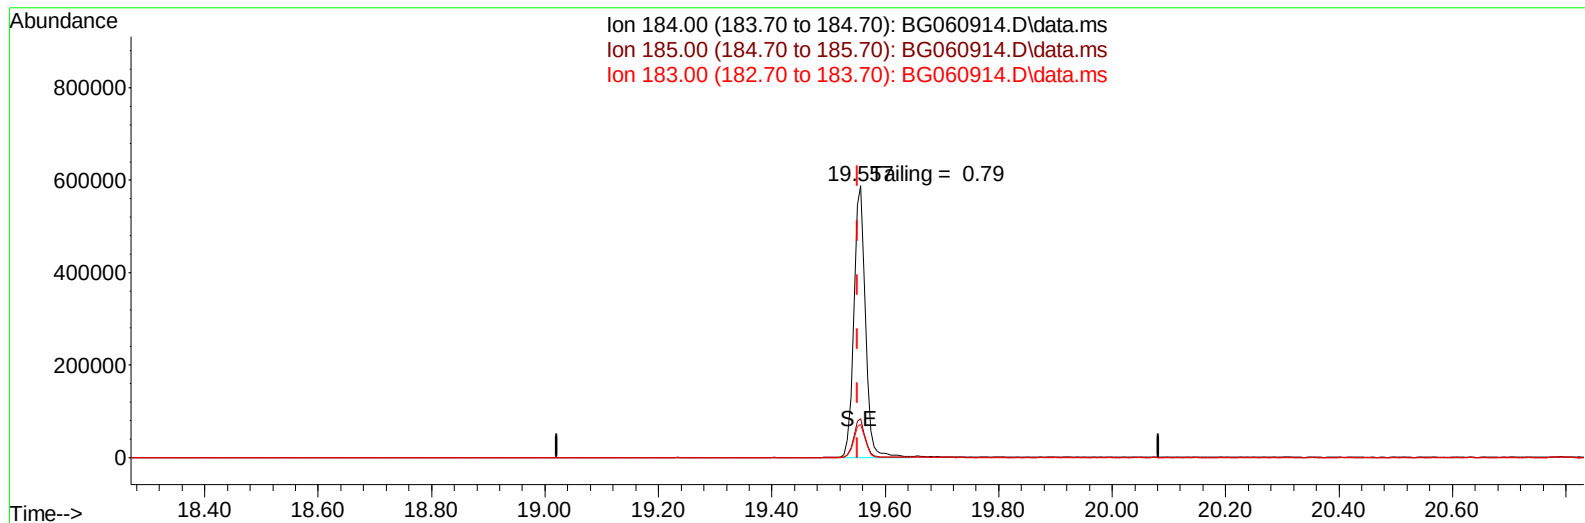

TIC: BG060914.D\data.ms

(77) Benzidine**19.557min (+ 0.005) 146974.90 ng****response 836402**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.28
183.00	11.80	12.22
0.00	0.00	0.00