
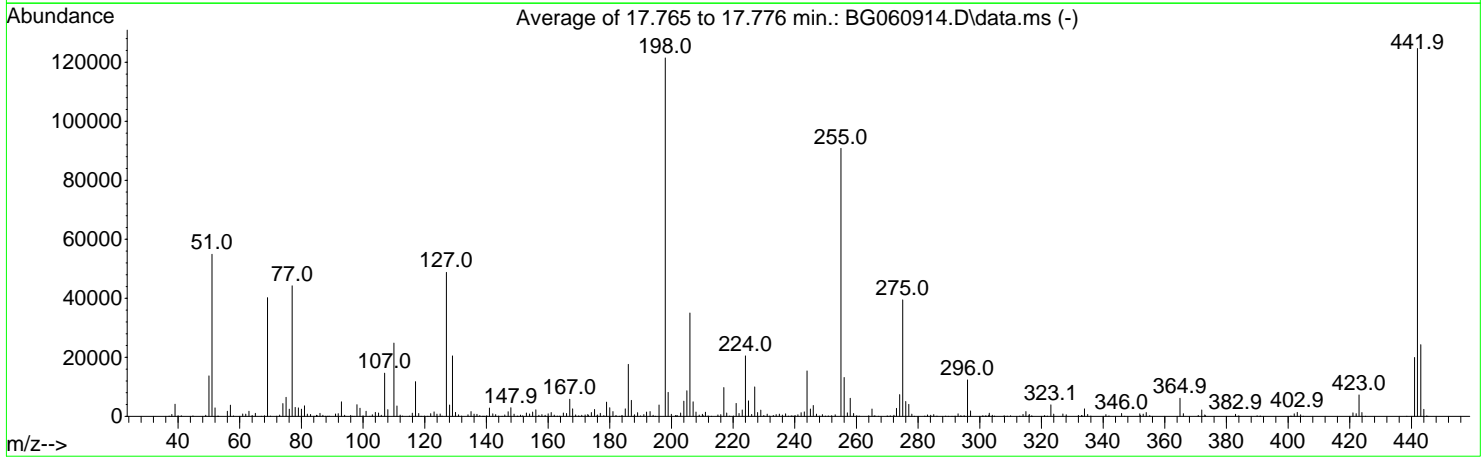


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041724\
 Data File : BG060914.D
 Acq On : 17 Apr 2024 10:20
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 18 02:02:19 2024

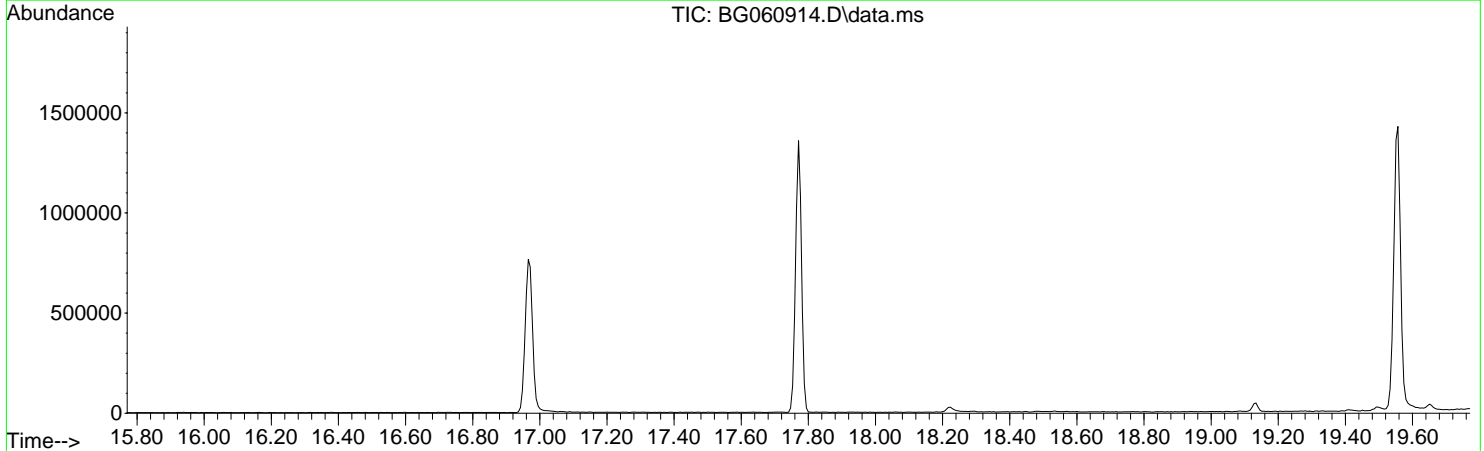




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	54912	PASS
68	69	0.00	2	0.6	235	PASS
69	198	0.00	100	33.1	40254	PASS
70	69	0.00	2	0.2	93	PASS
127	198	10	80	40.2	48829	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121451	PASS
199	198	5	9	6.7	8117	PASS
275	198	10	60	32.5	39480	PASS
365	198	1	100	5.1	6145	PASS
441	198	0.01	100	16.4	19935	PASS
442	442	50	100	100.0	124660	PASS
443	442	15	24	19.5	24288	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041724\
 Data File : BG060914.D
 Acq On : 17 Apr 2024 10:20
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 DFTPP

Quant Time: Apr 18 02:10:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 02:02:19 2024
 Response via : Initial Calibration

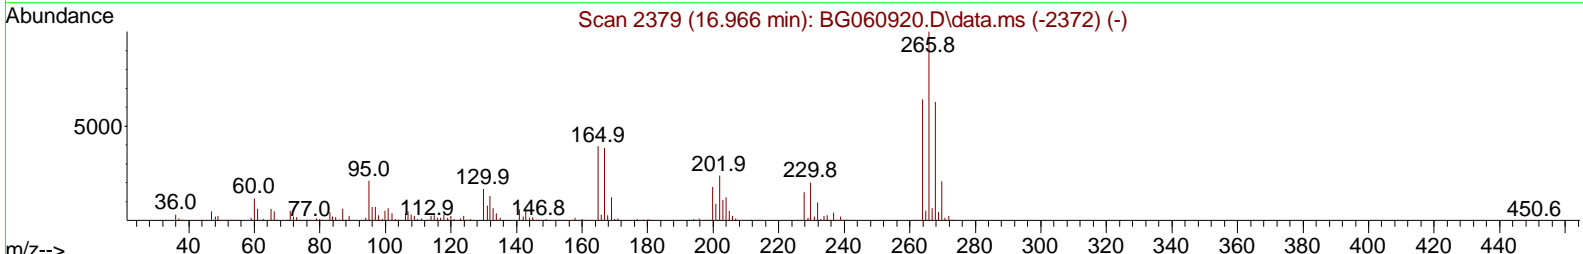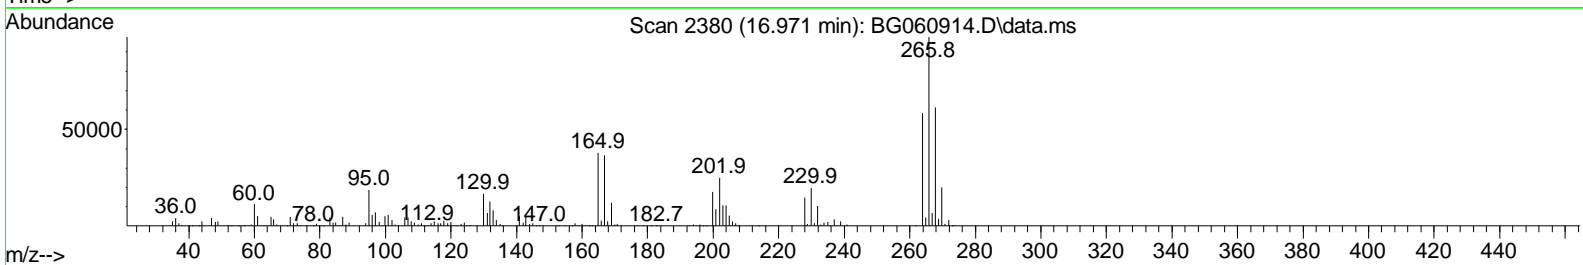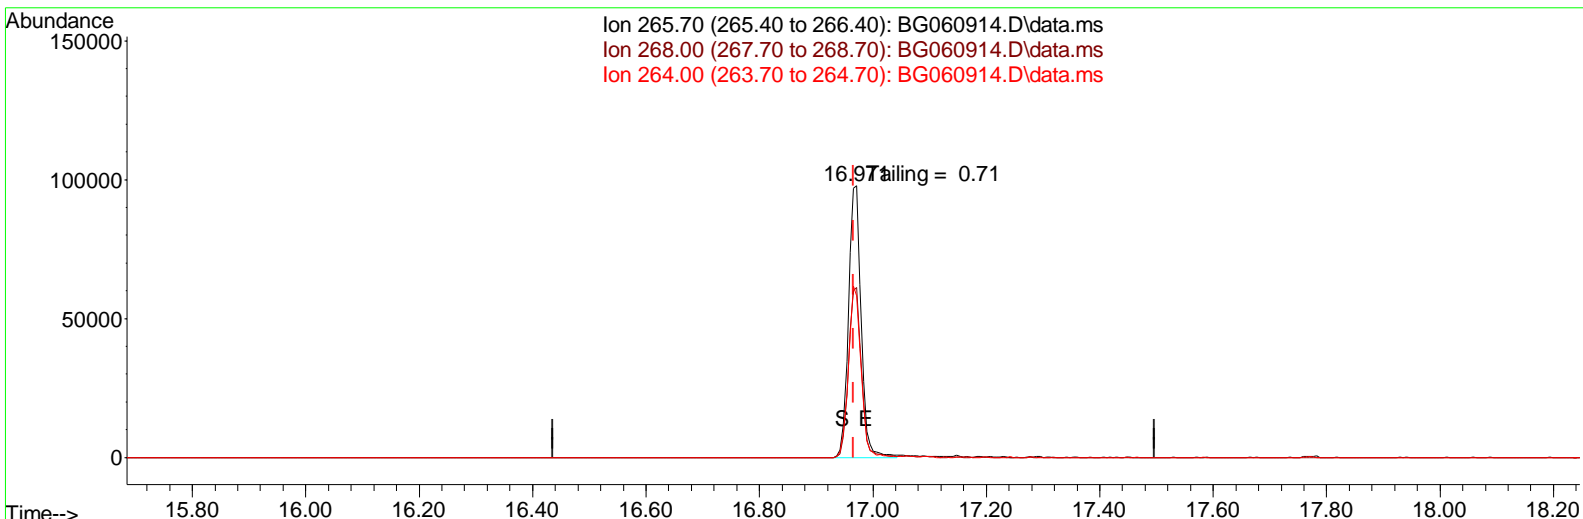

TIC: BG060914.D\data.ms

(70) Pentachlorophenol (C)

16.971min (+ 0.005) 103623.87 ng




response 152268

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.63
264.00	64.00	59.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041724\
 Data File : BG060914.D
 Acq On : 17 Apr 2024 10:20
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 DFTPP

Quant Time: Apr 18 02:10:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 02:02:19 2024
 Response via : Initial Calibration

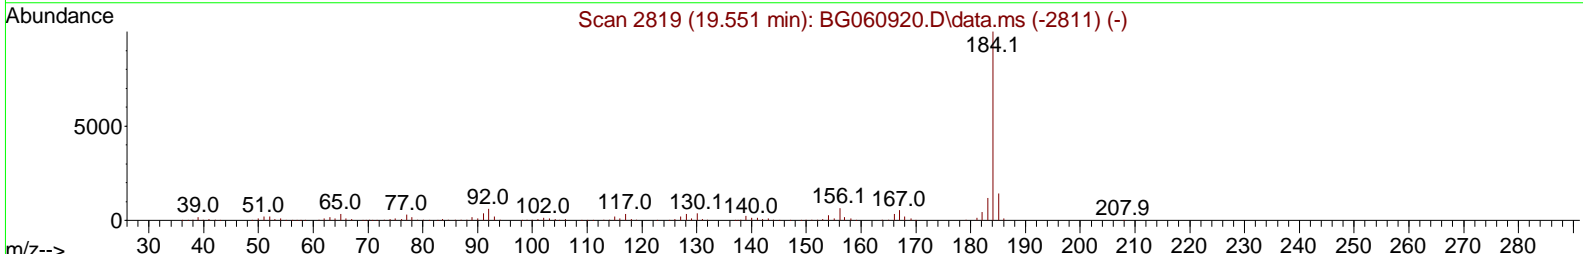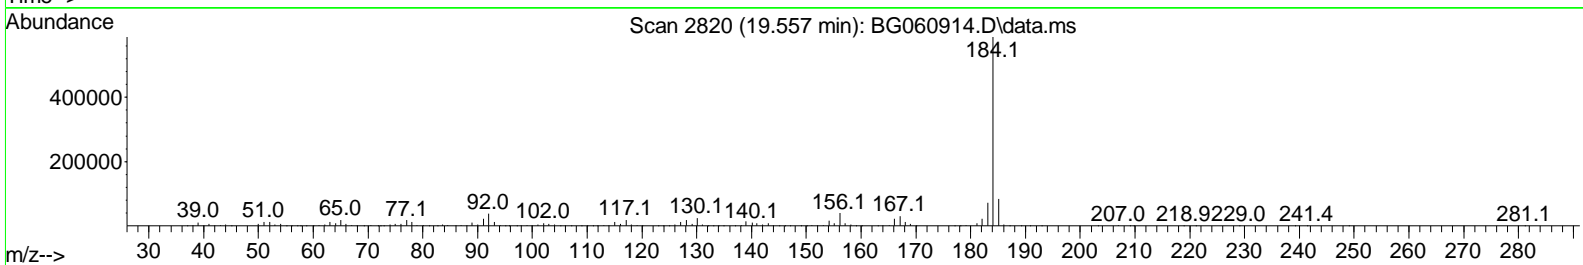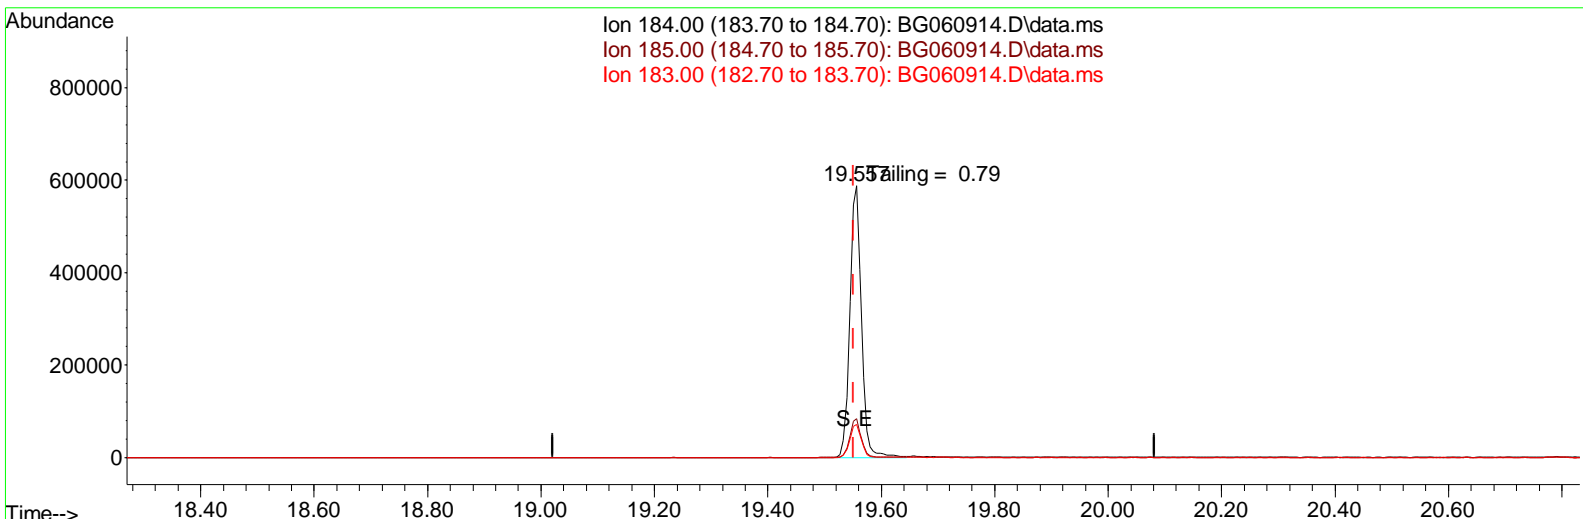

TIC: BG060914.D\data.ms

(77) Benzidine

19.557min (+ 0.005) 146974.90 ng

response 836402

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.28
183.00	11.80	12.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/17/2024	BNA_G	<u>BG060914.D</u>
Compound Name	Response	Retention Time
DDT	462799	20.796
DDD	11544	20.356
DDE	1665	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13209	476008	2.77

Instrument :
 BNA_G
 ClientSampled :
 DFTPP