


Data Path : Z:\HPCHEM1\BNA G\Data\BG041816\
 Data File : BG021719.D
 Acq On : 18 Apr 2016 1:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 13 15:48:13 2016

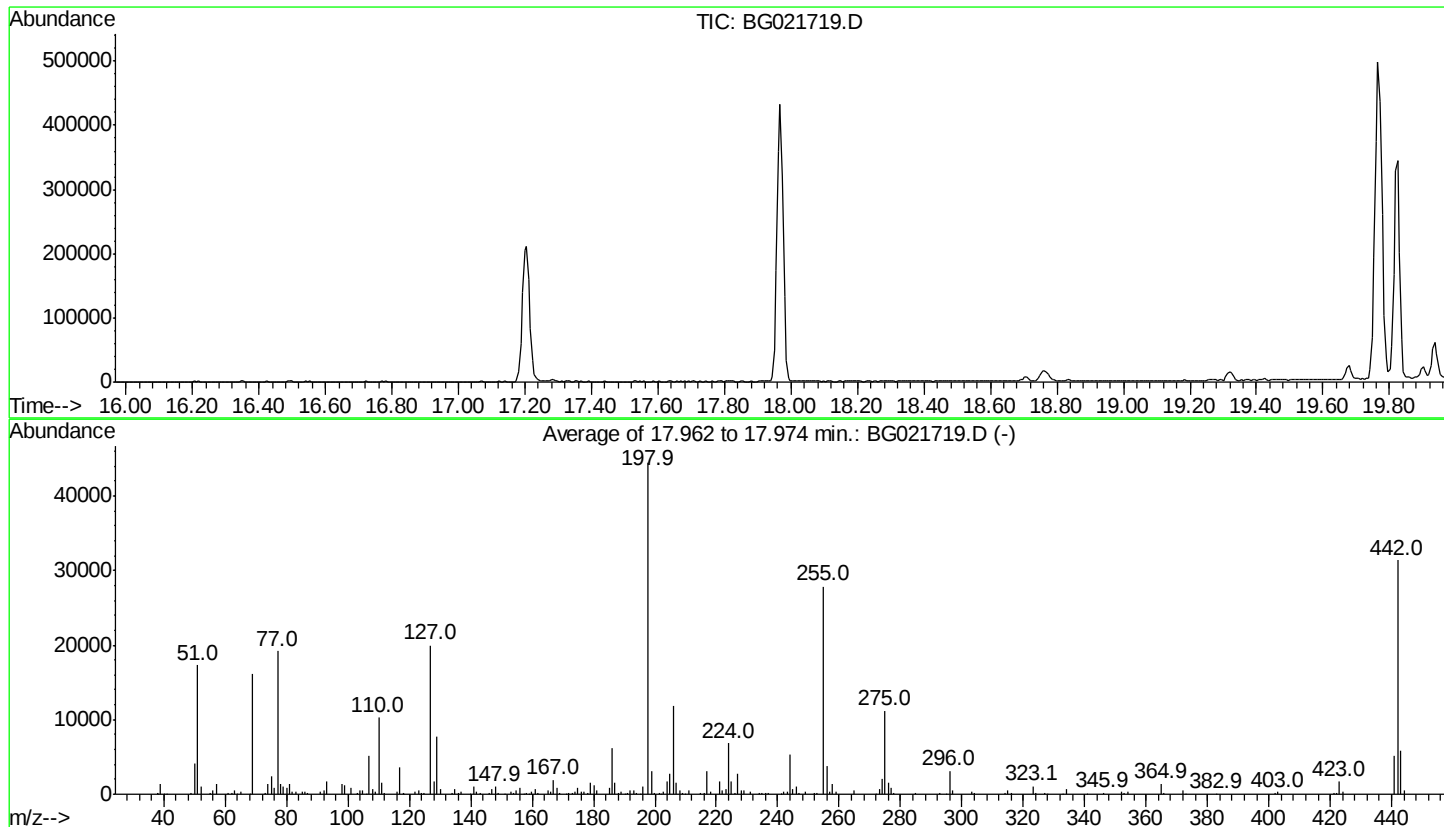

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	17304	PASS
68	69	0.00	2	0.5	83	PASS
69	198	0.00	100	36.2	16089	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.8	19937	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44477	PASS
199	198	5	9	6.8	3033	PASS
275	198	10	60	25.3	11240	PASS
365	198	1	100	3.2	1432	PASS
441	442	0.01	24	16.4	5137	PASS
442	198	50	100	70.5	31378	PASS
443	442	15	24	18.7	5865	PASS