
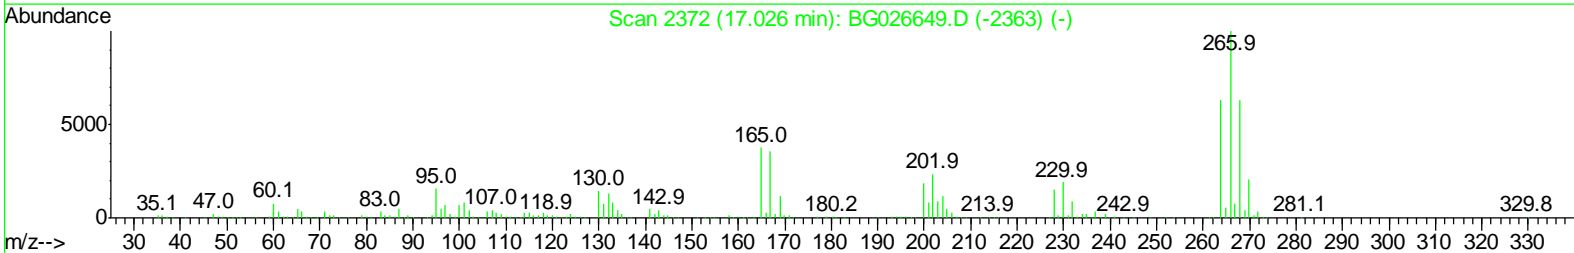
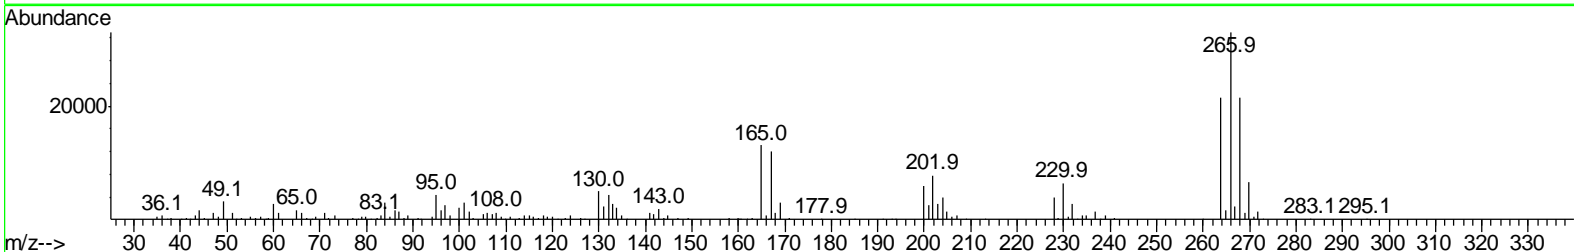


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041817\
 Data File : BG026645.D
 Acq On : 18 Apr 2017 12:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 19:24:15 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 18:04:39 2017
 Response via : Initial Calibration

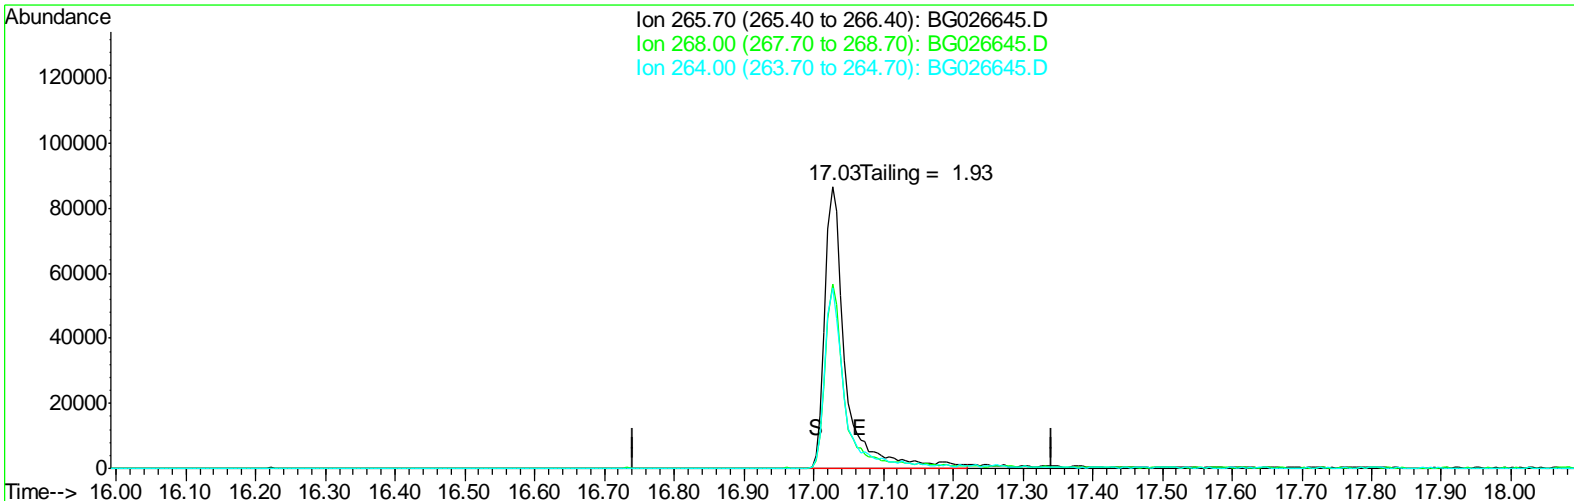

TIC: BG026645.D

(69) Pentachlorophenol (C)




17.043min (-17.043) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG041817\
 Data File : BG026645.D
 Acq On : 18 Apr 2017 12:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 19:24:15 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 18 18:04:39 2017
 Response via : Initial Calibration

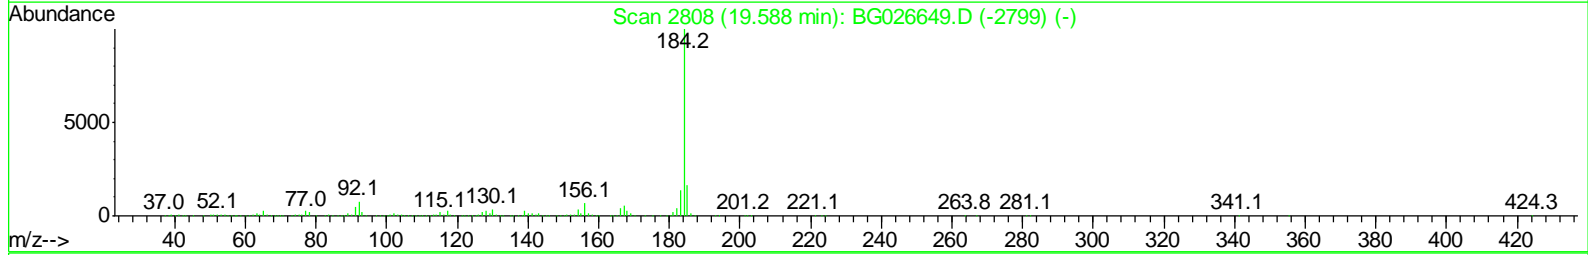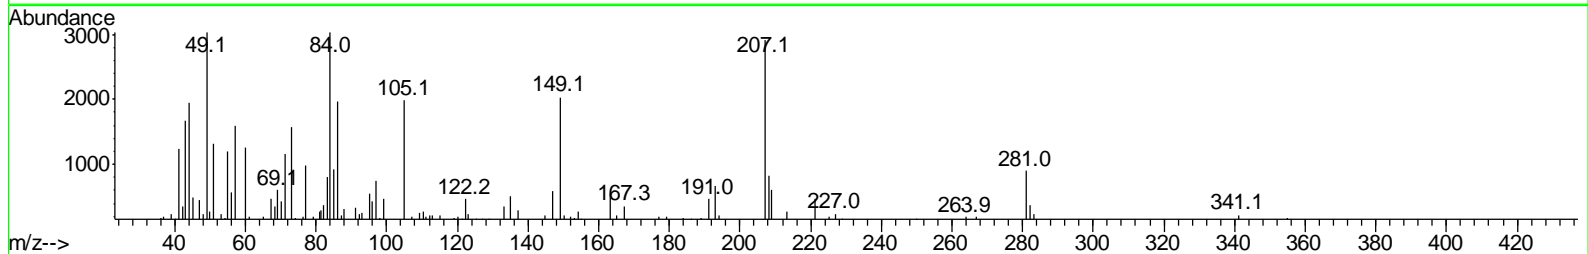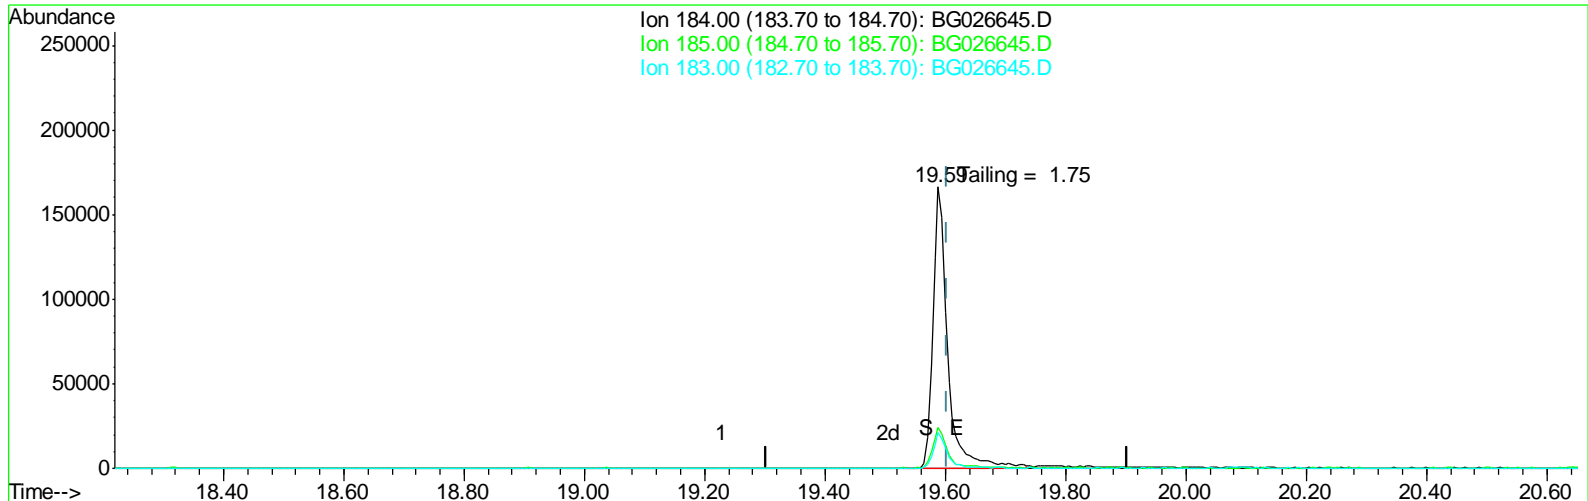

TIC: BG026645.D

(76) Benzidine

19.230min (-0.374) 42.52ng

response 65

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	13.80	0.00#
0.00	0.00	0.00