


Data Path : Z:\HPCHEM1\BNA G\DATA\BG041817\
 Data File : BG026645.D
 Acq On : 18 Apr 2017 12:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 18 18:04:39 2017

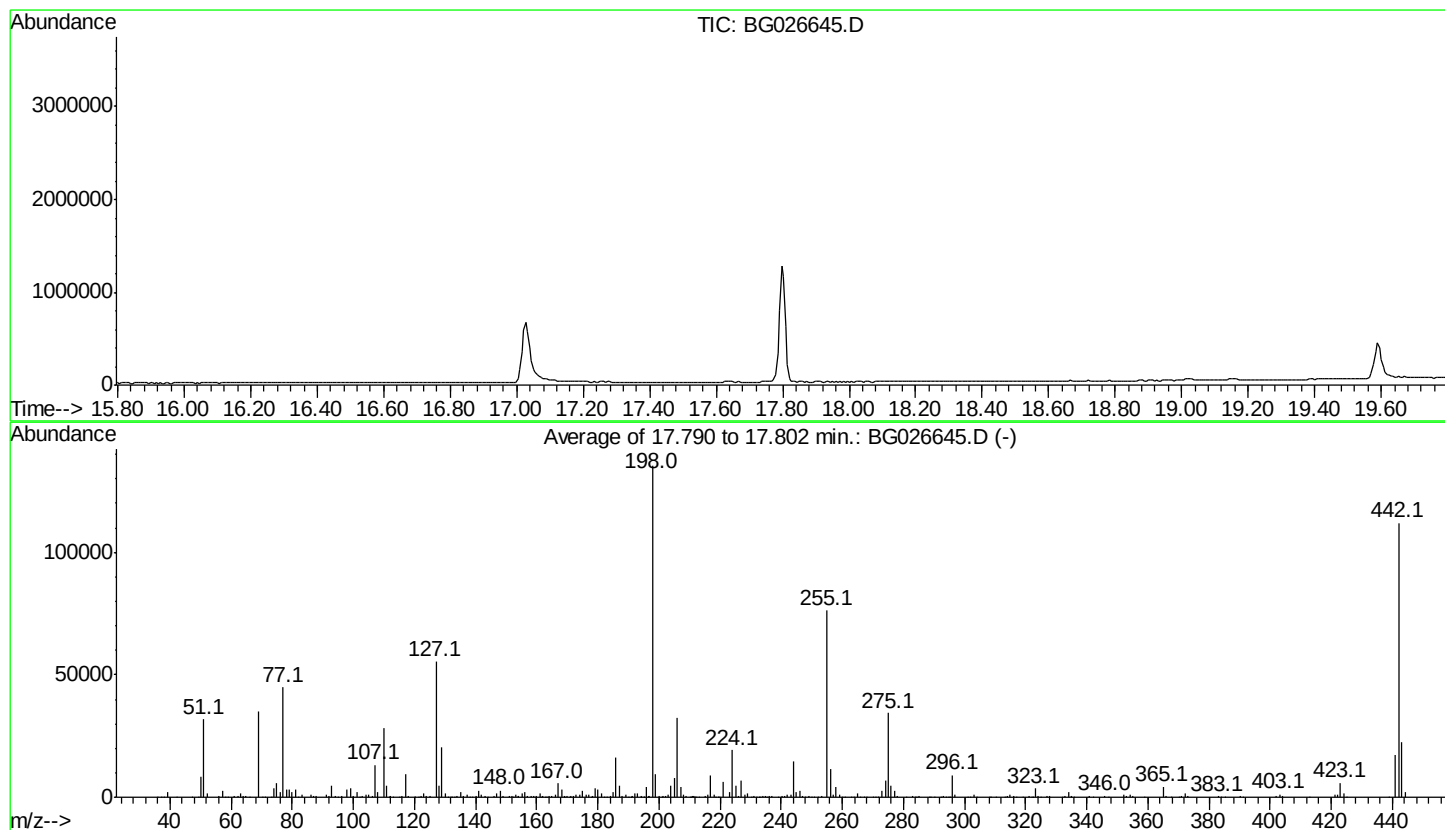

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	31752	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.9	35093	PASS
70	69	0.00	2	0.1	36	PASS
127	198	10	80	40.9	55349	PASS
197	198	0.00	2	0.4	482	PASS
198	198	100	100	100.0	135424	PASS
199	198	5	9	6.9	9340	PASS
275	198	10	60	25.3	34314	PASS
365	198	1	100	3.1	4258	PASS
441	442	0.01	24	15.4	17260	PASS
442	198	50	100	82.7	112032	PASS
443	442	15	24	20.3	22736	PASS