
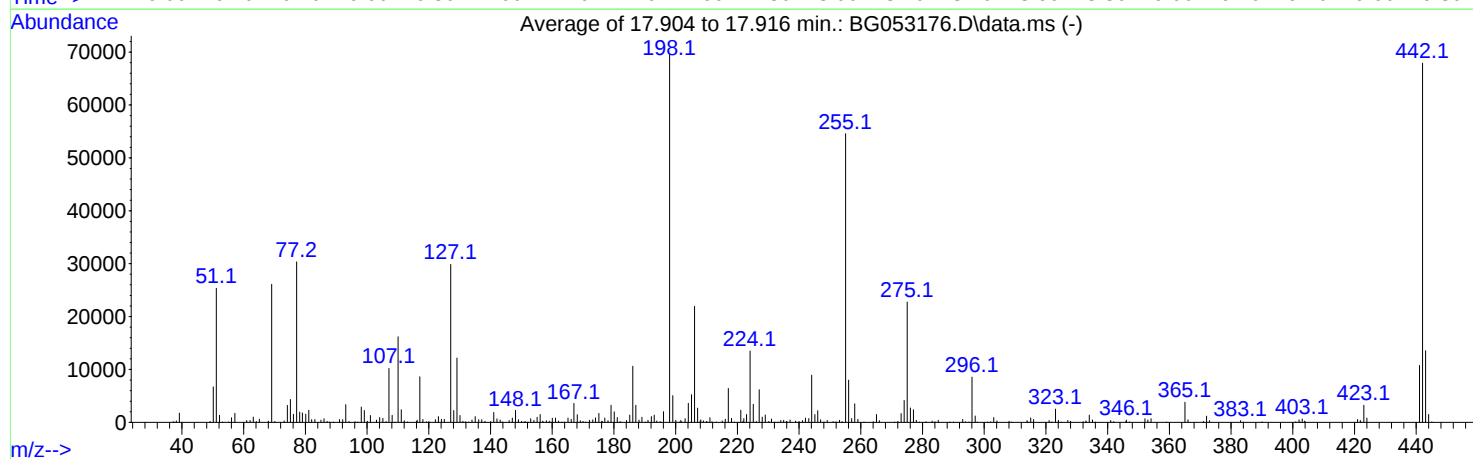


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041822\
 Data File : BG053176.D
 Acq On : 18 Apr 2022 10:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 15:31:24 2022

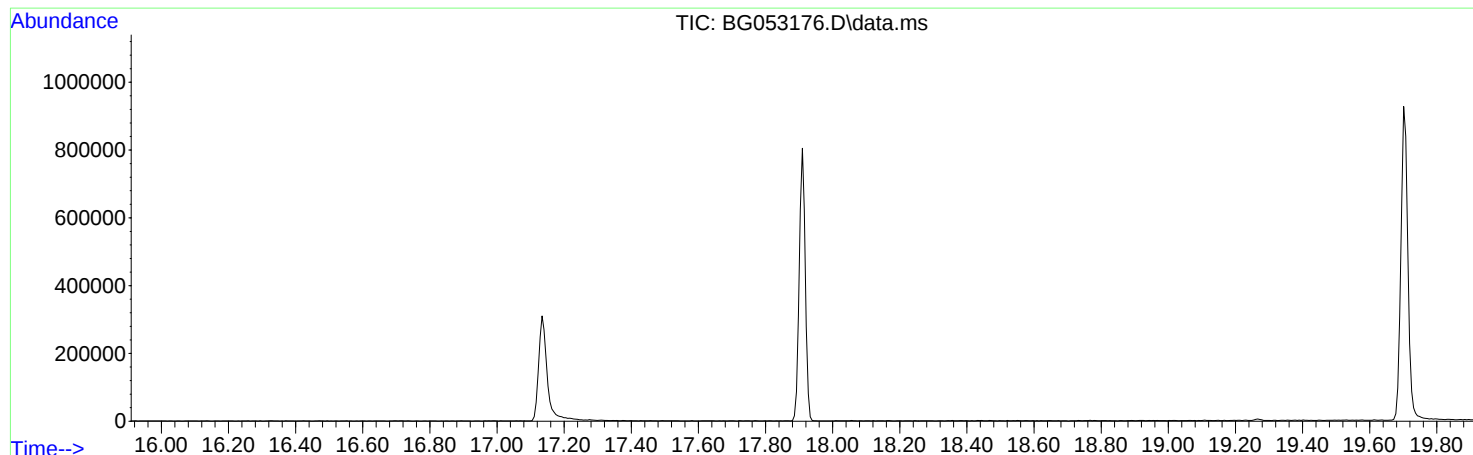




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	25352	PASS
68	69	0.00	2	1.0	251	PASS
69	198	0.00	100	37.6	26117	PASS
70	69	0.00	2	0.7	173	PASS
127	198	10	80	42.9	29867	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69544	PASS
199	198	5	9	7.3	5046	PASS
275	198	10	60	32.7	22749	PASS
365	198	1	100	5.5	3819	PASS
441	198	0.01	100	15.5	10769	PASS
442	442	50	100	100.0	67904	PASS
443	442	15	24	20.0	13550	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041822\
Data File : BG053176.D
Acq On : 18 Apr 2022 10:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 08:02:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

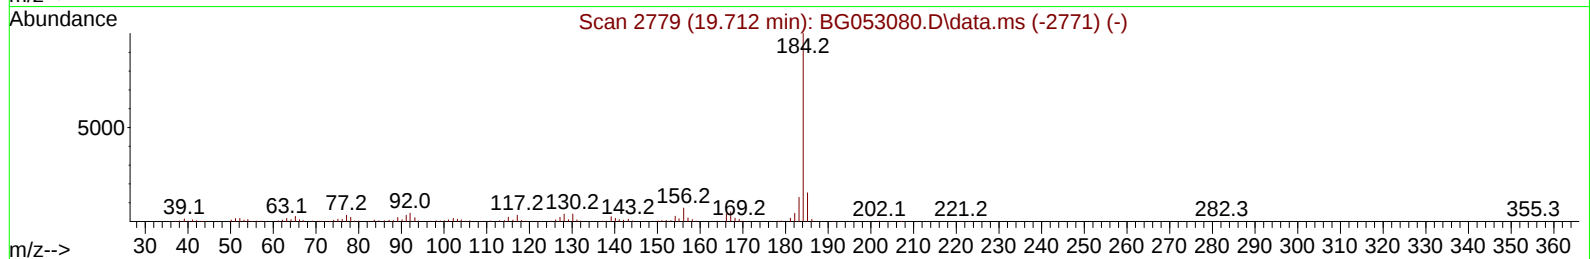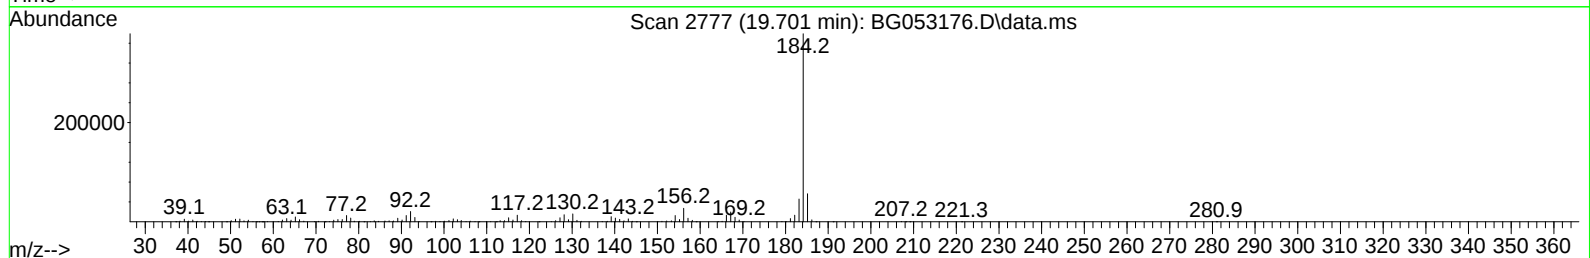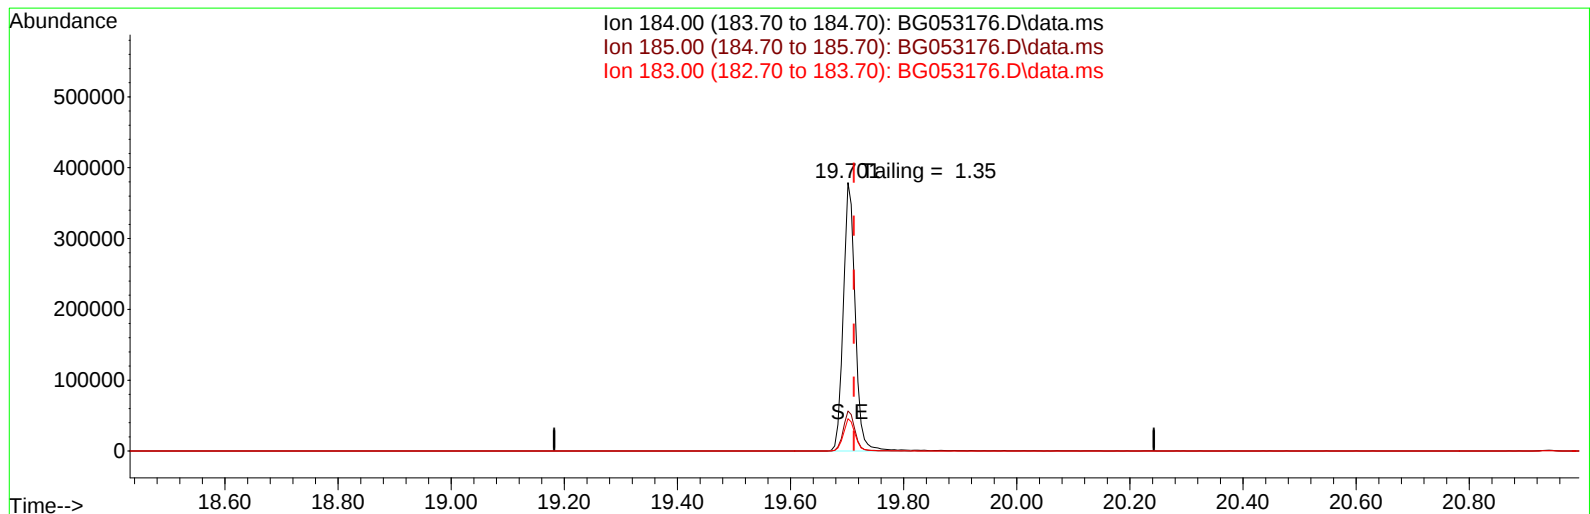

TIC: BG053176.D\data.ms

(77) Benzidine

19.701min (-0.011) 0.00 ng




response 554365

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.90
183.00	11.80	12.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041822\
Data File : BG053176.D
Acq On : 18 Apr 2022 10:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 08:02:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

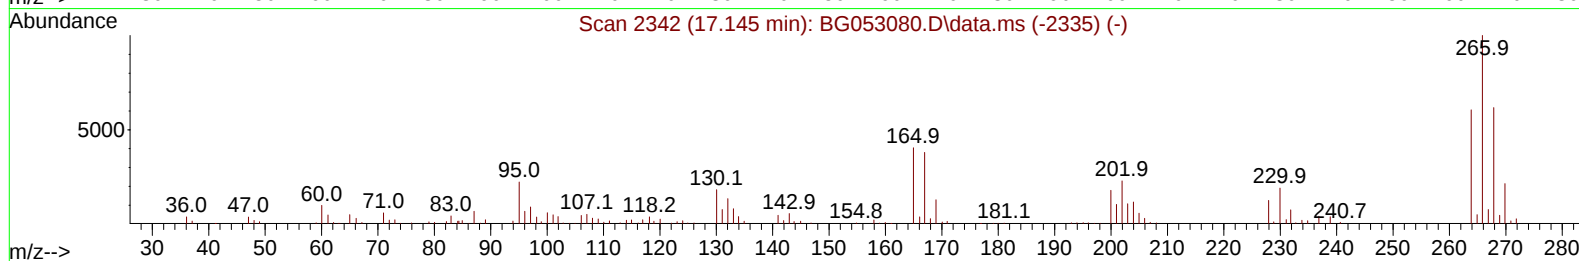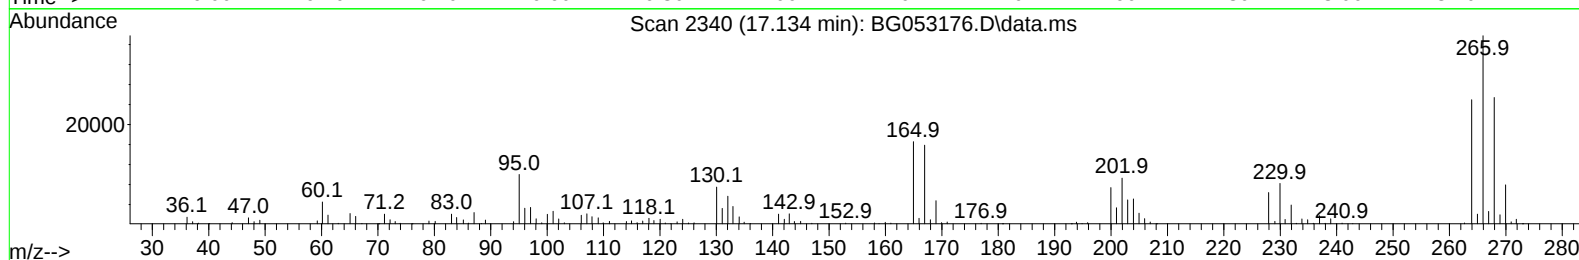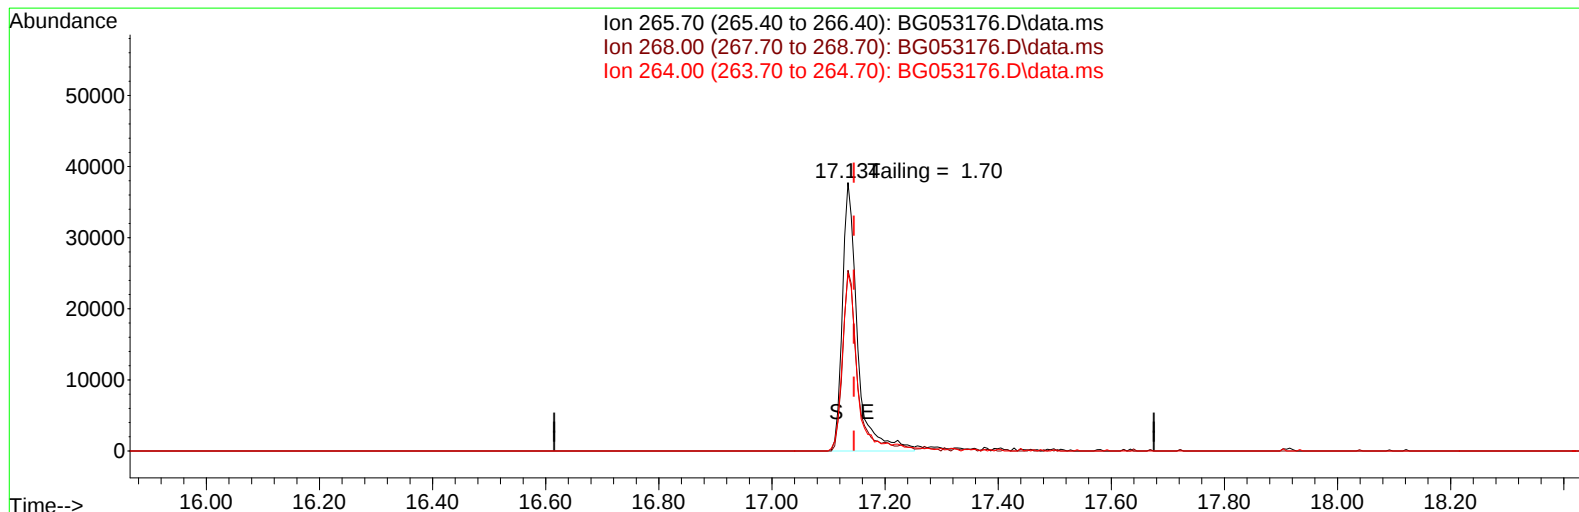

TIC: BG053176.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.011) 20588.44 ng

response 70731

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.34
264.00	56.60	66.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/18/2022	BNA_G	<u>BG053176.D</u>
Compound Name	Response	Retention Time
DDT	290623	20.941
DDD	5151	20.5
DDE	567	19.989
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5718	296341	1.93

Instrument :
BNA_G
ClientSampleId :
DFTPP