
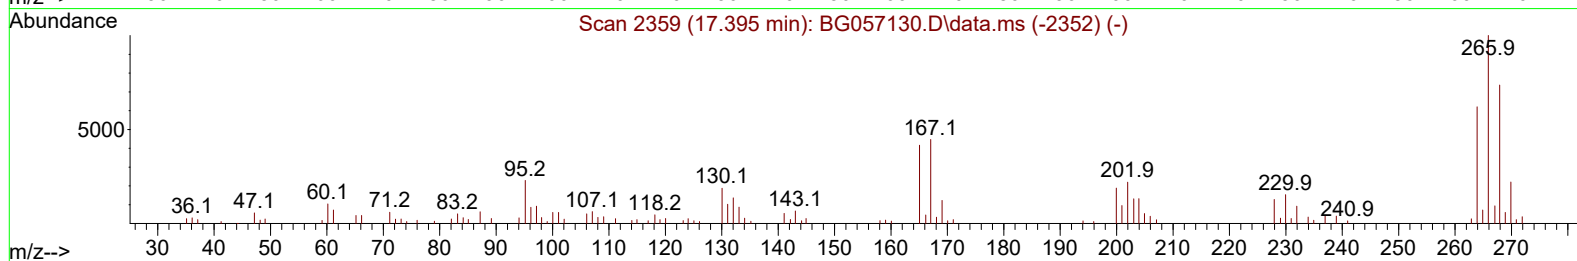
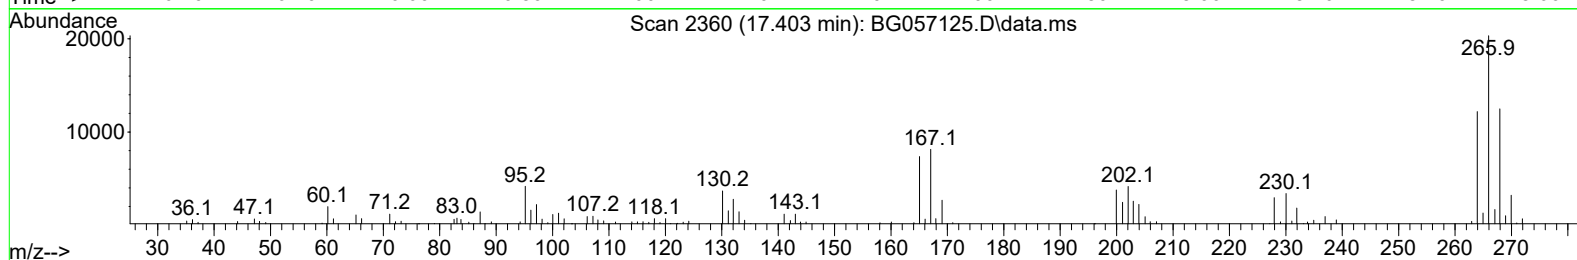


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041823\
Data File : BG057125.D
Acq On : 18 Apr 2023 14:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:18:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 04:21:14 2023
Response via : Initial Calibration

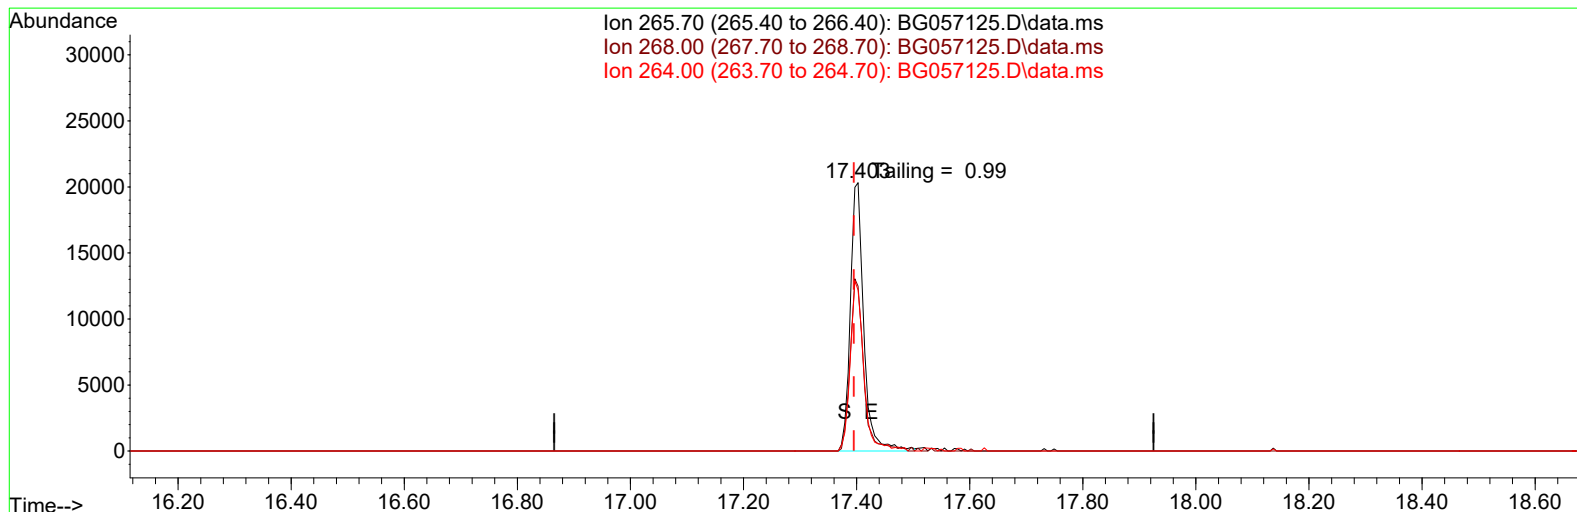

TIC: BG057125.D\data.ms

(70) Pentachlorophenol (C)

17.403min (+ 0.008) 17642.00 ng

response 33447

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	73.60	61.41
--------	-------	-------

264.00	62.00	59.93
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041823\
Data File : BG057125.D
Acq On : 18 Apr 2023 14:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 07:18:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 04:21:14 2023
Response via : Initial Calibration

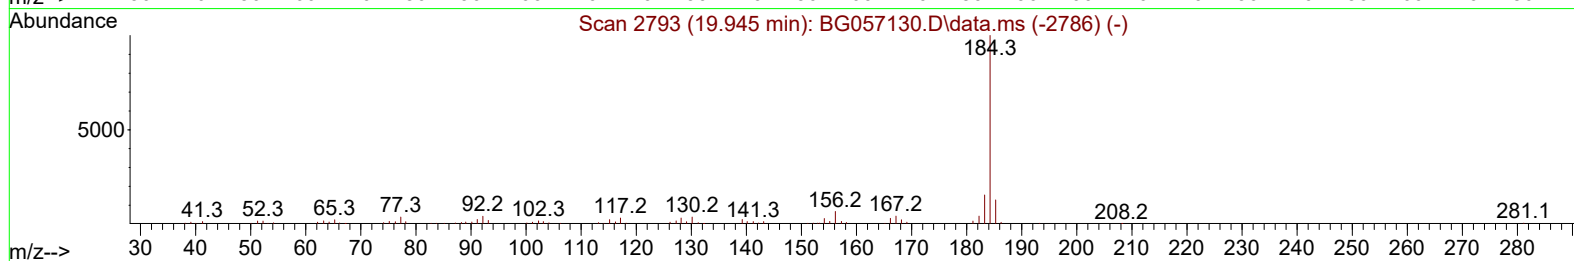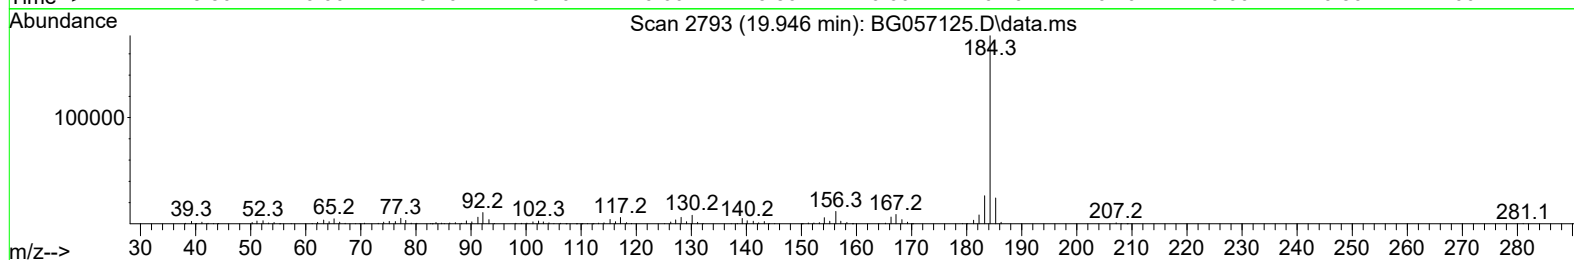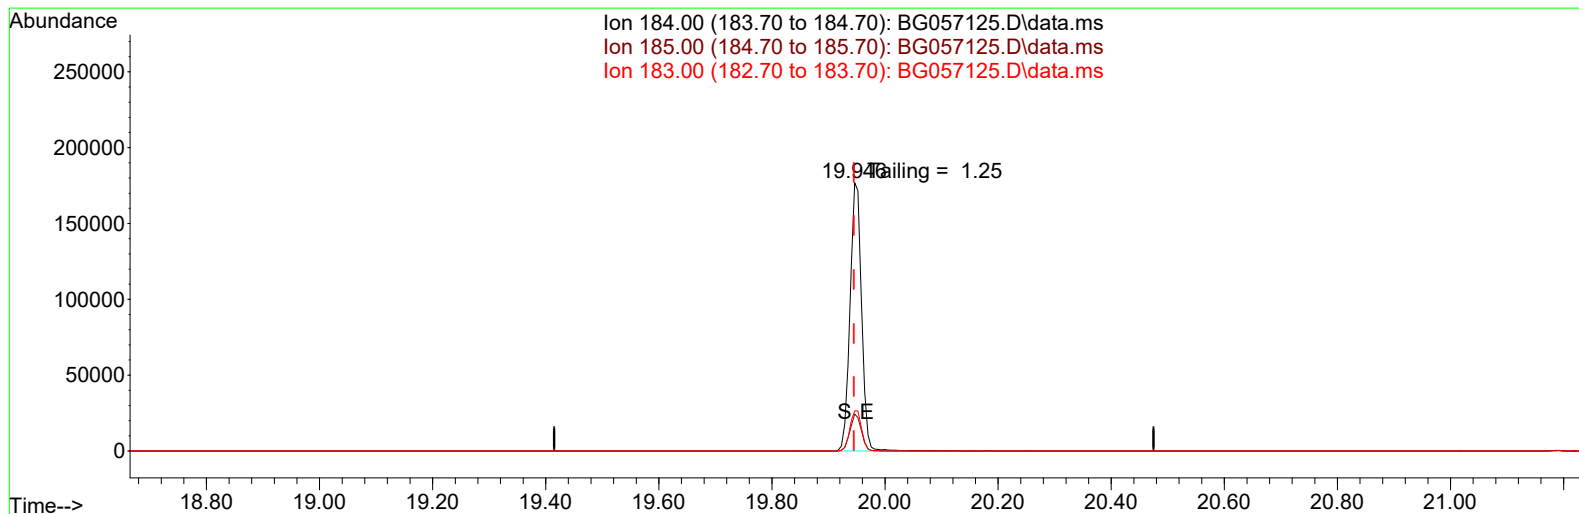

TIC: BG057125.D\data.ms

(77) Benzidine**19.946min (+ 0.001) 0.00 ng****response 250536**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.80	13.82
183.00	15.40	15.00
0.00	0.00	0.00