


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041823\
Data File : BG057125.D
Acq On : 18 Apr 2023 14:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 19 04:21:14 2023

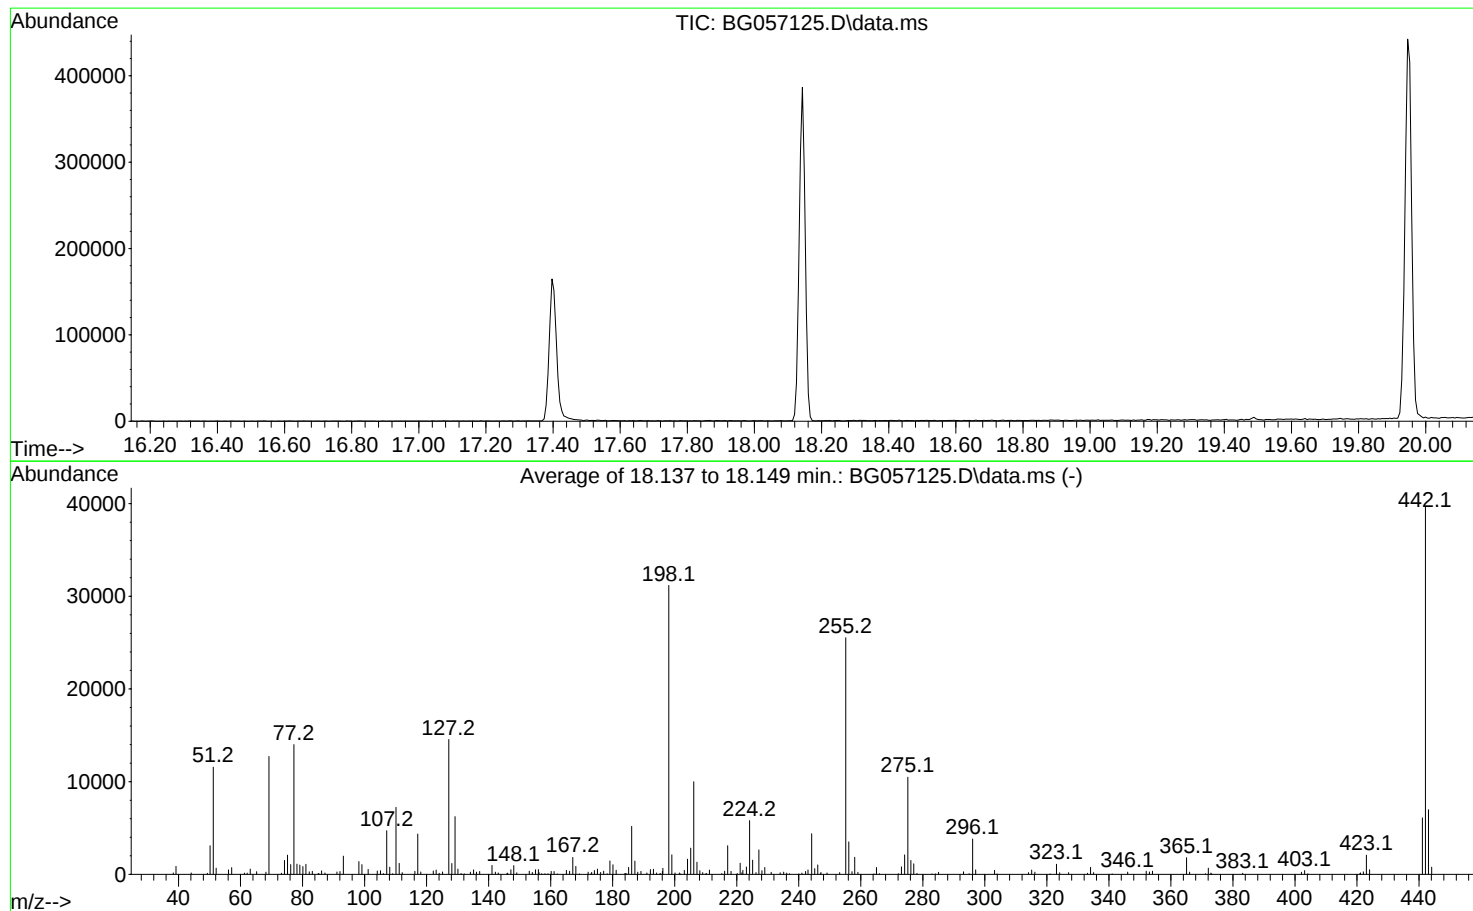

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	11569	PASS
68	69	0.00	2	1.9	247	PASS
69	198	0.00	100	40.8	12720	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	14554	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31173	PASS
199	198	5	9	6.8	2110	PASS
275	198	10	60	33.6	10476	PASS
365	198	1	100	5.8	1805	PASS
441	198	0.01	100	19.5	6091	PASS
442	442	50	100	100.0	39685	PASS
443	442	15	24	17.6	6979	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/18/2023	BNA_G	<u>BG057125.D</u>
Compound Name	Response	Retention Time
DDT	112920	21.186
DDD	1541	20.78
DDE	0	20.217
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1541	114461	1.35

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041823\
Data File : BG057125.D
Acq On : 18 Apr 2023 14:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 07:18:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 04:21:14 2023
Response via : Initial Calibration

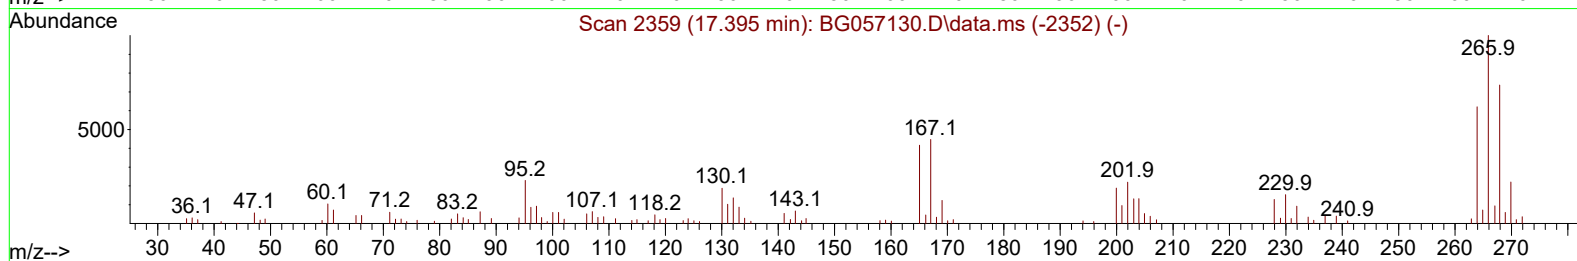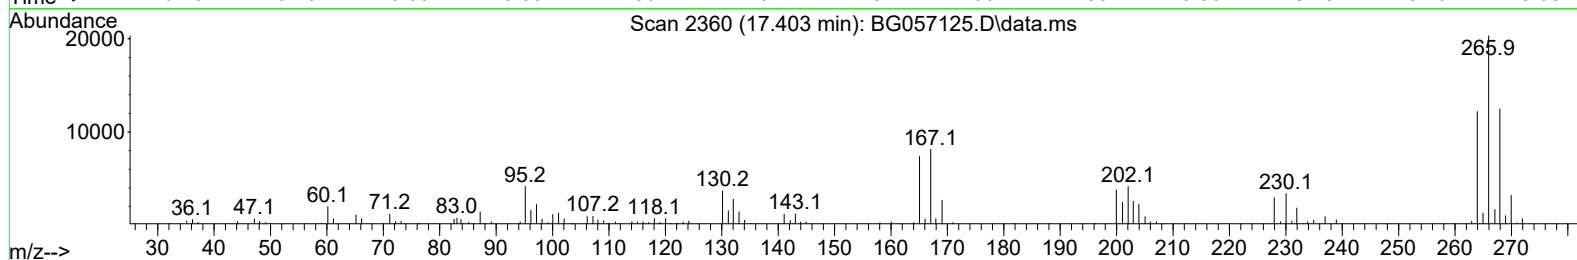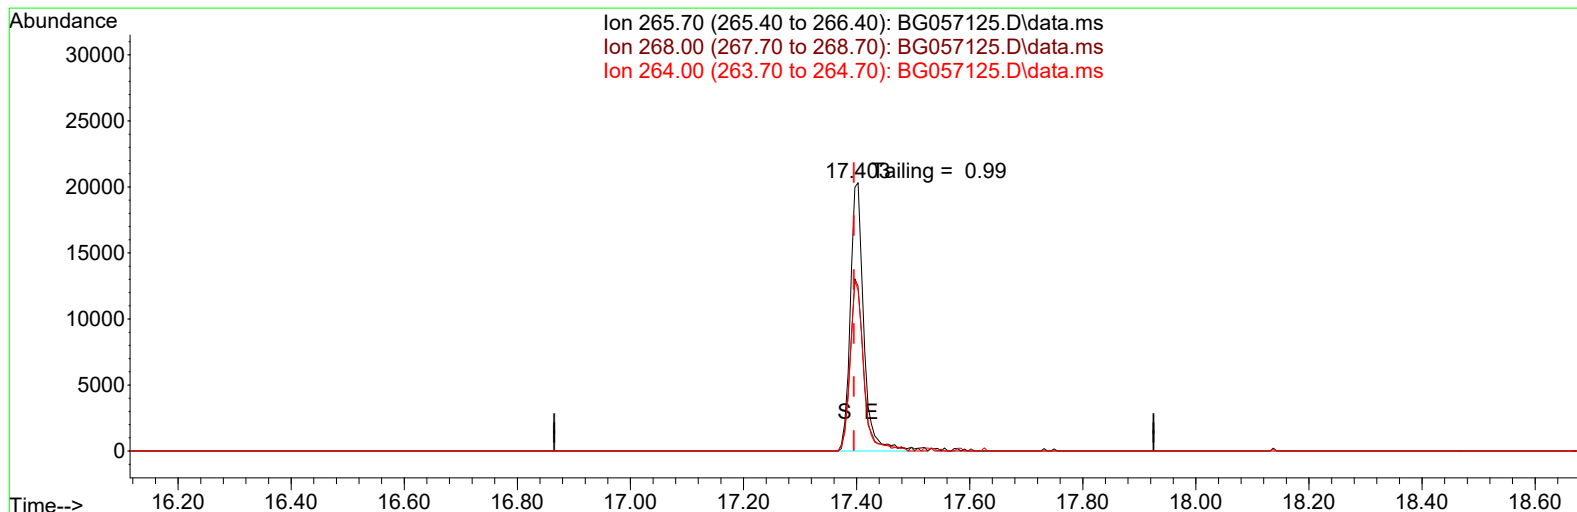

TIC: BG057125.D\data.ms

(70) Pentachlorophenol (C)

17.403min (+ 0.008) 17642.00 ng




response 33447

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	73.60	61.41
264.00	62.00	59.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041823\
Data File : BG057125.D
Acq On : 18 Apr 2023 14:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 07:18:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 19 04:21:14 2023
Response via : Initial Calibration

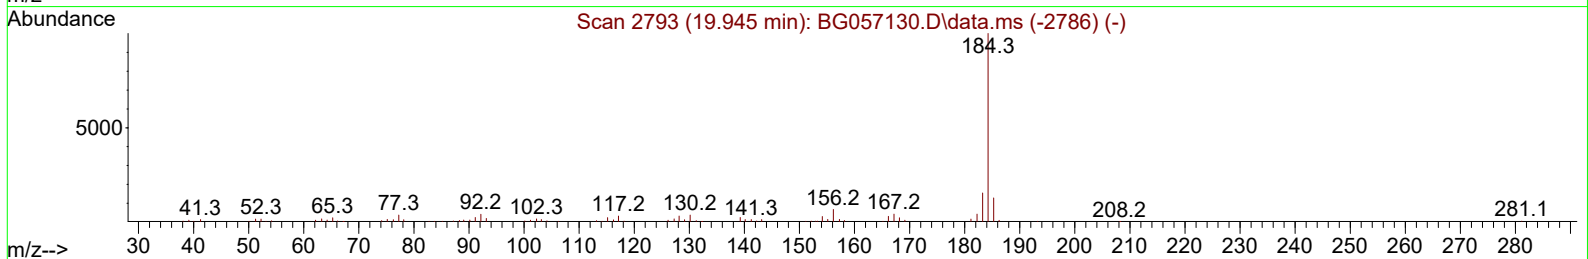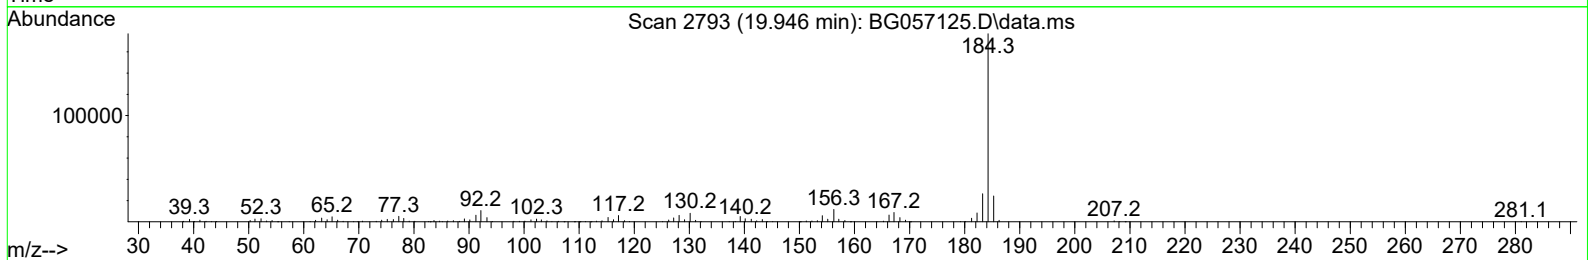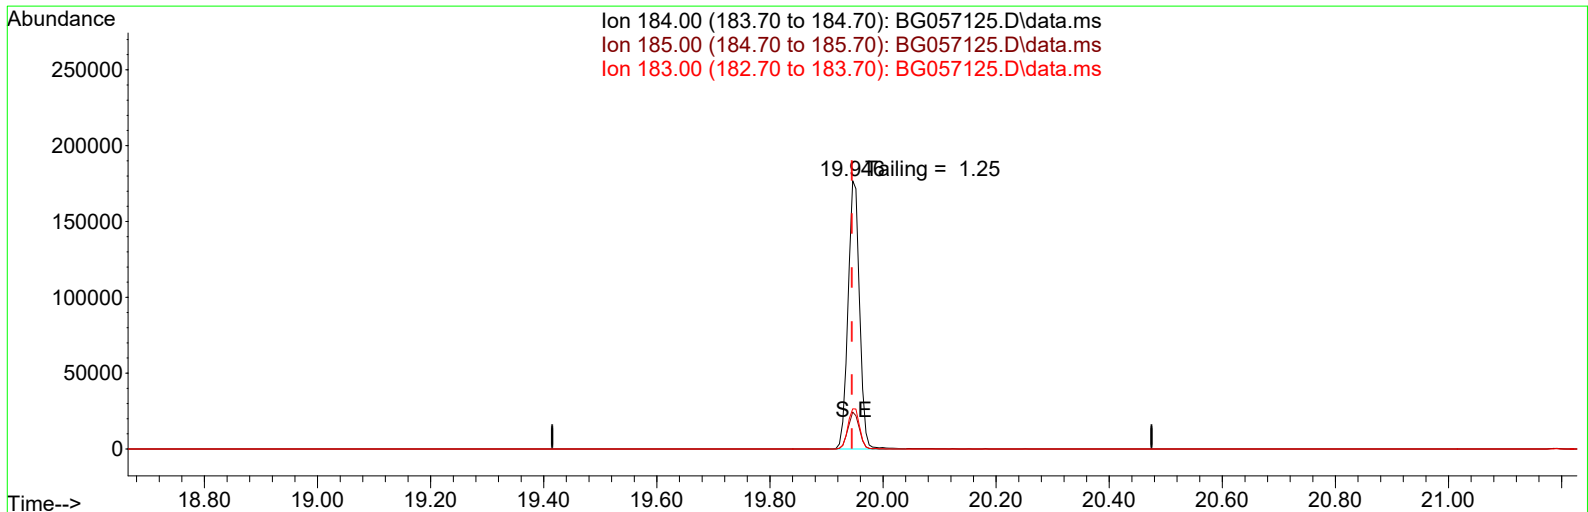

TIC: BG057125.D\data.ms

(77) Benzidine

19.946min (+ 0.001) 0.00 ng

response 250536

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.80	13.82
183.00	15.40	15.00
0.00	0.00	0.00