
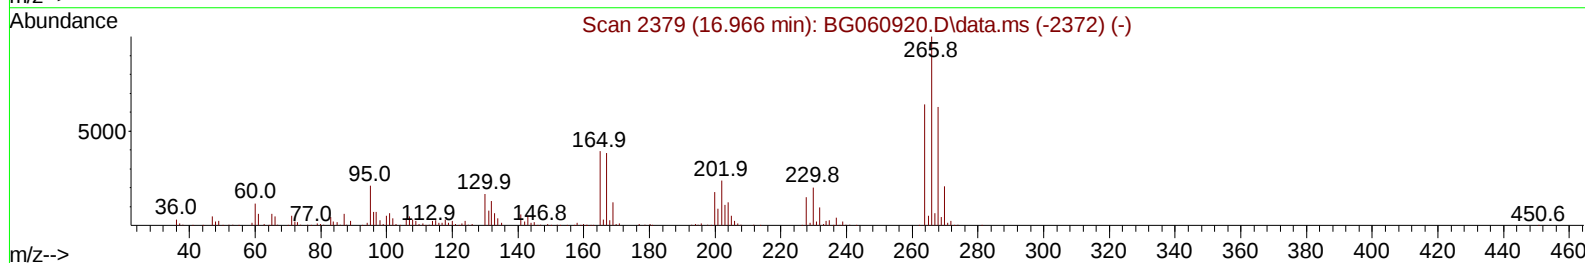
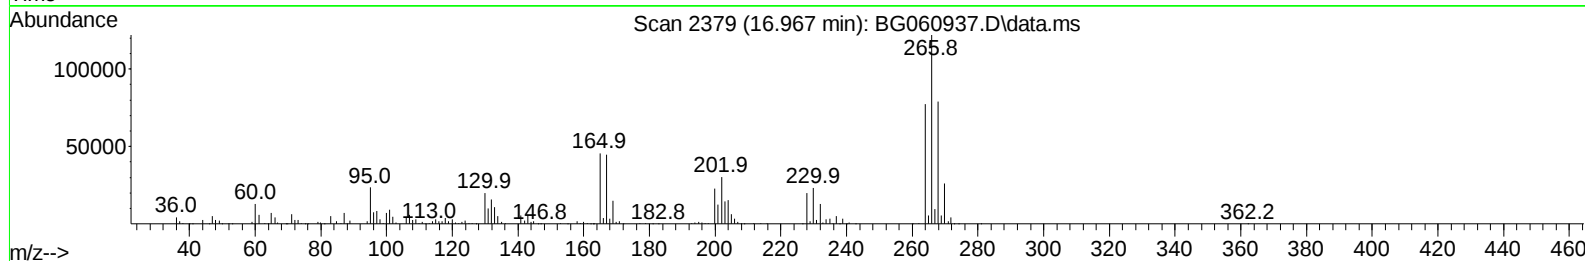


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060937.D
Acq On : 18 Apr 2024 15:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 01:43:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

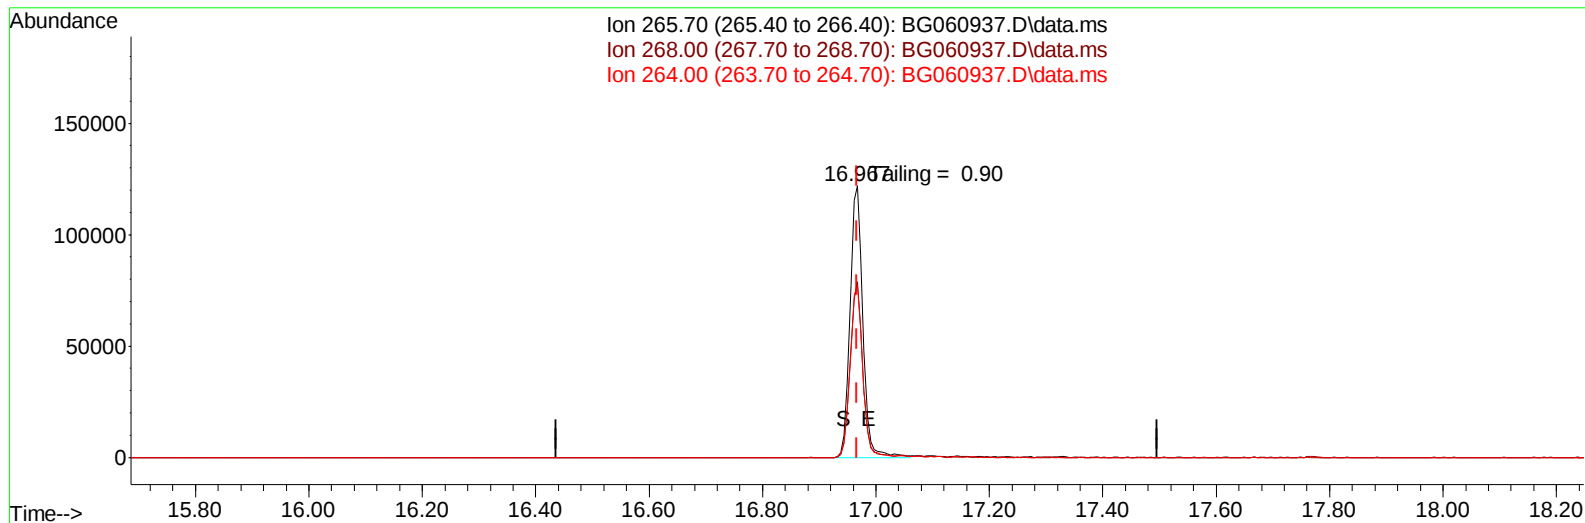




TIC: BG060937.D\data.ms

(70) Pentachlorophenol (C)**16.967min (+ 0.001) 23710.07 ng****response 189860**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.67
264.00	64.00	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060937.D
Acq On : 18 Apr 2024 15:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 01:43:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

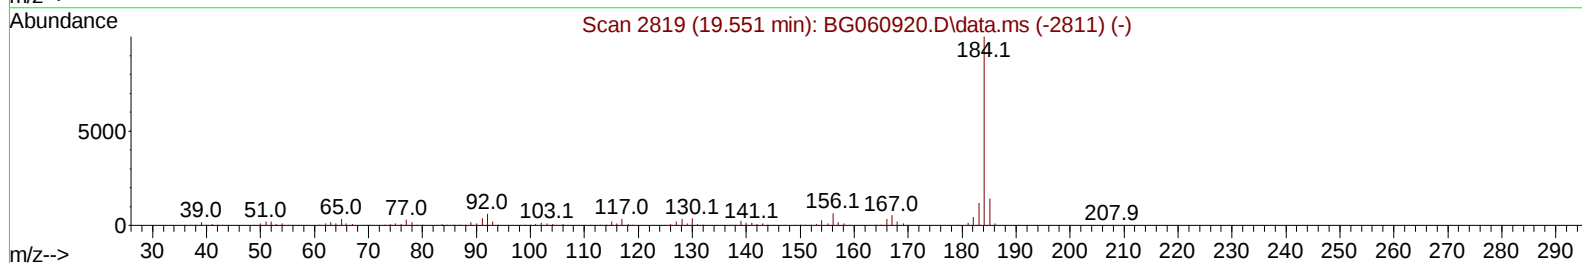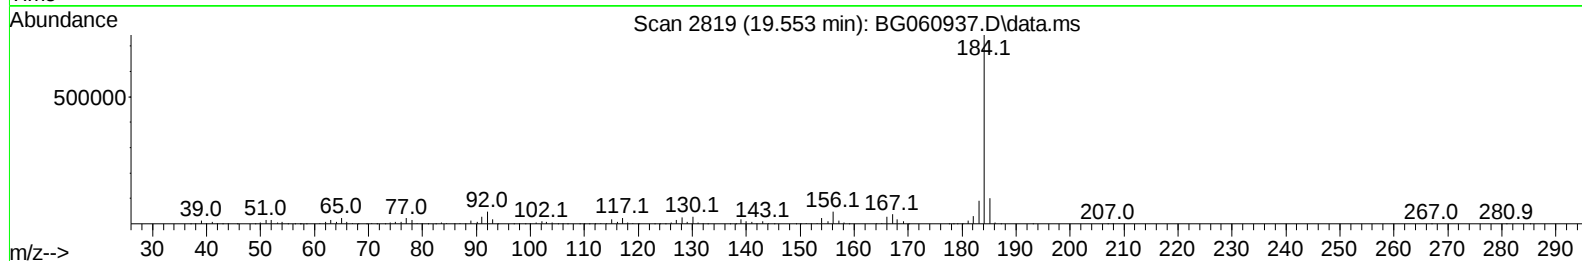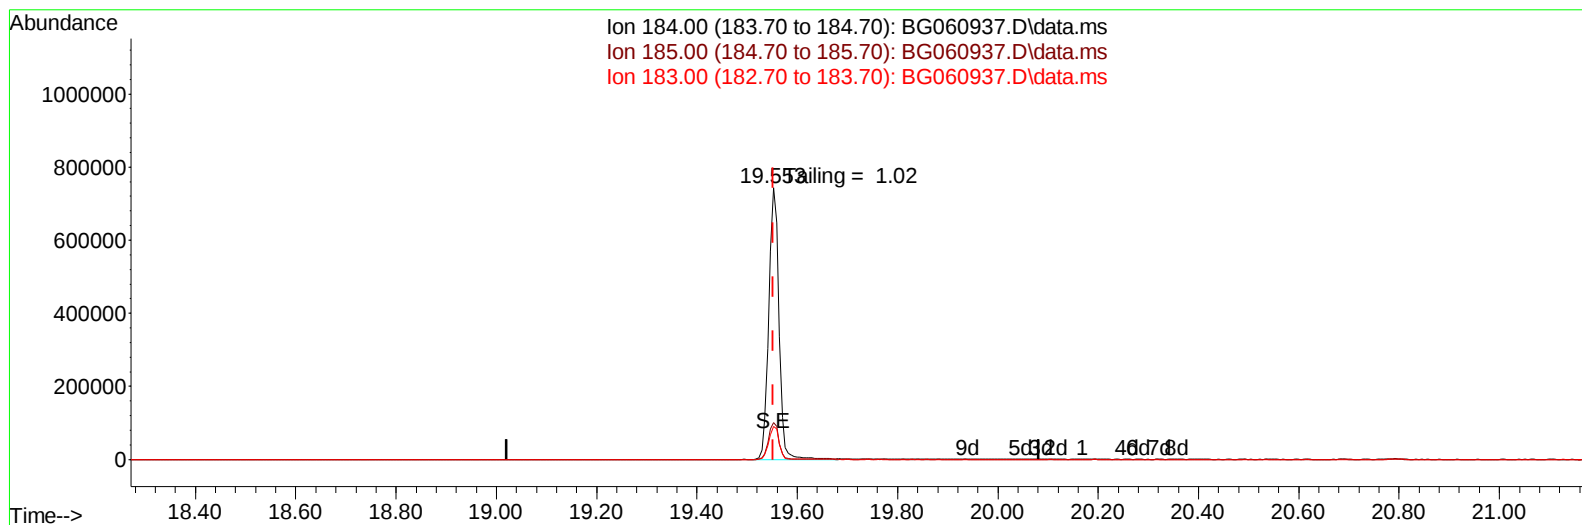

TIC: BG060937.D\data.ms

(77) Benzidine**19.553min (+ 0.001) 766582.35 ng m****response 1065250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.59
183.00	11.80	12.15
0.00	0.00	0.00