

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041824\  
Data File : BG060933.D  
Acq On : 18 Apr 2024 12:28  
Operator : MA/JU  
Sample : PB160330BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB160330BL

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG041724.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060933.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.527       | 425           | 432         | 443          | rBV      | 993003         | 1550445       | 27.25%          | 7.855%        |
| 2         | 7.107       | 693           | 701         | 709          | rBV      | 975837         | 1670695       | 29.36%          | 8.464%        |
| 3         | 7.936       | 836           | 842         | 850          | rVB      | 168496         | 283630        | 4.99%           | 1.437%        |
| 4         | 9.093       | 1030          | 1039        | 1048         | rBV      | 601485         | 1072456       | 18.85%          | 5.433%        |
| 5         | 10.733      | 1310          | 1318        | 1327         | rBV      | 215837         | 362181        | 6.37%           | 1.835%        |
| 6         | 13.194      | 1728          | 1737        | 1750         | rBV      | 1642571        | 2516677       | 44.23%          | 12.750%       |
| 7         | 14.569      | 1963          | 1971        | 1977         | rBV      | 385873         | 609250        | 10.71%          | 3.087%        |
| 8         | 16.056      | 2217          | 2224        | 2247         | rBV      | 1678884        | 2595764       | 45.62%          | 13.151%       |
| 9         | 17.313      | 2431          | 2438        | 2448         | rBV      | 668103         | 976863        | 17.17%          | 4.949%        |
| 10        | 19.940      | 2878          | 2885        | 2896         | rBV      | 4331933        | 5689429       | 100.00%         | 28.824%       |
| 11        | 21.573      | 3156          | 3163        | 3175         | rBV      | 723902         | 1189432       | 20.91%          | 6.026%        |
| 12        | 24.693      | 3684          | 3694        | 3707         | rBV2     | 408541         | 1221728       | 21.47%          | 6.190%        |




Sum of corrected areas: 19738550

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041824\  
Data File : BG060933.D  
Acq On : 18 Apr 2024 12:28  
Operator : MA/JU  
Sample : PB160330BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB160330BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG041724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

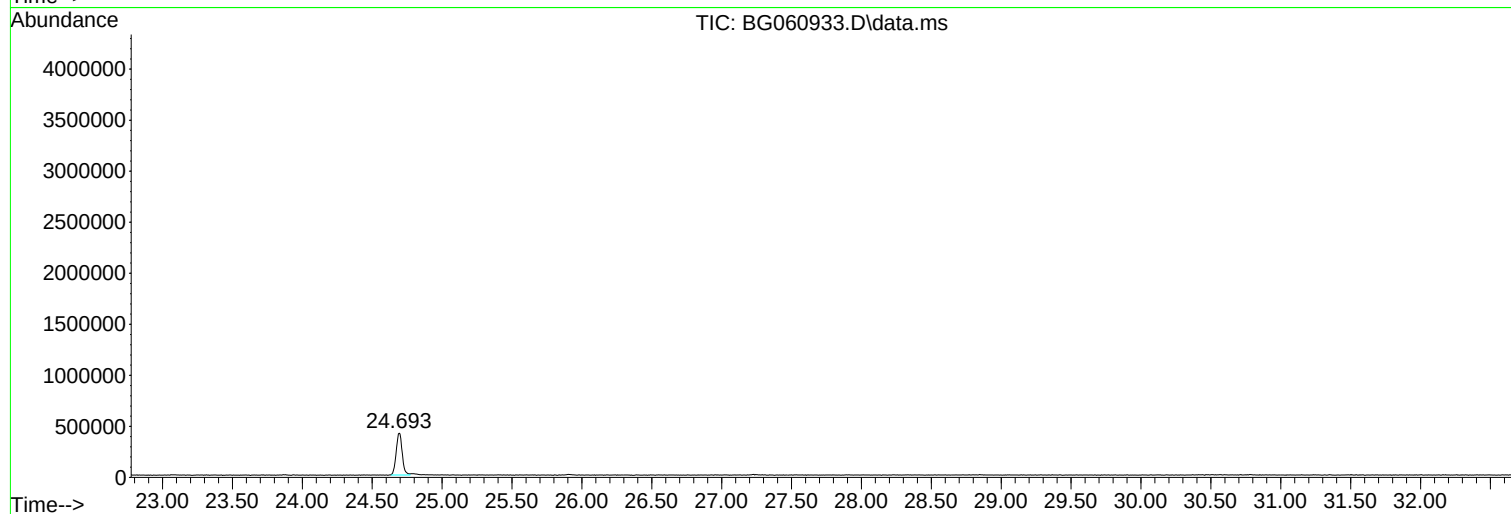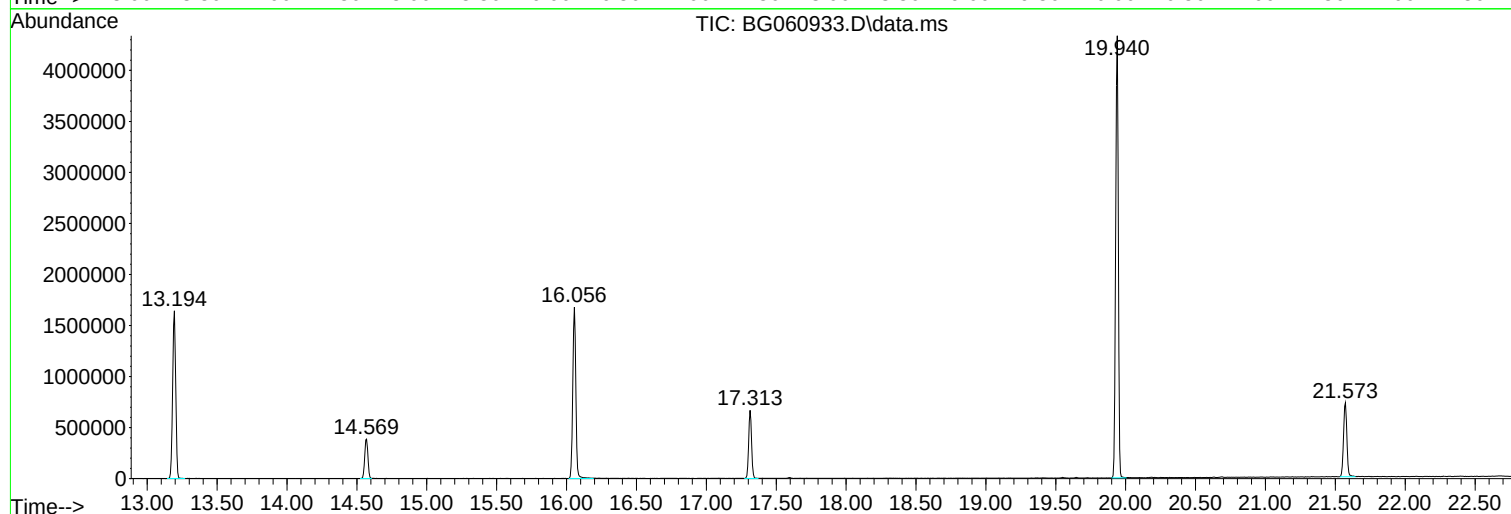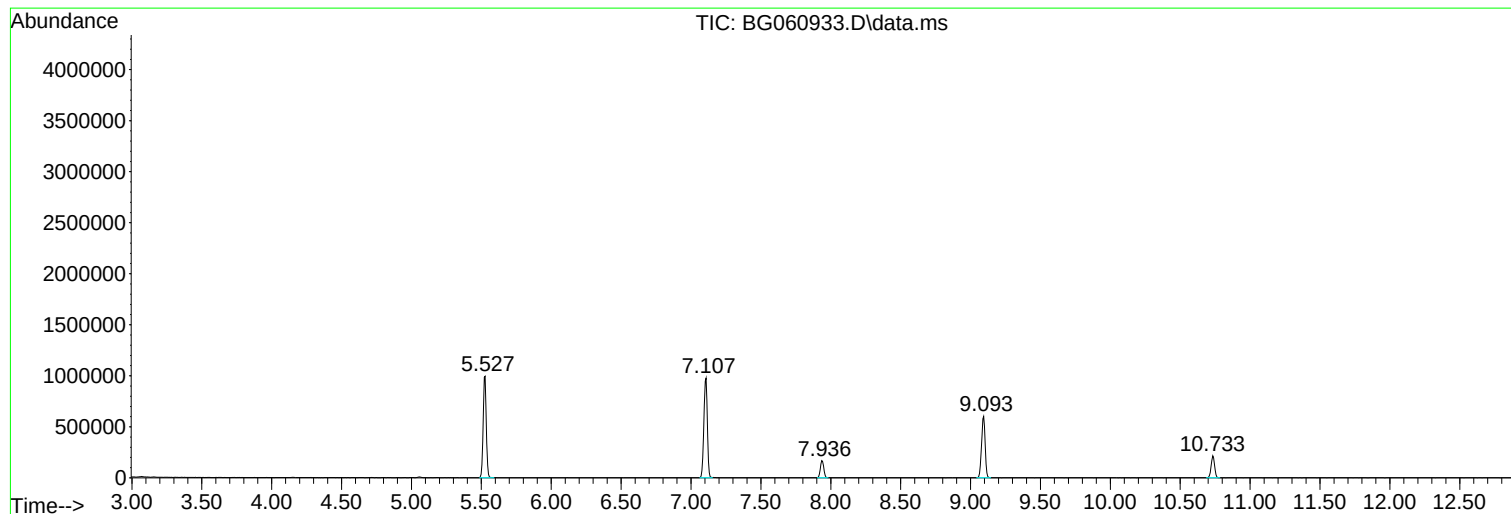

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041824\  
Data File : BG060933.D  
Acq On : 18 Apr 2024 12:28  
Operator : MA/JU  
Sample : PB160330BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB160330BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG041724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG041824\  
Data File : BG060933.D  
Acq On : 18 Apr 2024 12:28  
Operator : MA/JU  
Sample : PB160330BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB160330BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG041724.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|