
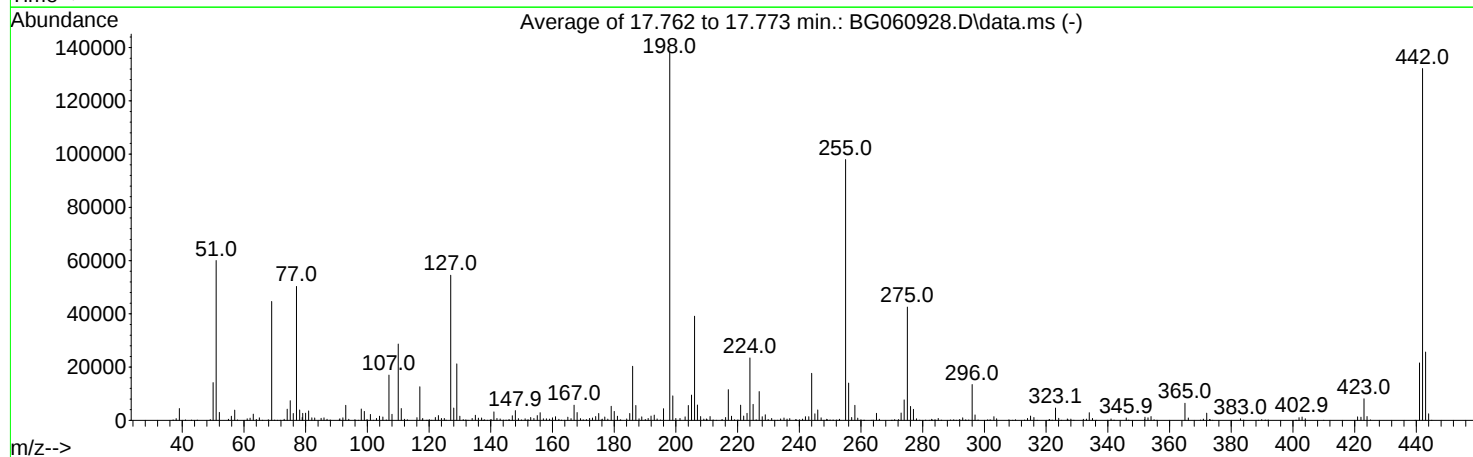


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060928.D
Acq On : 18 Apr 2024 8:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 18 02:02:19 2024

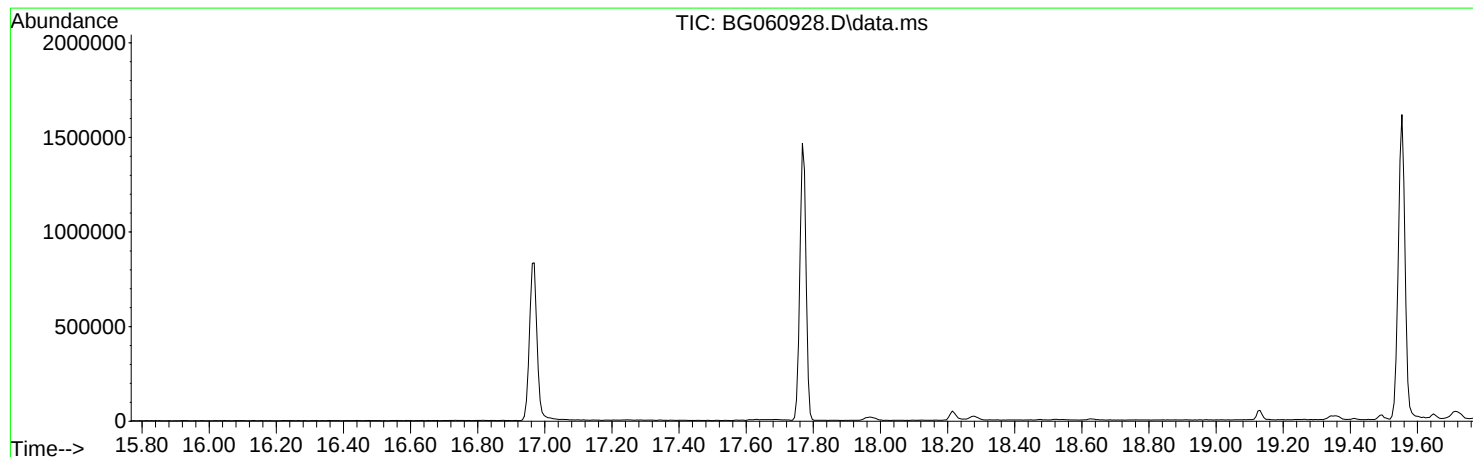




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	60037	PASS
68	69	0.00	2	0.6	249	PASS
69	198	0.00	100	32.3	44629	PASS
70	69	0.00	2	0.3	149	PASS
127	198	10	80	39.4	54507	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	138168	PASS
199	198	5	9	6.7	9194	PASS
275	198	10	60	30.8	42528	PASS
365	198	1	100	4.7	6453	PASS
441	198	0.01	100	15.6	21564	PASS
442	442	50	100	100.0	132165	PASS
443	442	15	24	19.4	25664	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060928.D
Acq On : 18 Apr 2024 8:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 18 12:22:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

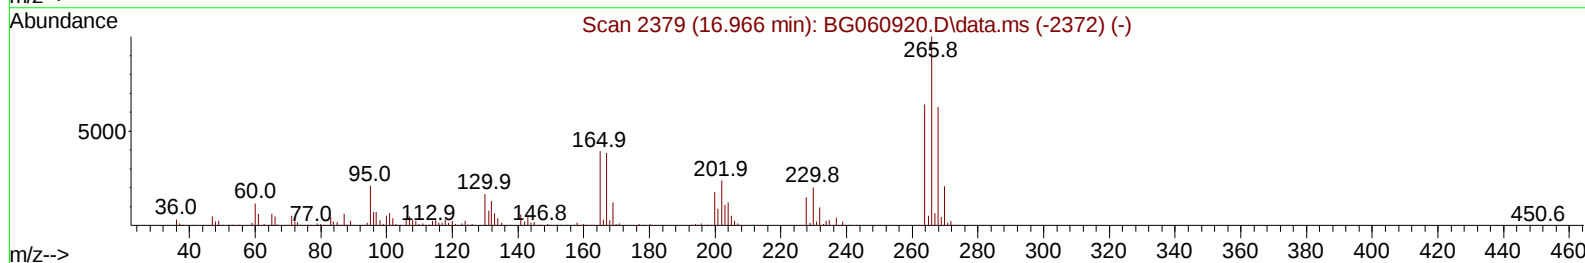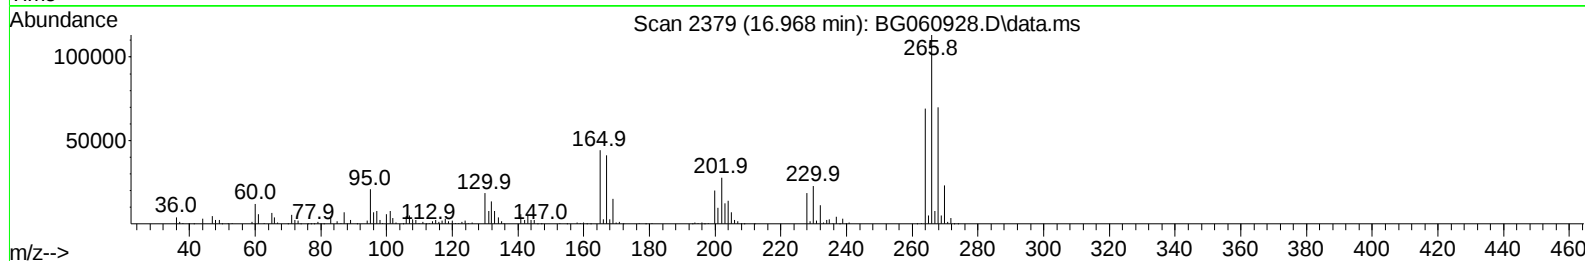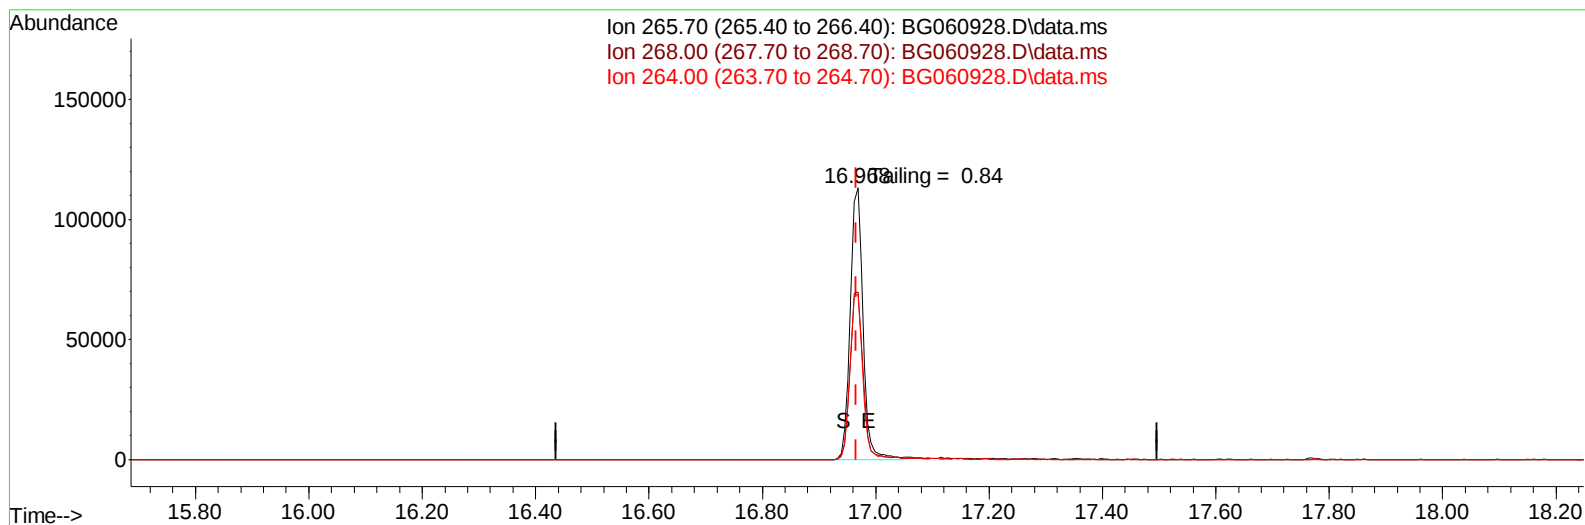

TIC: BG060928.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.002) 97461.47 ng




response 176200

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	61.77
264.00	64.00	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060928.D
Acq On : 18 Apr 2024 8:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 18 12:22:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

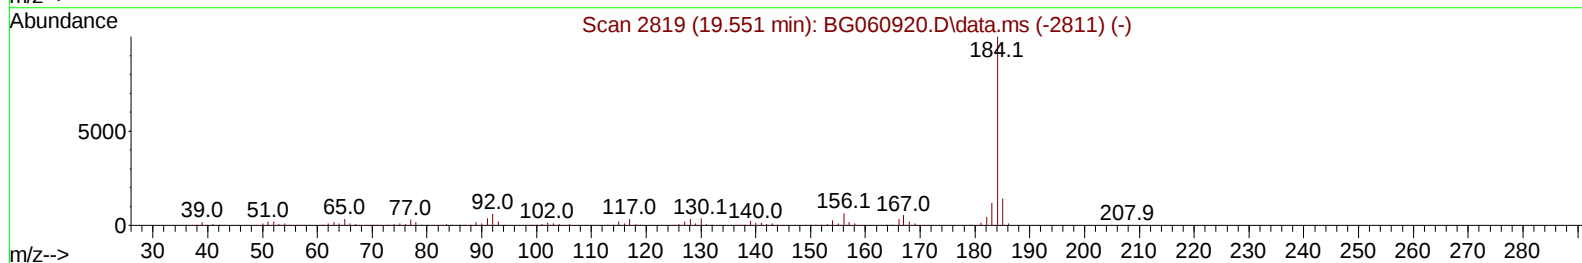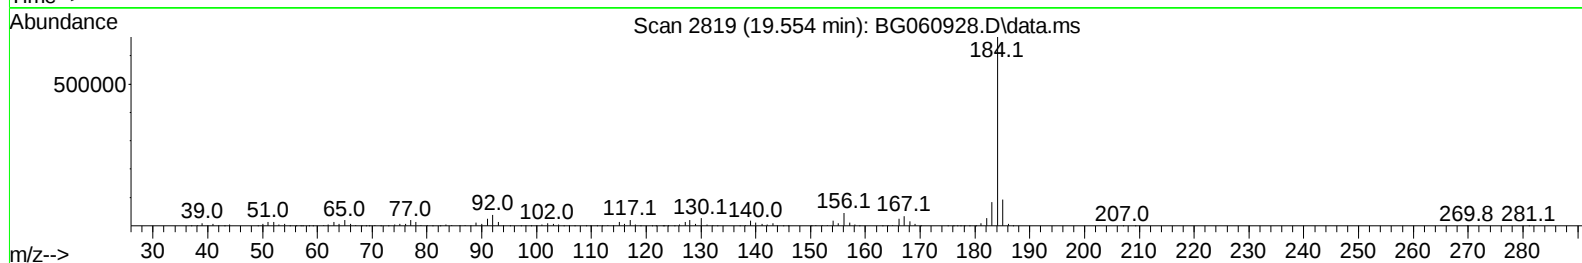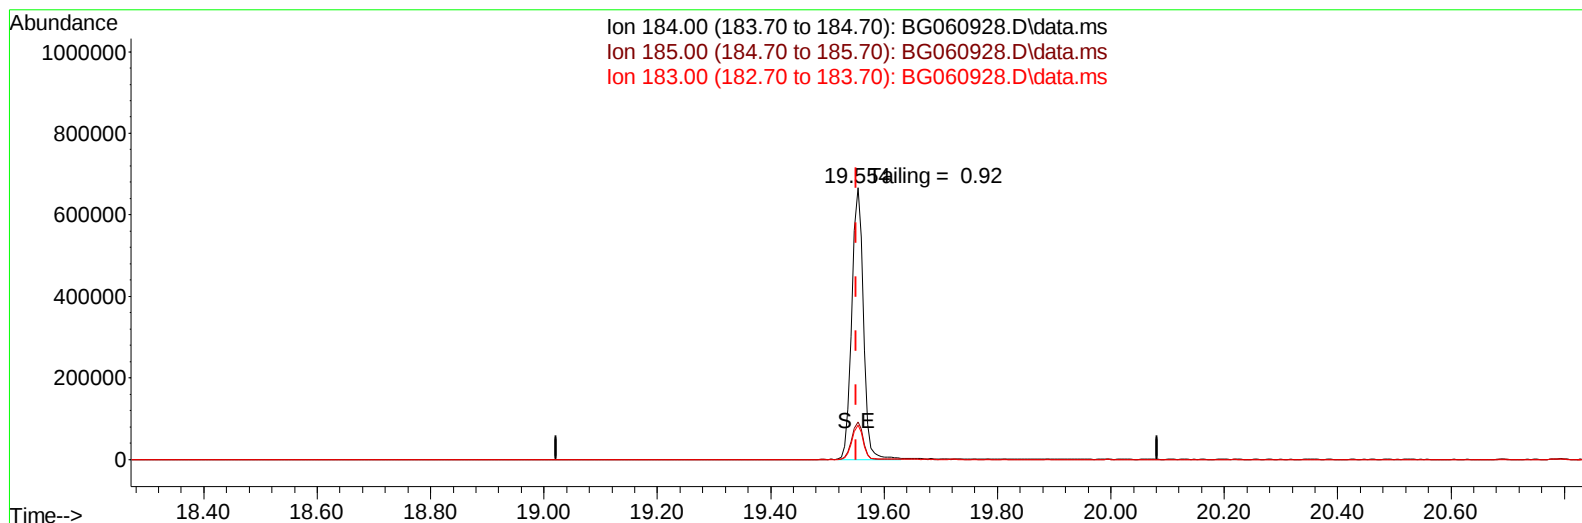

TIC: BG060928.D\data.ms

(77) Benzidine

19.554min (+ 0.002) 9473.87 ng

response 948505

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.94
183.00	11.80	12.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/18/2024	BNA_G	<u>BG060928.D</u>
Compound Name	Response	Retention Time
DDT	525363	20.793
DDD	14288	20.347
DDE	1791	19.847
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16079	541442	2.97

Instrument :
BNA_G
ClientSampleId :
DFTPP