


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060937.D
Acq On : 18 Apr 2024 15:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 18 02:02:19 2024

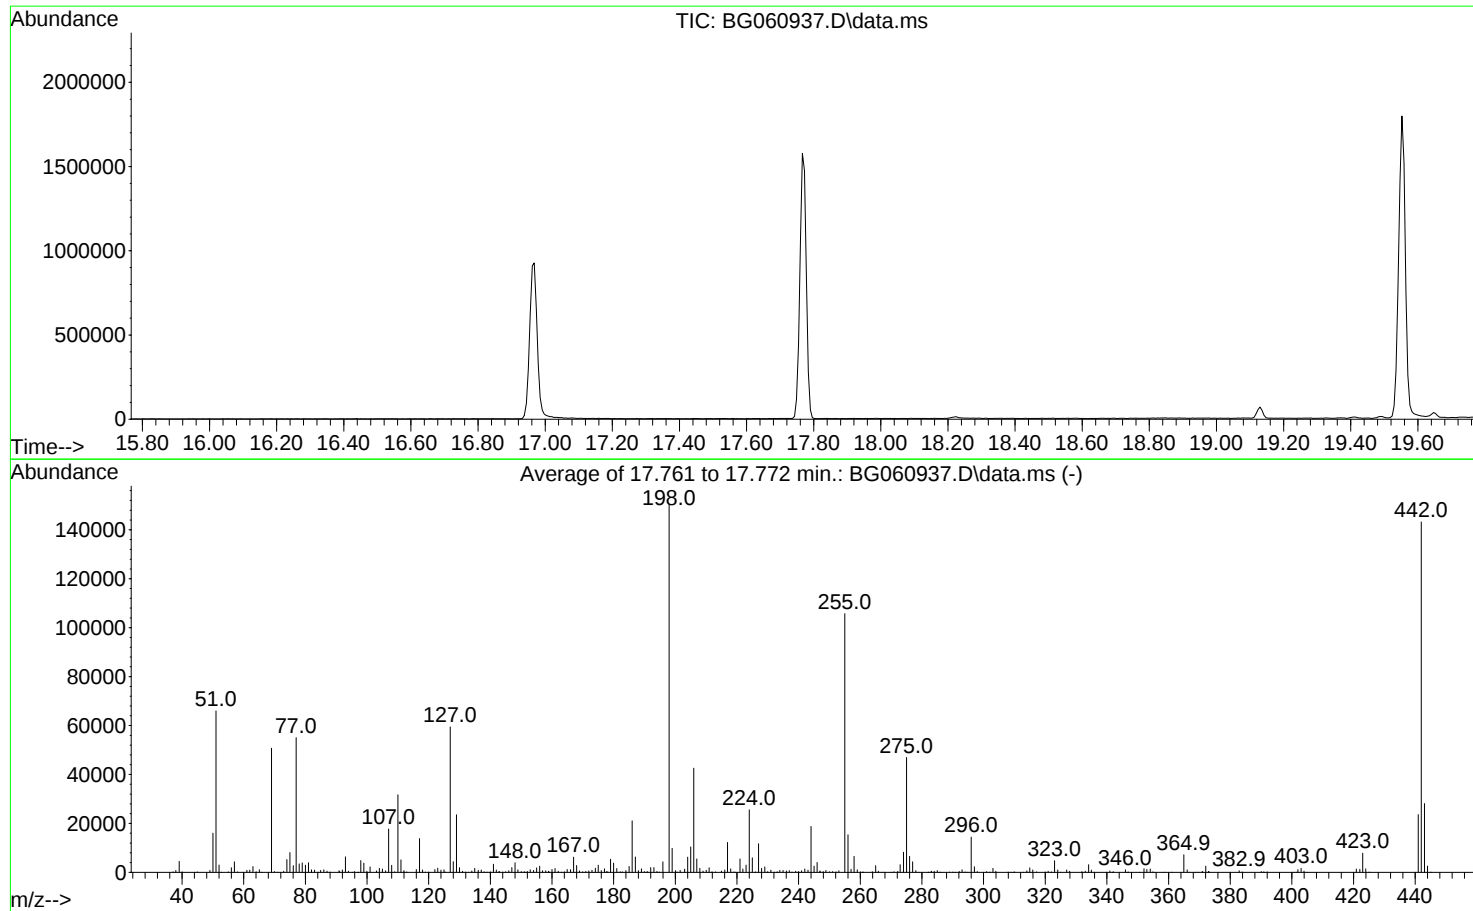




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	65997	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.7	50723	PASS
70	69	0.00	2	0.6	315	PASS
127	198	10	80	39.5	59451	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150331	PASS
199	198	5	9	6.5	9821	PASS
275	198	10	60	31.2	46925	PASS
365	198	1	100	4.8	7185	PASS
441	198	0.01	100	15.7	23599	PASS
442	442	50	100	100.0	143195	PASS
443	442	15	24	19.7	28144	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060937.D
Acq On : 18 Apr 2024 15:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 01:43:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

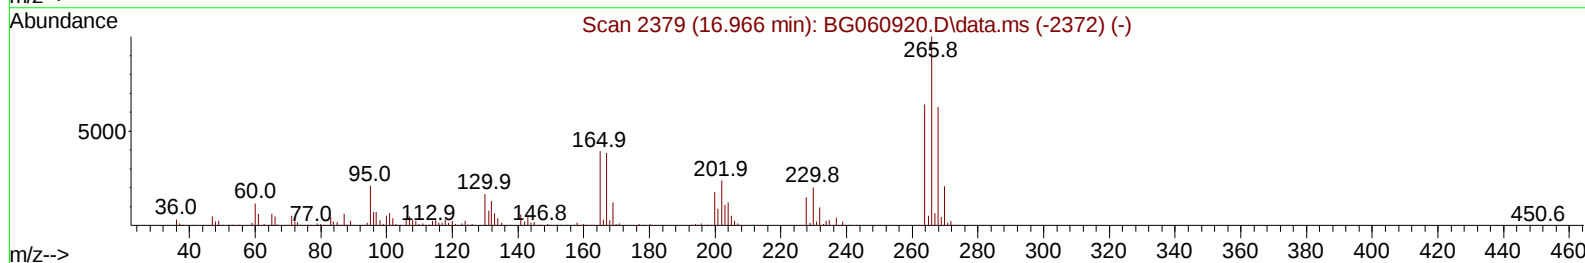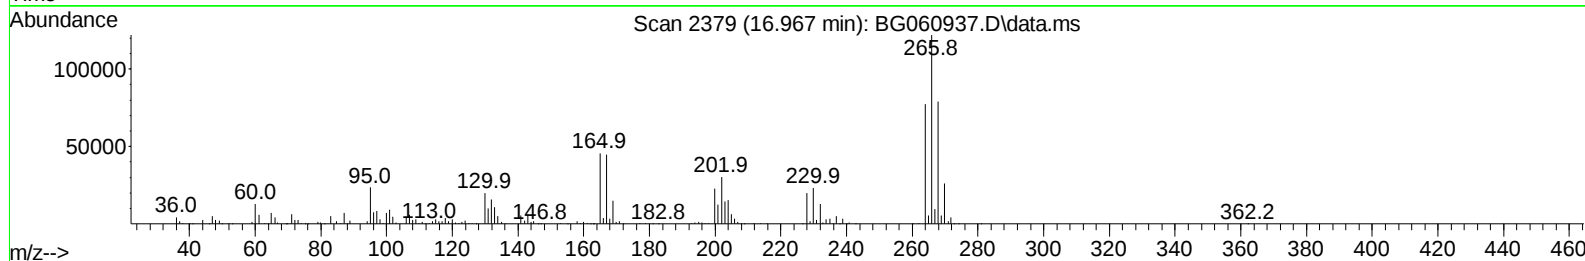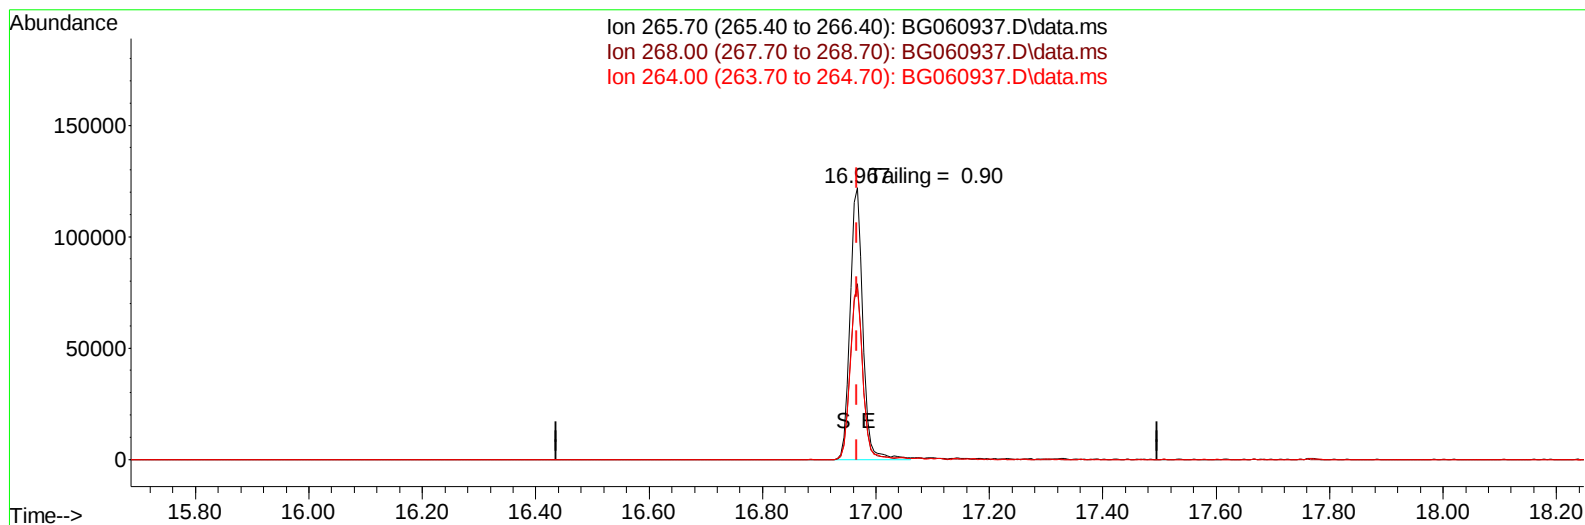

TIC: BG060937.D\data.ms

(70) Pentachlorophenol (C)

16.967min (+ 0.001) 23710.07 ng




response 189860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.67
264.00	64.00	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041824\
Data File : BG060937.D
Acq On : 18 Apr 2024 15:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 19 01:43:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG041724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 02:02:19 2024
Response via : Initial Calibration

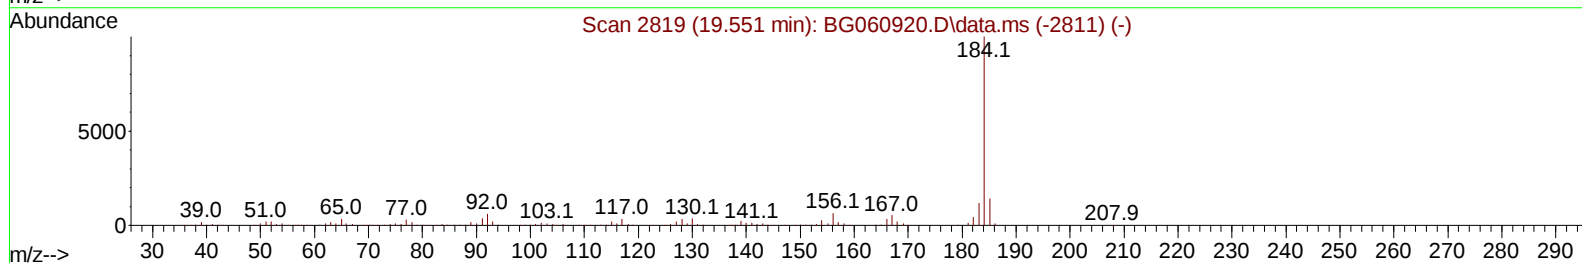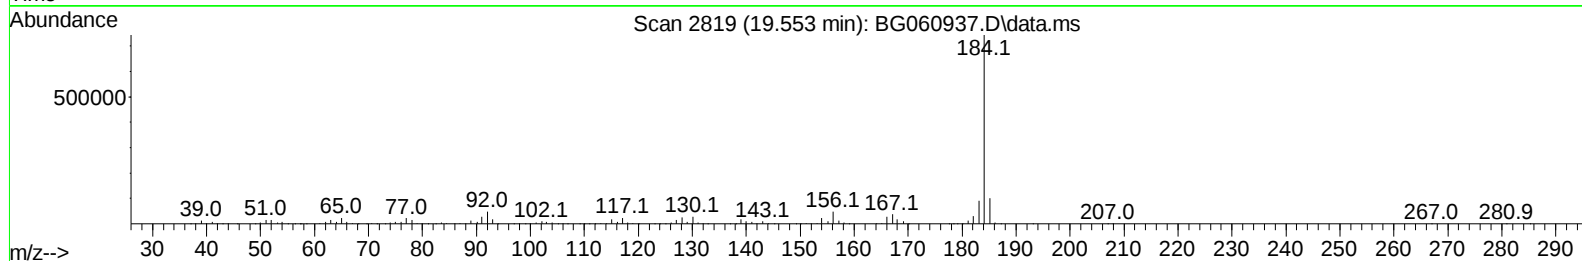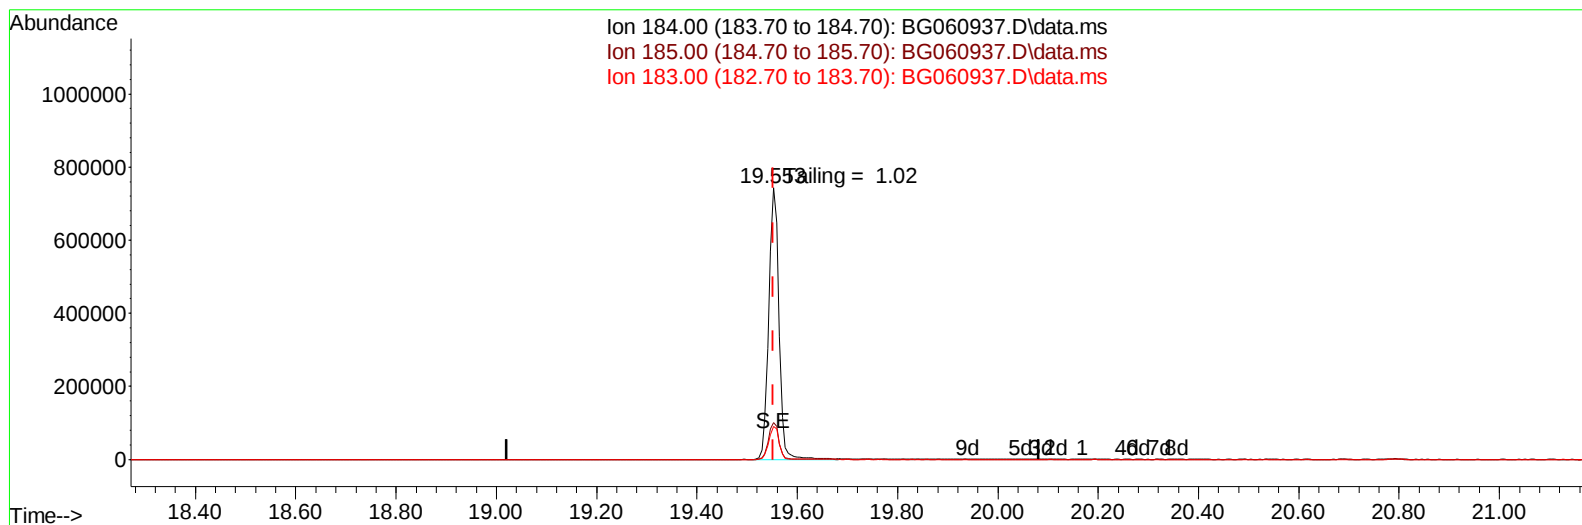

TIC: BG060937.D\data.ms

(77) Benzidine

19.553min (+ 0.001) 766582.35 ng m

response 1065250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.59
183.00	11.80	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/18/2024	BNA_G	<u>BG060937.D</u>
Compound Name	Response	Retention Time
DDT	591931	20.792
DDD	12904	20.352
DDE	1688	19.846
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14592	606523	2.41

Instrument :
BNA_G
ClientSampleId :
DFTPP